

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
 Data File : BM032343.D
 Acq On : 06 Oct 2021 15:18
 Operator : CG/JU
 Sample : PB139634BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK634

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.960	16	21	33	rVB	65822	99801	1.75%	0.163%
2	3.384	89	93	115	rBV	795831	1253093	22.02%	2.050%
3	3.743	149	154	163	rVB	17139	28034	0.49%	0.046%
4	6.807	668	675	688	rBV	933206	1451671	25.51%	2.375%
5	6.942	691	698	711	rVV	752481	1171460	20.58%	1.917%
6	7.154	728	734	746	rBV	938204	1494254	26.26%	2.445%
7	7.619	806	813	826	rBV	936841	1445538	25.40%	2.365%
8	8.342	929	936	954	rBV	1187223	1843218	32.39%	3.016%
9	8.772	1002	1009	1024	rBV	880146	1376131	24.18%	2.251%
10	9.495	1125	1132	1145	rBV	688924	1098943	19.31%	1.798%
11	10.036	1218	1224	1239	rBV	1094836	1815342	31.90%	2.970%
12	10.142	1239	1242	1249	rVB8	5099	11720	0.21%	0.019%
13	10.407	1279	1287	1303	rBV	1300318	2163436	38.01%	3.539%
14	10.542	1303	1310	1325	rVV	1220222	1927071	33.86%	3.153%
15	12.001	1552	1558	1565	rBV	18382	32158	0.57%	0.053%
16	13.671	1835	1842	1848	rBV	2171909	2900889	50.97%	4.746%
17	13.960	1884	1891	1901	rBV	2336893	3313353	58.22%	5.421%
18	14.265	1936	1943	1955	rBV	2050859	2969204	52.17%	4.858%
19	14.471	1972	1978	2001	rBV	994579	1377701	24.21%	2.254%
20	15.260	2105	2112	2125	rBV	3102790	4376656	76.90%	7.160%
21	15.371	2125	2131	2145	rVV	909908	1194022	20.98%	1.953%
22	15.495	2148	2152	2157	rVB2	37169	54170	0.95%	0.089%
23	16.036	2241	2244	2250	rBV7	4328	5755	0.10%	0.009%
24	16.783	2367	2371	2376	rBV2	8786	14692	0.26%	0.024%
25	16.995	2401	2407	2417	rBV	2613904	3563737	62.62%	5.830%
26	17.089	2417	2423	2441	rVV2	3430083	4875422	85.67%	7.976%
27	18.942	2734	2738	2743	rBV2	36341	53272	0.94%	0.087%
28	19.012	2746	2750	2755	rVV	36417	53666	0.94%	0.088%
29	19.377	2806	2812	2826	rBV	4415864	5691260	100.00%	9.311%
30	21.159	3110	3115	3125	rBV	3192393	3935699	69.15%	6.439%
31	23.171	3450	3457	3470	rVB2	3214088	5549669	97.51%	9.080%
32	23.306	3474	3480	3494	rVB2	2285567	3981998	69.97%	6.515%




Sum of corrected areas: 61123035

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
Data File : BM032343.D
Acq On : 06 Oct 2021 15:18
Operator : CG/JU
Sample : PB139634BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK634

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

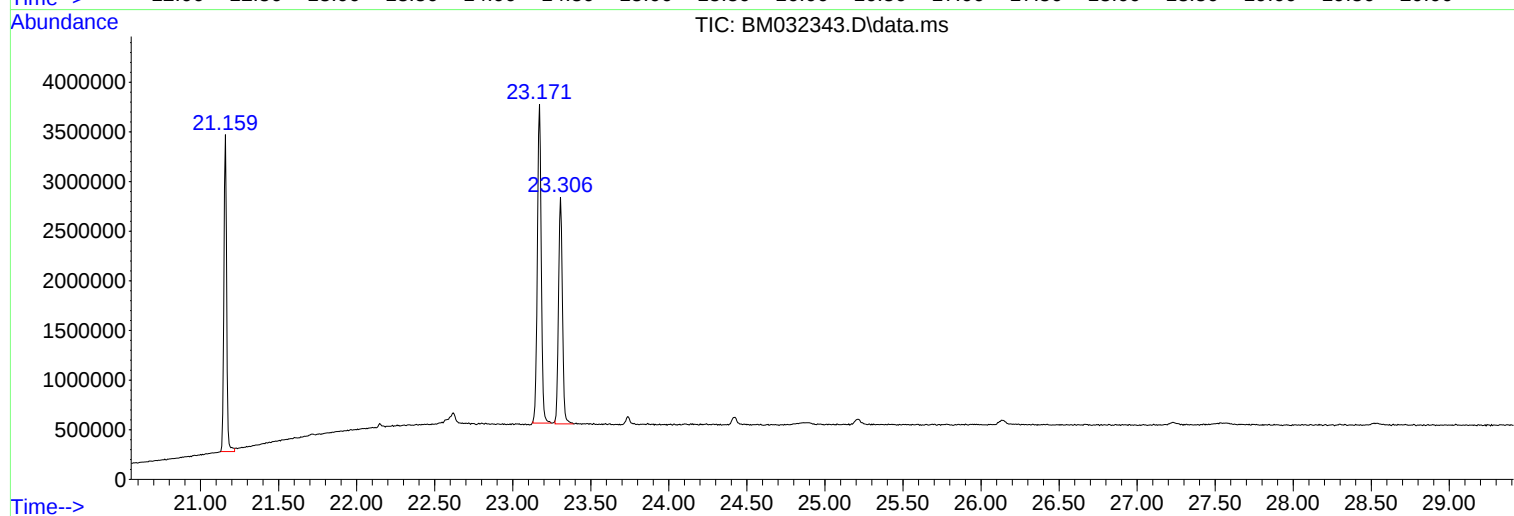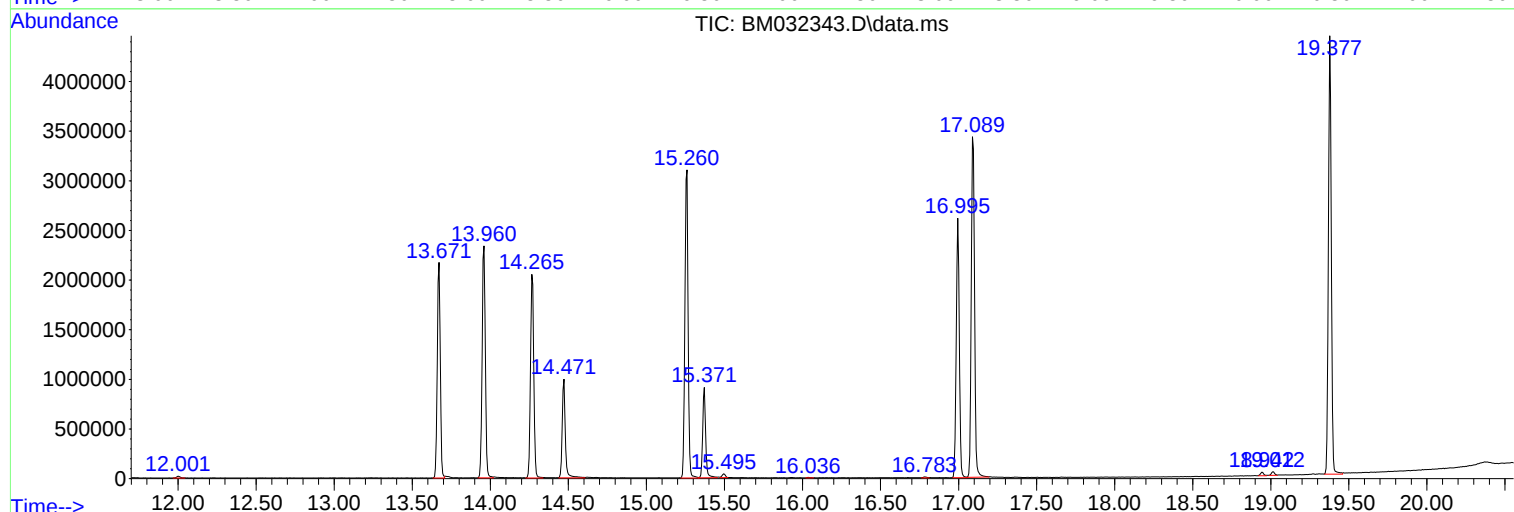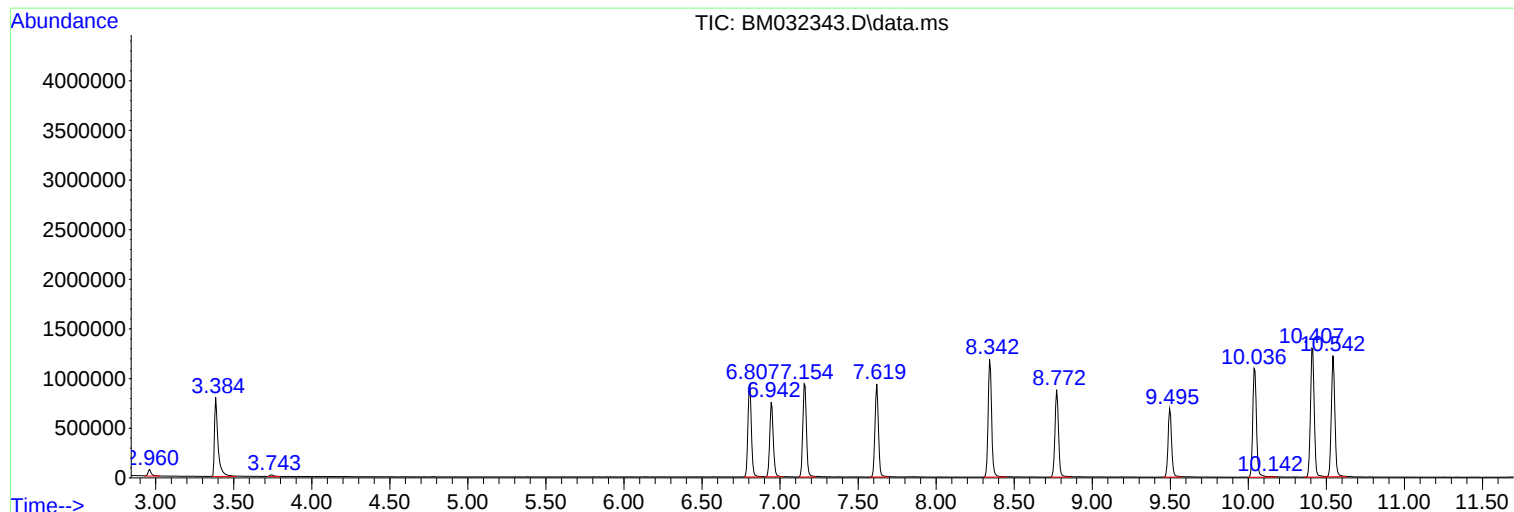

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
Data File : BM032343.D
Acq On : 06 Oct 2021 15:18
Operator : CG/JU
Sample : PB139634BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK634

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
Data File : BM032343.D
Acq On : 06 Oct 2021 15:18
Operator : CG/JU
Sample : PB139634BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK634

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
