

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036854.D
 Acq On : 07 Oct 2022 12:44
 Operator : CG/JU
 Sample : N4847-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8R4

Quant Time: Oct 08 02:21:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 06 17:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.968	152	5844	0.400	ng/ul	0.00
4) Naphthalene-d8	10.770	136	19863	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.594	164	10851	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	21689	0.400	ng/ul	0.00
17) Chrysene-d12	21.497	240	17651	0.400	ng/ul	0.00
23) Perylene-d12	23.902	264	17611	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	36850	4.471	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.360	152	10197	0.340	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	21715	0.411	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.390	88	980	0.122	ng/ul#	43
20) Pyrene	19.712	202	3855	0.053	ng/ul#	1
26) Benzo(a)pyrene	23.750	252	7319	0.115	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036854.D
Acq On : 07 Oct 2022 12:44
Operator : CG/JU
Sample : N4847-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8R4

Quant Time: Oct 08 02:21:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 17:02:30 2022
Response via : Initial Calibration




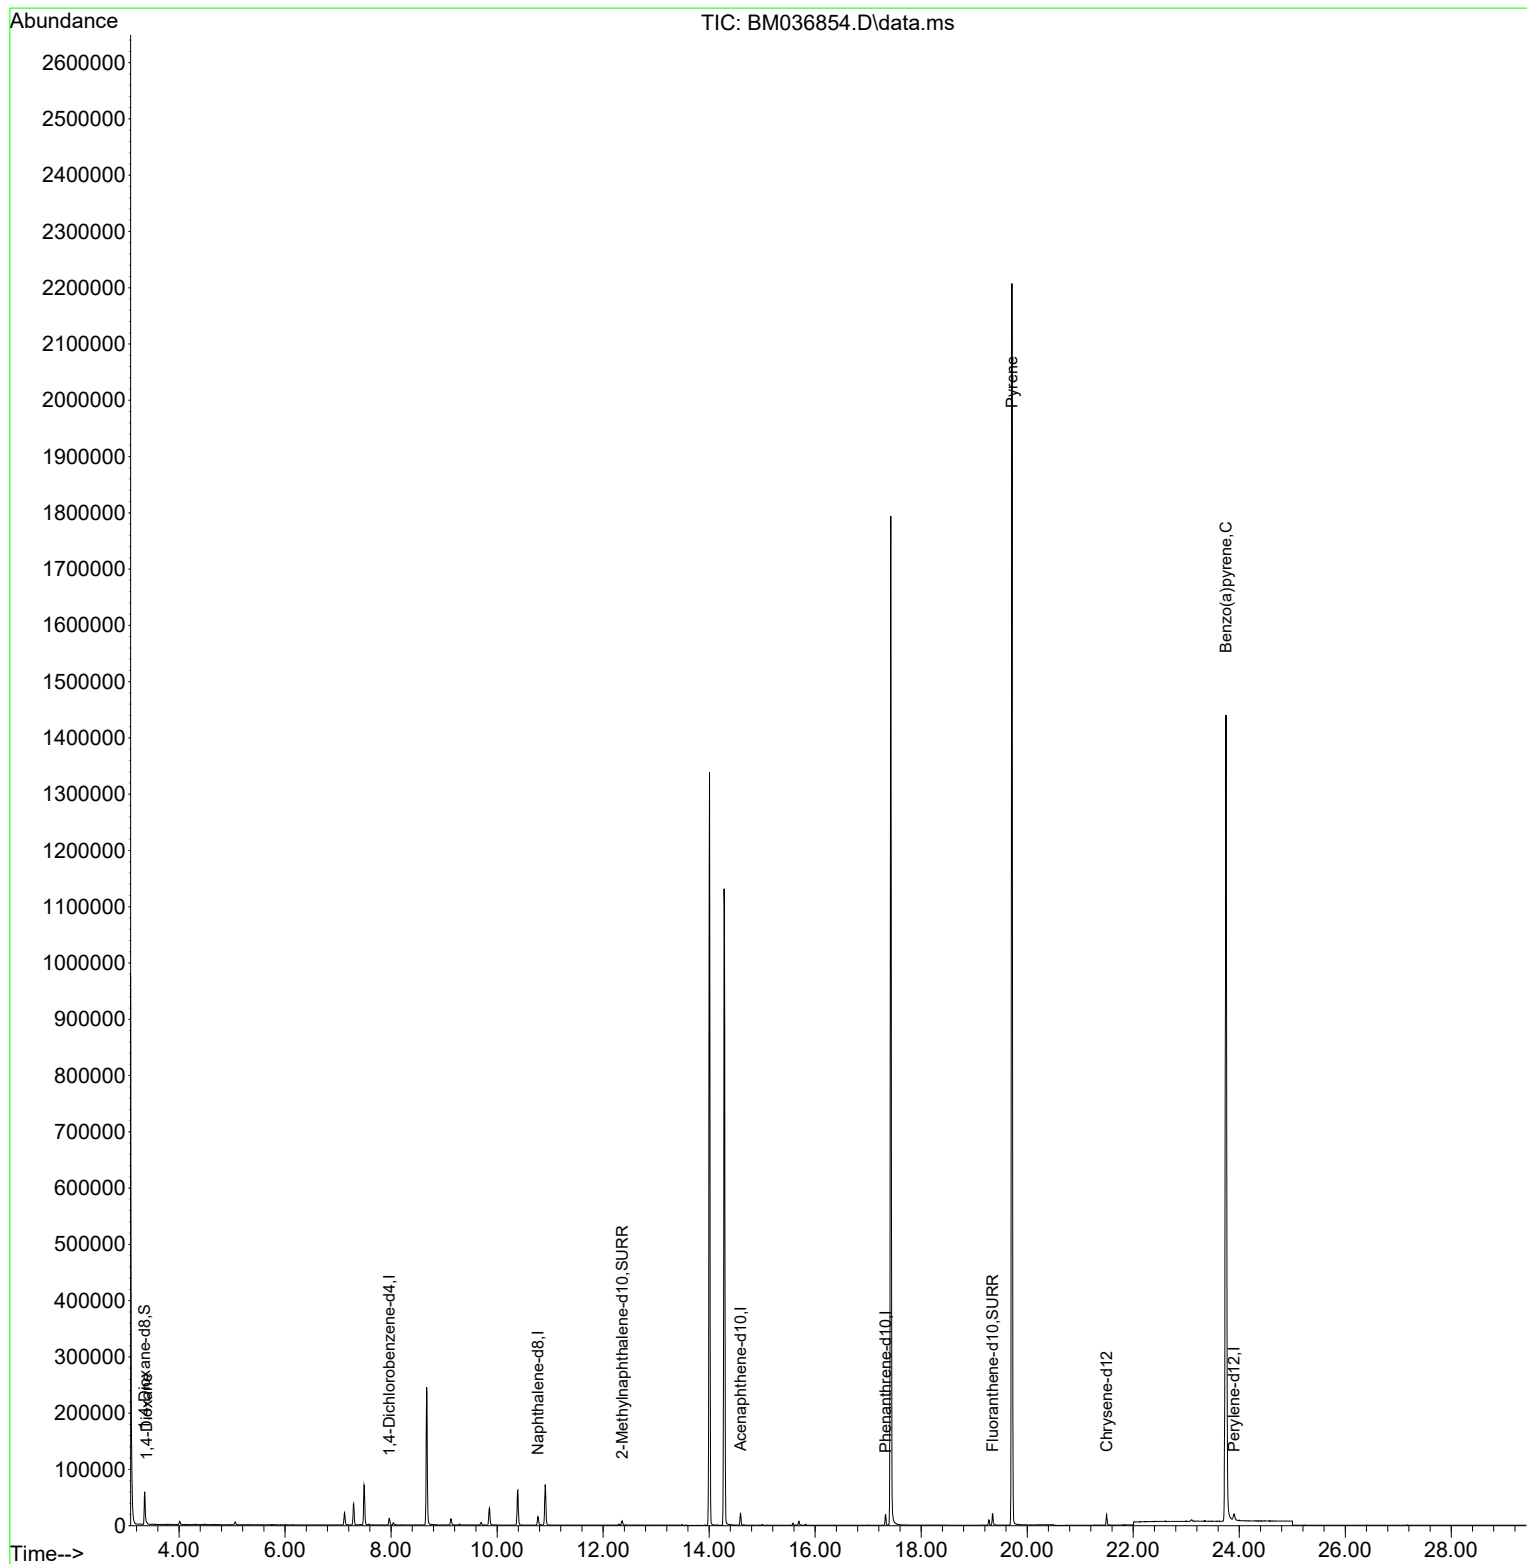


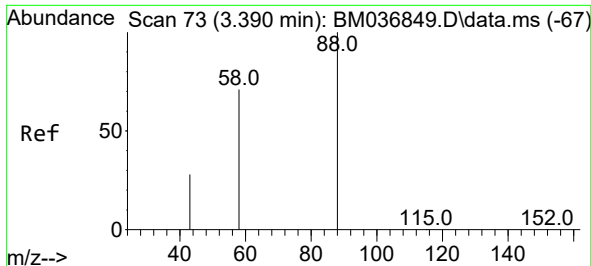

#2
1,4-Dioxane
Concen: 0.122 ng/ul
RT: 3.390 min Scan# 71
Delta R.T. 0.000 min
Lab File: BM036854.D
Acq: 07 Oct 2022 12:44




Instrument :
BNA_M
ClientSampleId :
CB8R4


Tgt Ion: 88 Resp: 980
Ion Ratio Lower Upper
88 100
43 111.4 37.8 56.6#
58 69.2 42.6 63.8#

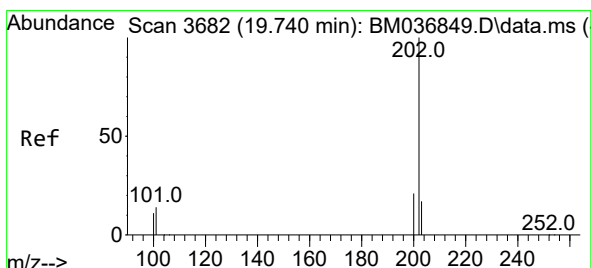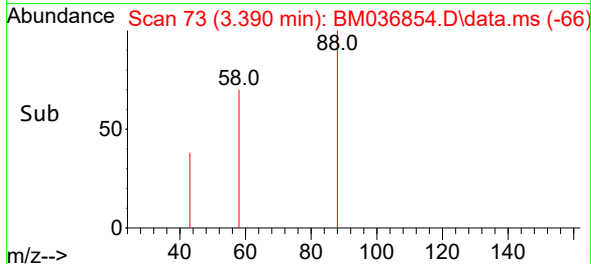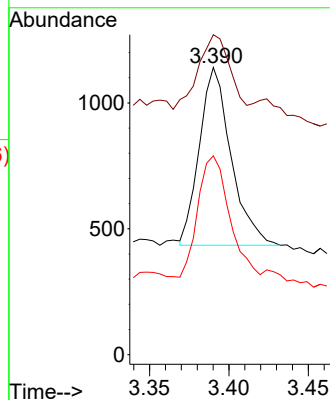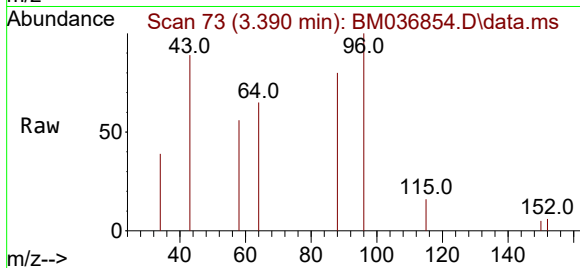

#20
Pyrene
Concen: 0.053 ng/ul
RT: 19.712 min Scan# 3676
Delta R.T. -0.029 min
Lab File: BM036854.D
Acq: 07 Oct 2022 12:44

Tgt Ion: 202 Resp: 3855
Ion Ratio Lower Upper
202 100
101 175.6 12.0 18.0#
100 1266.1 9.8 14.6#

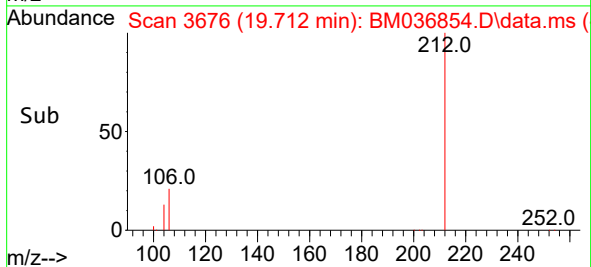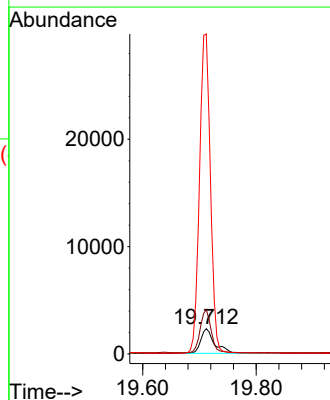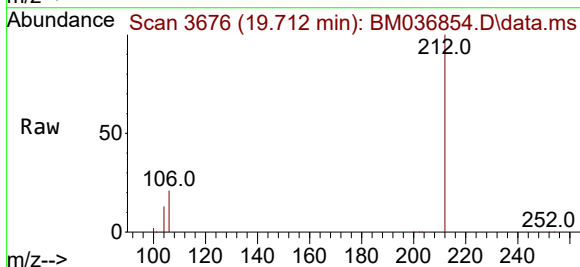

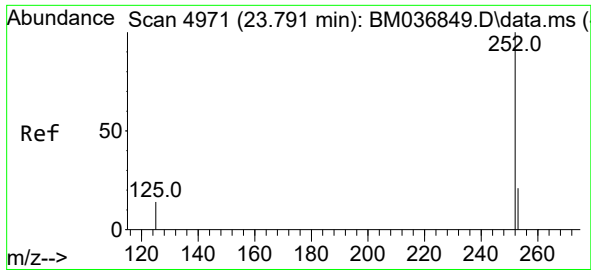

#26

Benzo(a)pyrene

Concen: 0.115 ng/ul

RT: 23.750 min Scan# 49

Delta R.T. -0.043 min

Lab File: BM036854.D


Acq: 07 Oct 2022 12:44

Instrument :

BNA_M

ClientSampleId :

CB8R4

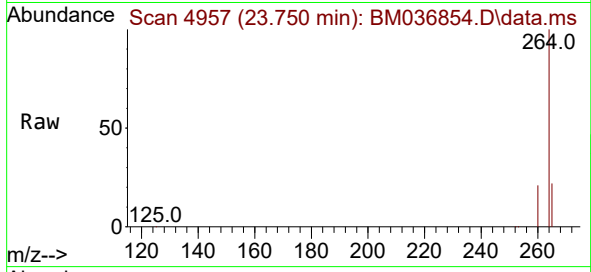

Tgt Ion:252 Resp: 7319

Ion Ratio Lower Upper

252 100

253 44.0 29.7 44.5

125 51.3 23.6 35.4#

