

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036864.D
 Acq On : 07 Oct 2022 18:52
 Operator : CG/JU
 Sample : N4847-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Q9

Quant Time: Oct 08 02:23:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 06 17:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.968	152	7561	0.400	ng/ul	0.00
4) Naphthalene-d8	10.770	136	27265	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.590	164	15212	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.327	188	31373	0.400	ng/ul	0.00
17) Chrysene-d12	21.496	240	26425	0.400	ng/ul	0.00
23) Perylene-d12	23.902	264	25829	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	44798	4.201	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.360	152	10877	0.264	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	25433	0.322	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.390	88	2749	0.264	ng/ul#	70
26) Benzo(a)pyrene	23.747	252	7605	0.081	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036864.D
Acq On : 07 Oct 2022 18:52
Operator : CG/JU
Sample : N4847-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Q9

Quant Time: Oct 08 02:23:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 17:02:30 2022
Response via : Initial Calibration




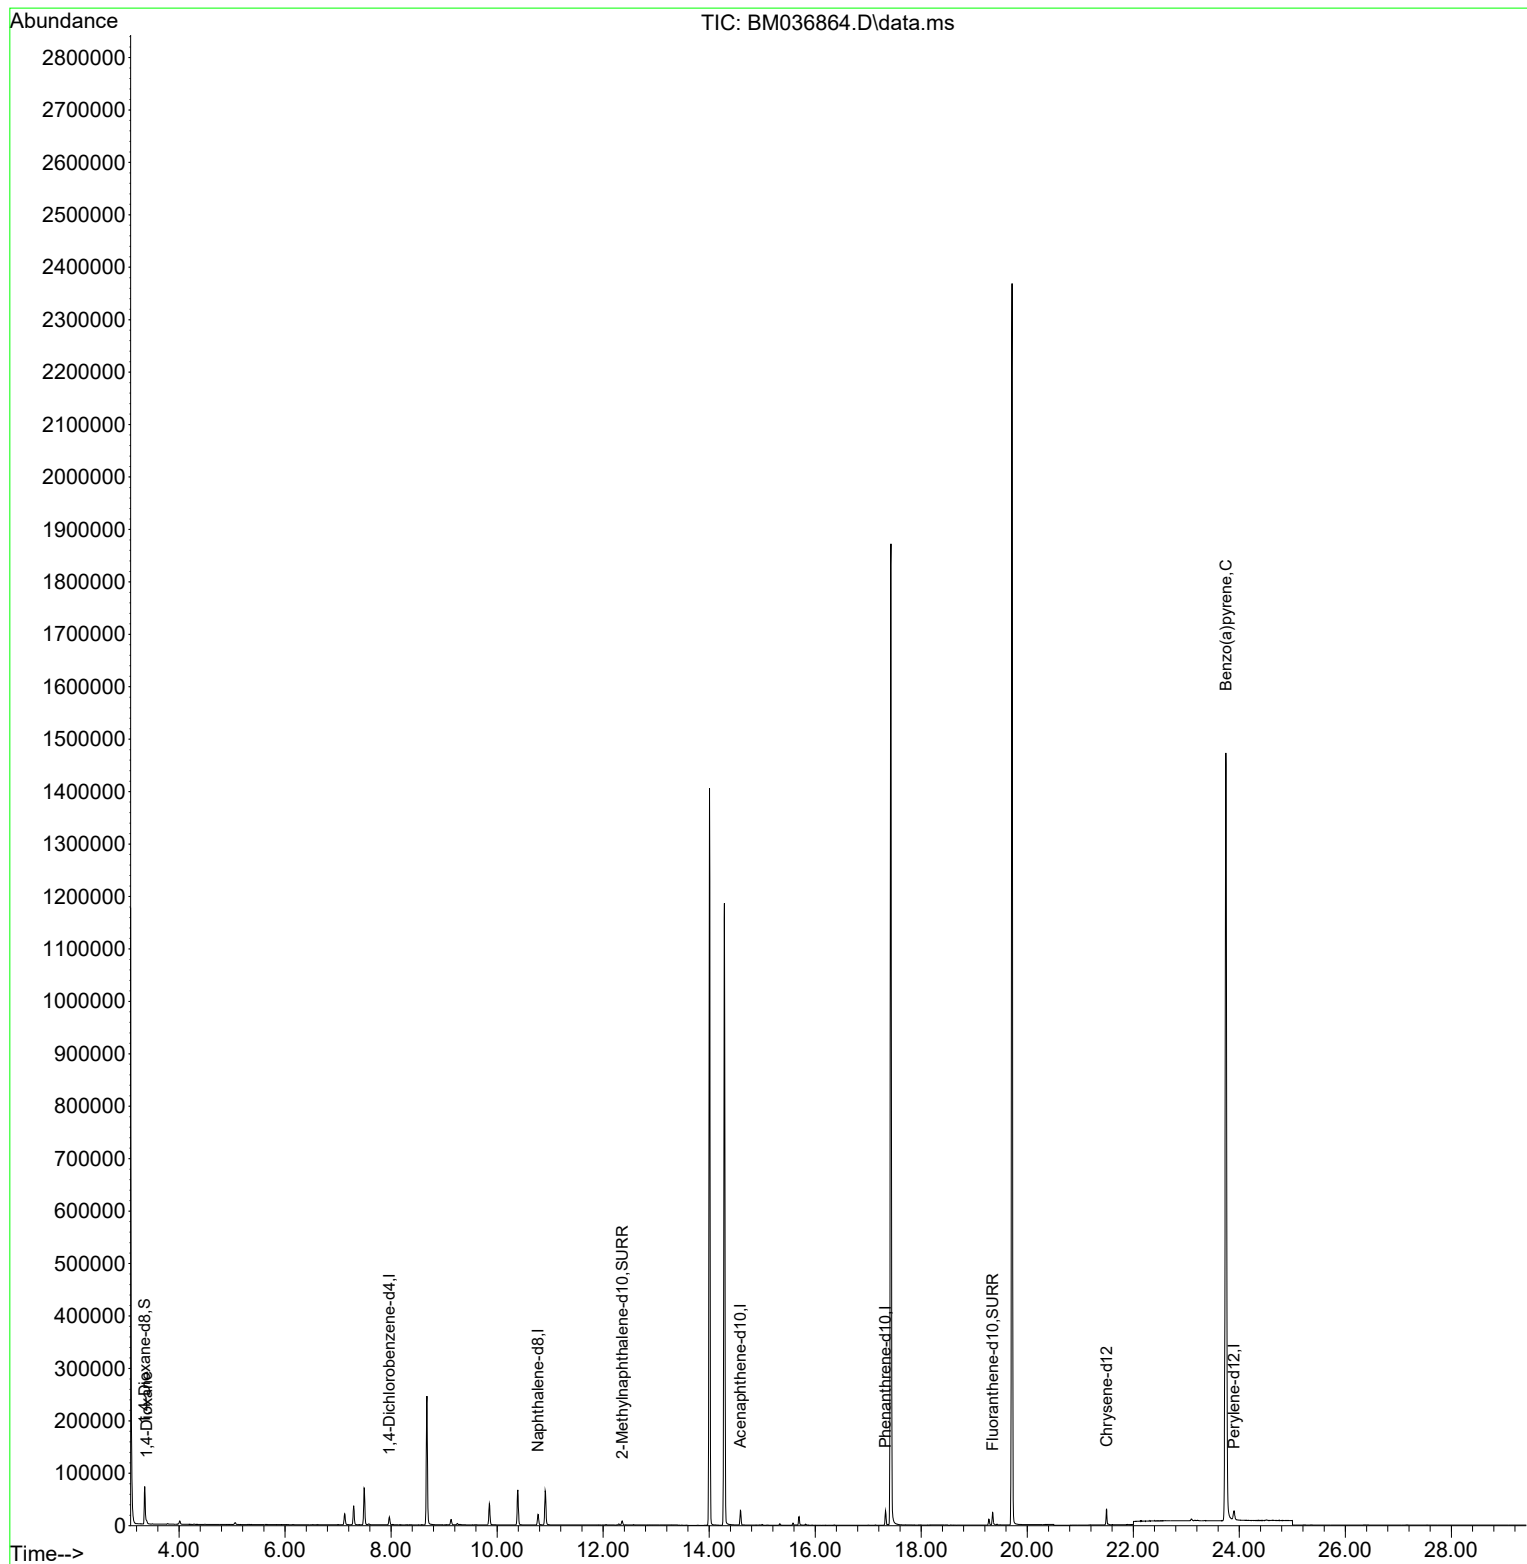


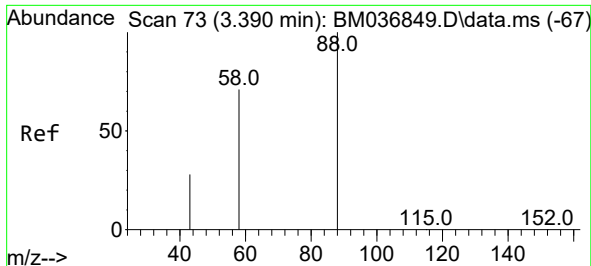

#2
1,4-Dioxane
Concen: 0.264 ng/ul
RT: 3.390 min Scan# 71
Delta R.T. 0.000 min
Lab File: BM036864.D
Acq: 07 Oct 2022 18:52

Instrument :
BNA_M
ClientSampleId :
CB8Q9

Tgt Ion: 88 Resp: 2749
Ion Ratio Lower Upper
88 100
43 70.7 37.8 56.6#
58 71.3 42.6 63.8#

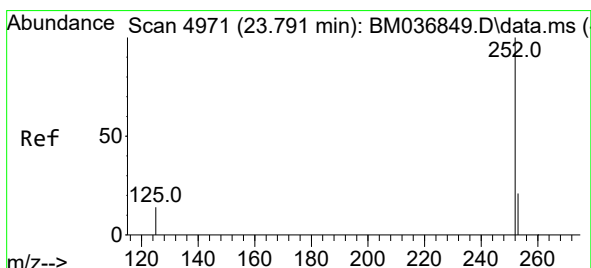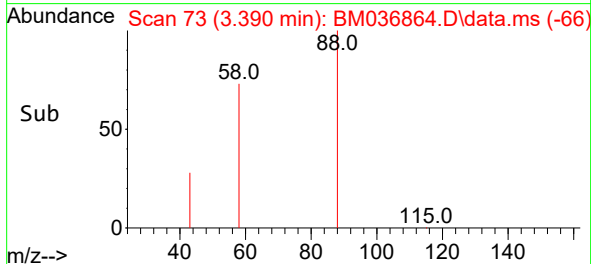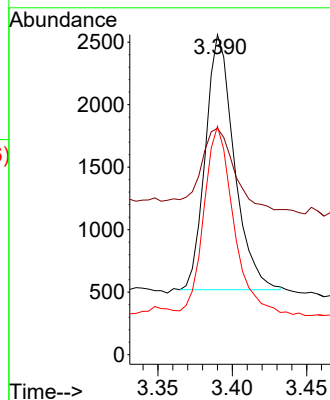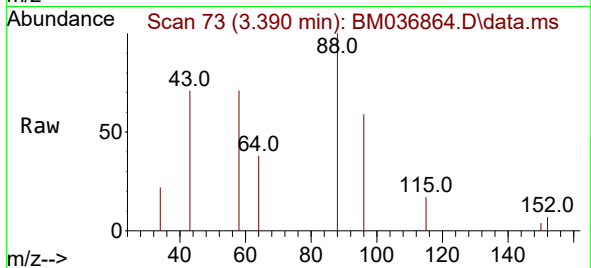

#26
Benzo(a)pyrene
Concen: 0.081 ng/ul
RT: 23.747 min Scan# 4956
Delta R.T. -0.047 min
Lab File: BM036864.D
Acq: 07 Oct 2022 18:52

Tgt Ion: 252 Resp: 7605
Ion Ratio Lower Upper
252 100
253 47.0 29.7 44.5#
125 54.4 23.6 35.4#

