

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036865.D
 Acq On : 07 Oct 2022 19:28
 Operator : CG/JU
 Sample : N4849-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Q9

Quant Time: Oct 08 02:23:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 06 17:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.968	152	6137	0.400	ng/ul	0.00
4) Naphthalene-d8	10.771	136	21845	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.590	164	12168	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.327	188	24835	0.400	ng/ul	0.00
17) Chrysene-d12	21.493	240	20921	0.400	ng/ul	0.00
23) Perylene-d12	23.899	264	20879	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	36833	4.256	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	10104	0.306	ng/ul	0.00
18) Fluoranthene-d10	19.346	212	23280	0.372	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.390	88	2356	0.278	ng/ul#	73
16) Anthracene	17.458	178	1439	0.022	ng/ul#	73
26) Benzo(a)pyrene	23.747	252	7232	0.096	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036865.D
Acq On : 07 Oct 2022 19:28
Operator : CG/JU
Sample : N4849-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Q9

Quant Time: Oct 08 02:23:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 17:02:30 2022
Response via : Initial Calibration




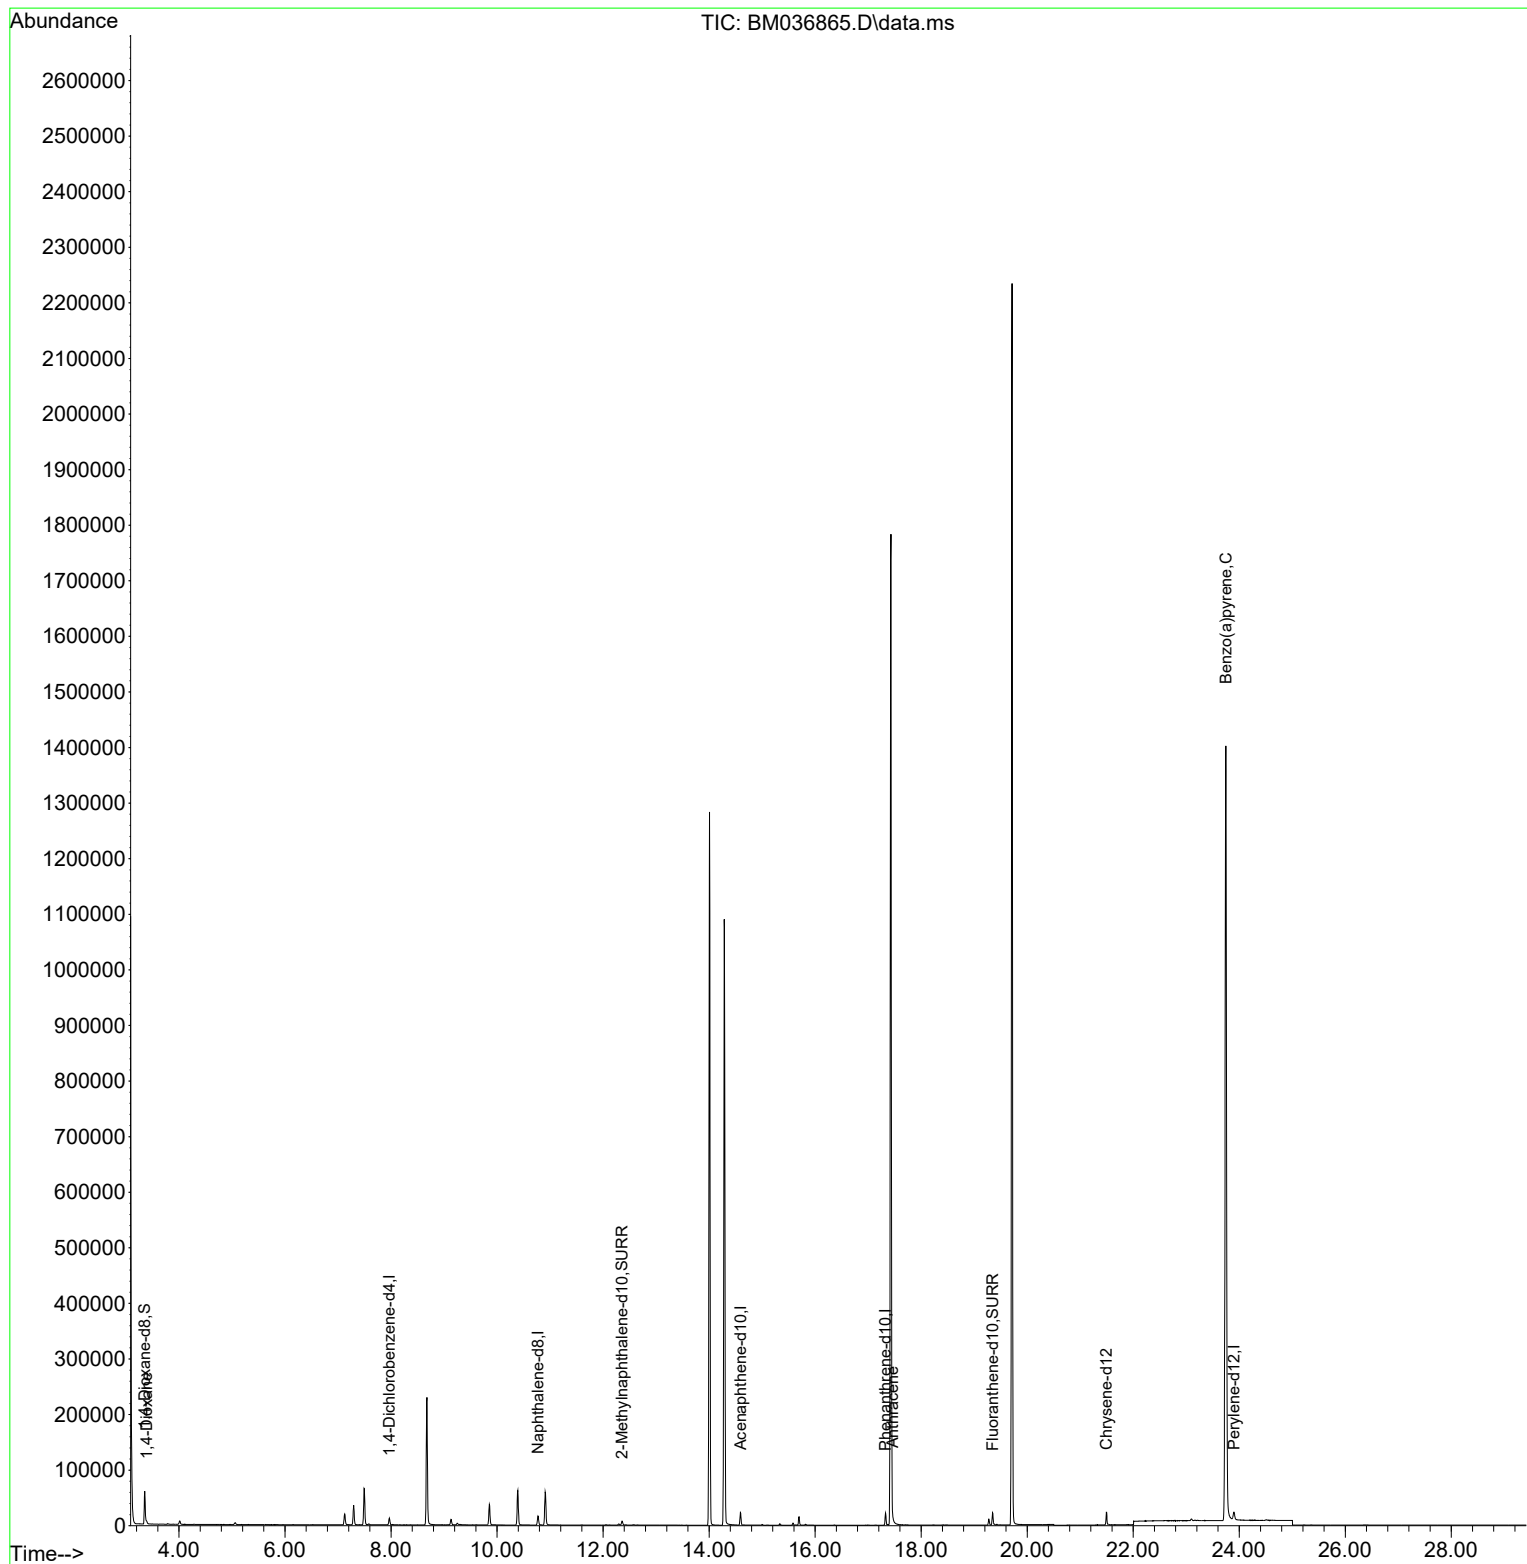


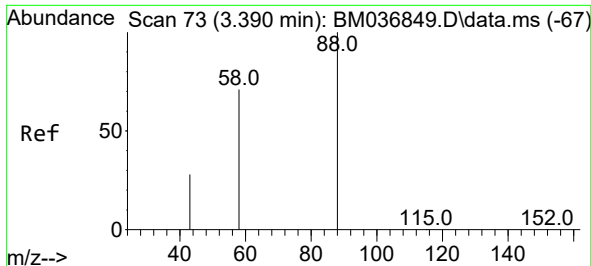

#2
 1,4-Dioxane
 Concen: 0.278 ng/ul
 RT: 3.390 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BM036865.D
 Acq: 07 Oct 2022 19:28




Instrument :
 BNA_M
 ClientSampleId :
 CB8Q9


Tgt Ion: 88 Resp: 2356
 Ion Ratio Lower Upper
 88 100
 43 70.2 37.8 56.6#
 58 68.3 42.6 63.8#

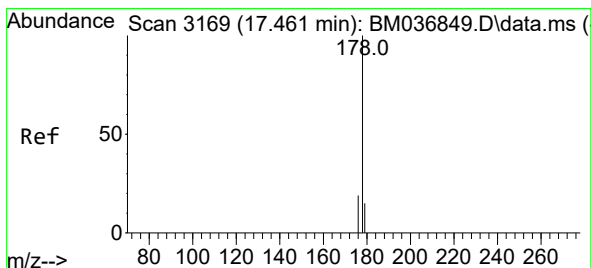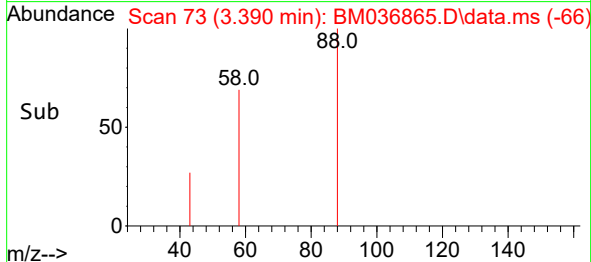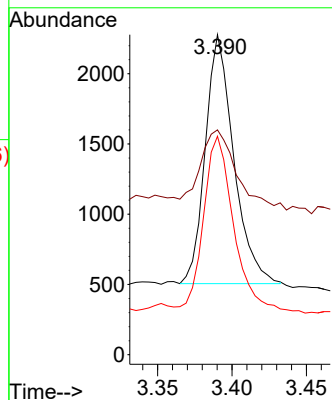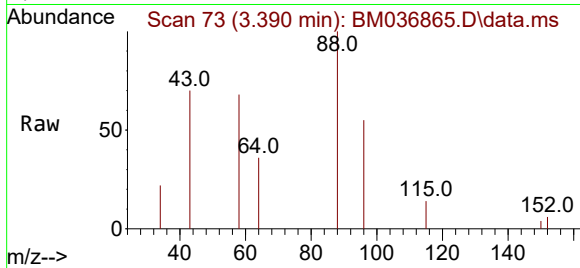

#16
 Anthracene
 Concen: 0.022 ng/ul
 RT: 17.458 min Scan# 3168
 Delta R.T. -0.004 min
 Lab File: BM036865.D
 Acq: 07 Oct 2022 19:28


Tgt Ion: 178 Resp: 1439
 Ion Ratio Lower Upper
 178 100
 179 32.3 13.6 20.4#
 176 28.4 15.6 23.4#

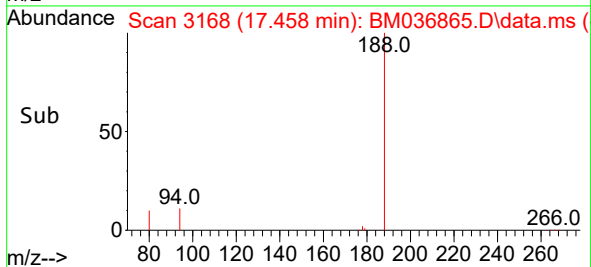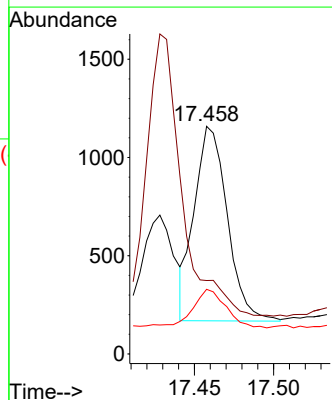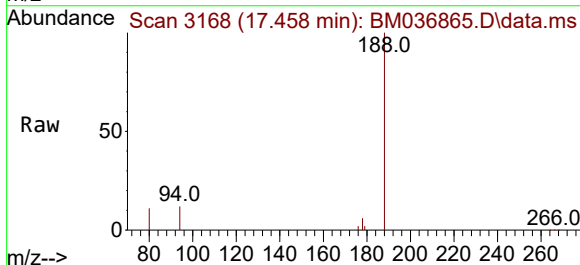

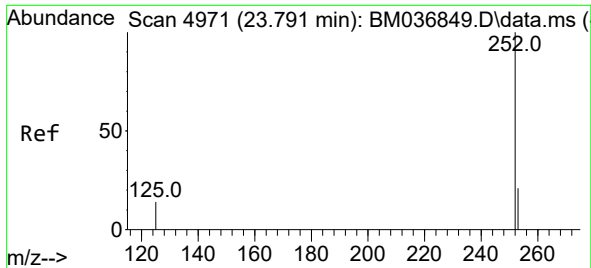

#26
 Benzo(a)pyrene
 Concen: 0.096 ng/ul
 RT: 23.747 min Scan# 49
 Delta R.T. -0.047 min
 Lab File: BM036865.D
 Acq: 07 Oct 2022 19:28

Instrument :
 BNA_M
 ClientSampleId :
 CB8Q9

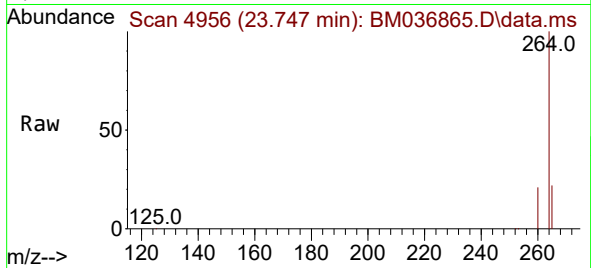

Tgt Ion:252 Resp: 7232
 Ion Ratio Lower Upper
 252 100
 253 47.5 29.7 44.5#
 125 56.6 23.6 35.4#

