

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036868.D
 Acq On : 07 Oct 2022 21:54
 Operator : CG/JU
 Sample : PB148013BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK013

Quant Time: Oct 08 02:23:31 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 06 17:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.968	152	7704	0.400	ng/ul	0.00
4) Naphthalene-d8	10.770	136	27020	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.589	164	14744	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	29685	0.400	ng/ul	0.00
17) Chrysene-d12	21.497	240	23552	0.400	ng/ul	0.00
23) Perylene-d12	23.900	264	21914	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	53228	4.899	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.360	152	11866	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	22063	0.313	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.579	166	3625	0.060	ng/ul#	14
20) Pyrene	19.712	202	3193	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.745	252	6656	0.084	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036868.D
Acq On : 07 Oct 2022 21:54
Operator : CG/JU
Sample : PB148013BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK013

Quant Time: Oct 08 02:23:31 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 17:02:30 2022
Response via : Initial Calibration




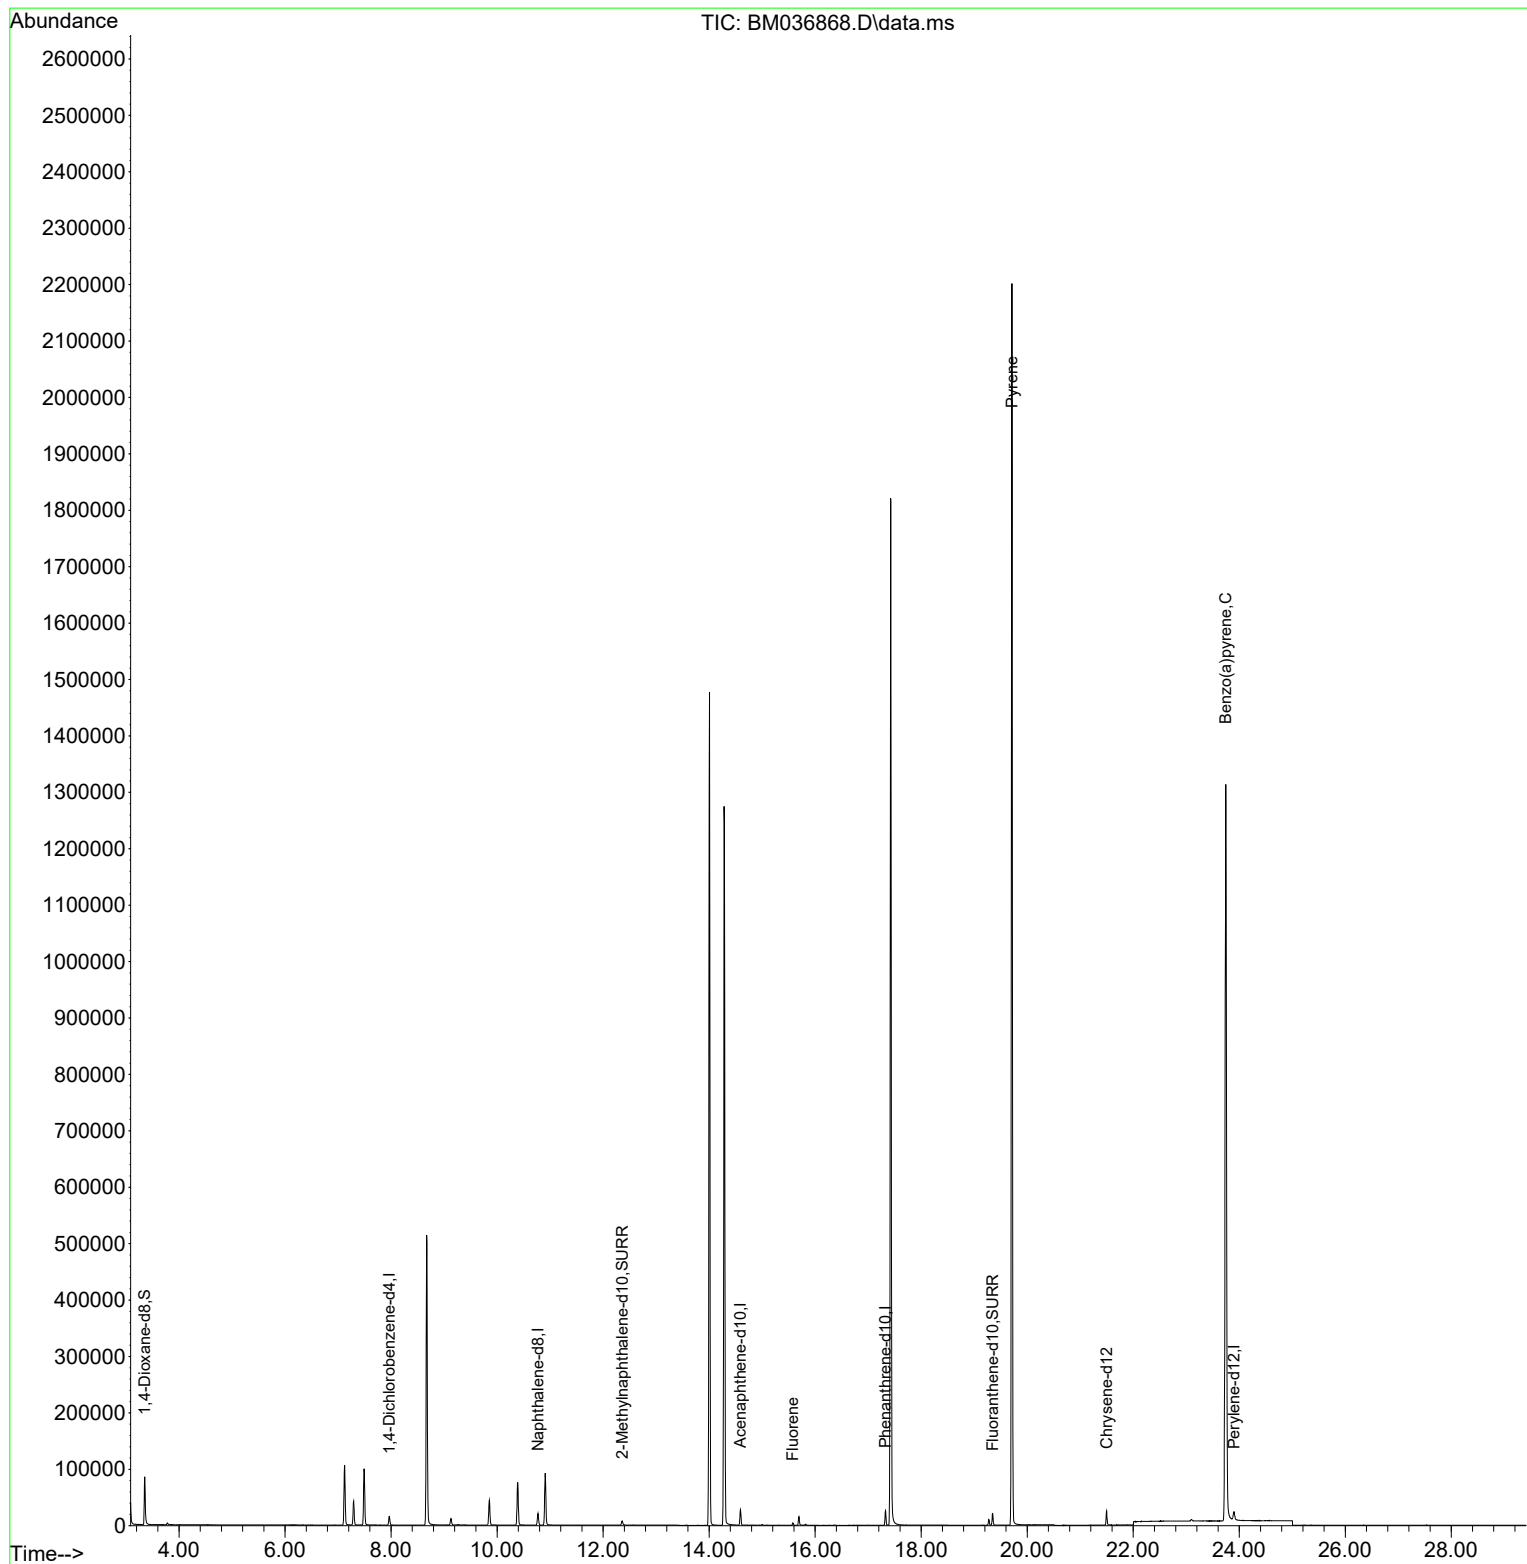


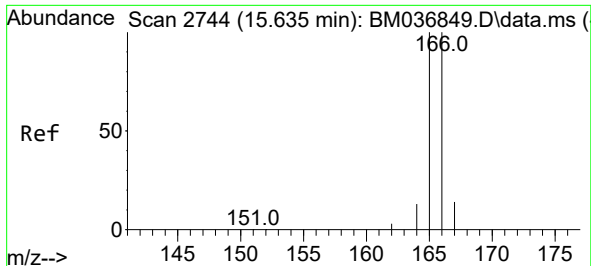

#12
Fluorene
Concen: 0.060 ng/ul
RT: 15.579 min Scan# 21
Delta R.T. -0.056 min
Lab File: BM036868.D
Acq: 07 Oct 2022 21:54




Instrument :
BNA_M
ClientSampleId :
SBLK013


Tgt Ion:166 Resp: 3625
Ion Ratio Lower Upper
166 100
165 6.9 78.9 118.3#
167 31.4 11.3 16.9#

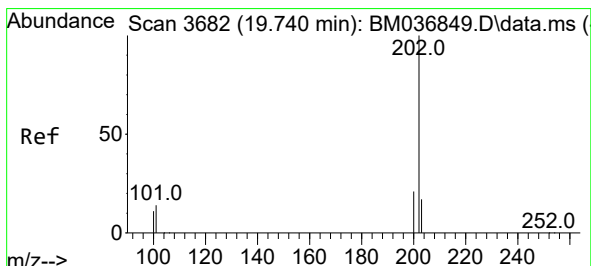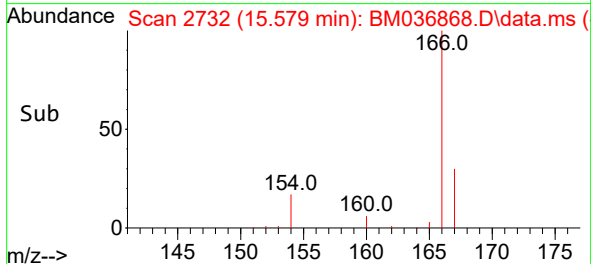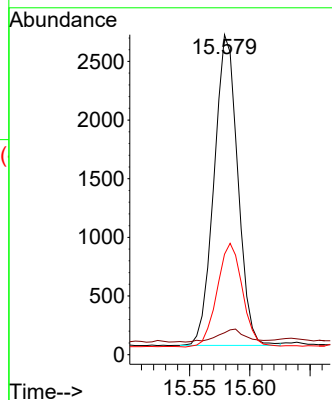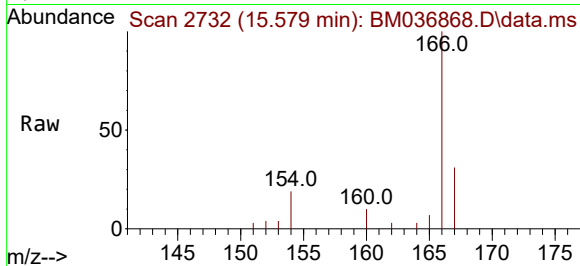

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.712 min Scan# 3676
Delta R.T. -0.029 min
Lab File: BM036868.D
Acq: 07 Oct 2022 21:54


Tgt Ion:202 Resp: 3193
Ion Ratio Lower Upper
202 100
101 169.6 12.0 18.0#
100 1254.4 9.8 14.6#

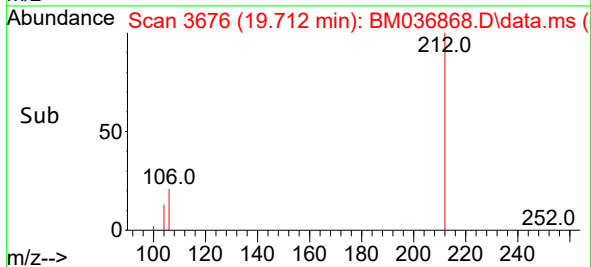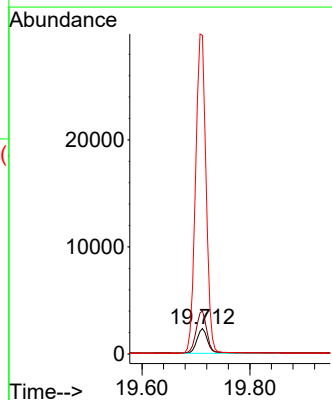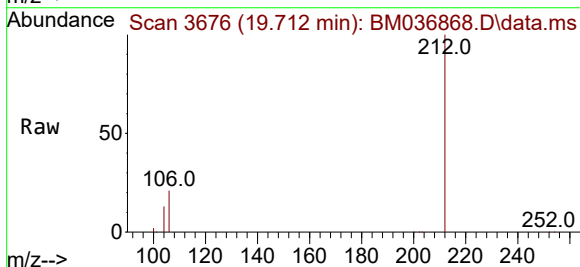

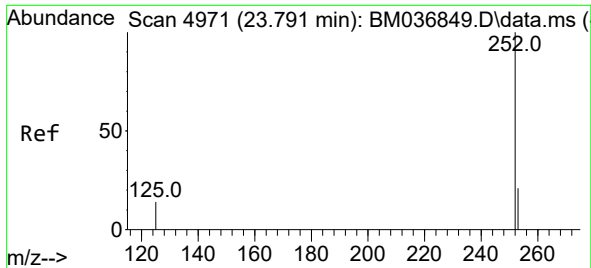

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.745 min Scan# 4971
Delta R.T. -0.049 min
Lab File: BM036868.D
Acq: 07 Oct 2022 21:54

Instrument :
BNA_M
ClientSampleId :
SBLK013

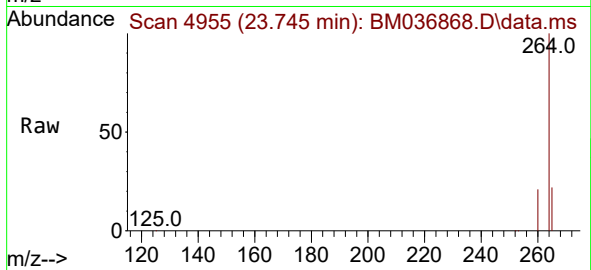

Tgt Ion:252 Resp: 6656
Ion Ratio Lower Upper
252 100
253 46.4 29.7 44.5#
125 54.5 23.6 35.4#

