

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036863.D
 Acq On : 07 Oct 2022 18:14
 Operator : CG/JU
 Sample : N4849-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Q5

Quant Time: Oct 08 02:22:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 06 17:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.968	152	8024	0.400	ng/ul	0.00
4) Naphthalene-d8	10.776	136	29500	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.594	164	17155	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	36565	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.497	240	30133	0.400	ng/ul	0.00
23) Perylene-d12	23.900	264	29048	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	42294	3.738	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	15535	0.349	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	39068	0.433	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.390	88	2131	0.193	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036863.D
Acq On : 07 Oct 2022 18:14
Operator : CG/JU
Sample : N4849-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Q5

Quant Time: Oct 08 02:22:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 17:02:30 2022
Response via : Initial Calibration

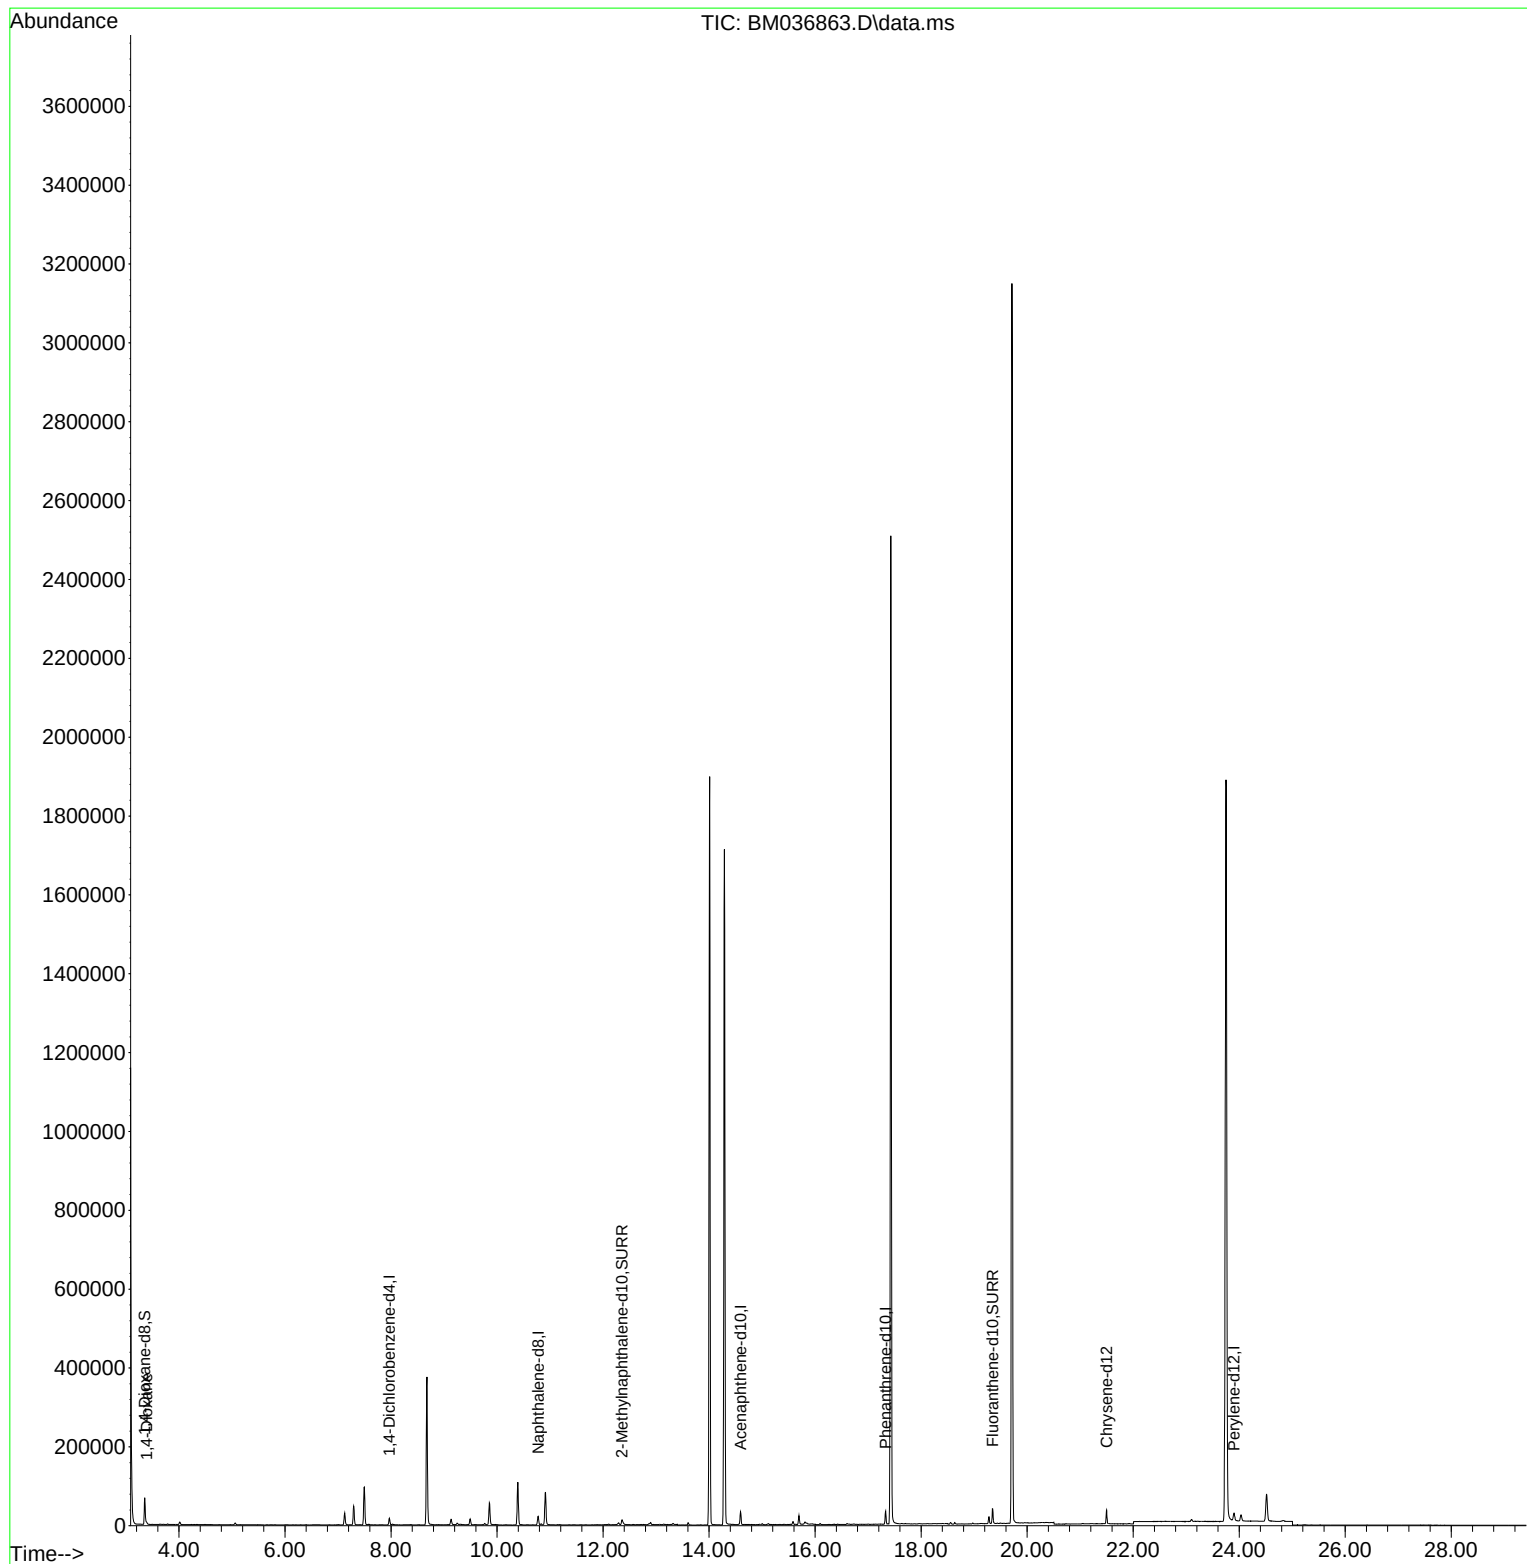

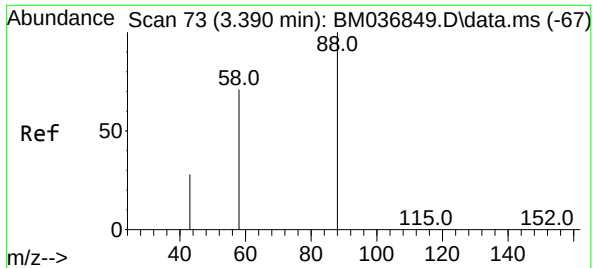

#2
 1,4-Dioxane
 Concen: 0.193 ng/ul
 RT: 3.390 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BM036863.D
 Acq: 07 Oct 2022 18:14

Instrument :
 BNA_M
 ClientSampleId :
 CB8Q5

Tgt Ion:	88	Resp:	2131
Ion	Ratio	Lower	Upper
88	100		
43	95.7	37.8	56.6#
58	70.1	42.6	63.8#

