

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036873.D
 Acq On : 08 Oct 2022 00:54
 Operator : CG/JU
 Sample : N4847-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8R1

Quant Time: Oct 08 02:24:16 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 06 17:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.964	152	5929	0.400	ng/ul	0.00
4) Naphthalene-d8	10.770	136	20662	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.589	164	11133	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	23131	0.400	ng/ul	0.00
17) Chrysene-d12	21.491	240	19576	0.400	ng/ul	0.00
23) Perylene-d12	23.897	264	19478	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	32937	3.939	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	9764	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.345	212	23888	0.408	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.368	178	1629	0.022	ng/ul#	81
19) Fluoranthene	19.373	202	1575	0.020	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036873.D
Acq On : 08 Oct 2022 00:54
Operator : CG/JU
Sample : N4847-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8R1

Quant Time: Oct 08 02:24:16 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 17:02:30 2022
Response via : Initial Calibration

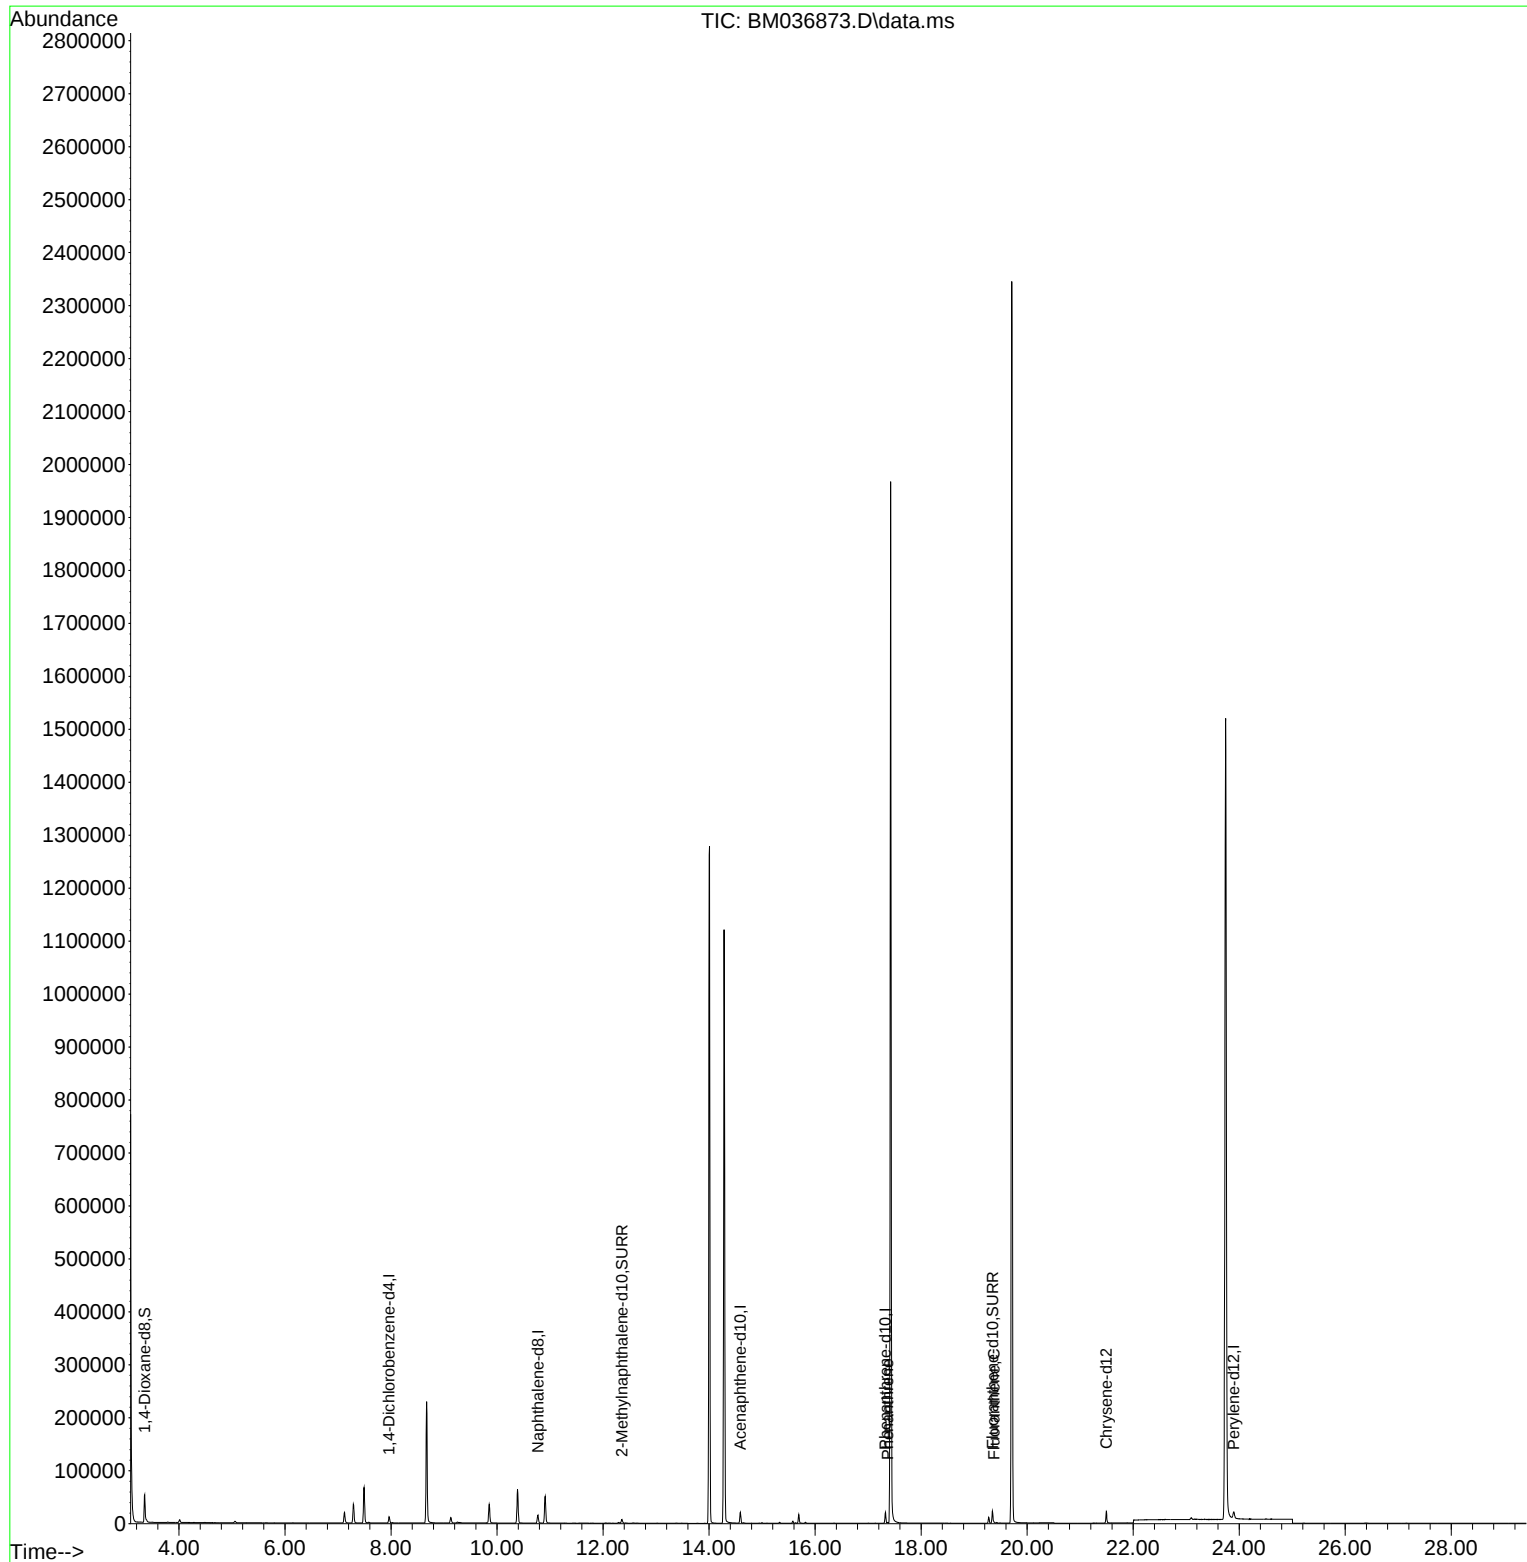

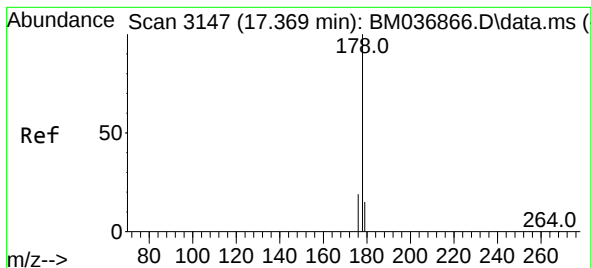

#15

Phenanthrene

Concen: 0.022 ng/ul

RT: 17.368 min Scan# 3147

Delta R.T. -0.001 min

Lab File: BM036873.D


Acq: 08 Oct 2022 00:54

Instrument :

BNA_M

ClientSampleId :

CB8R1

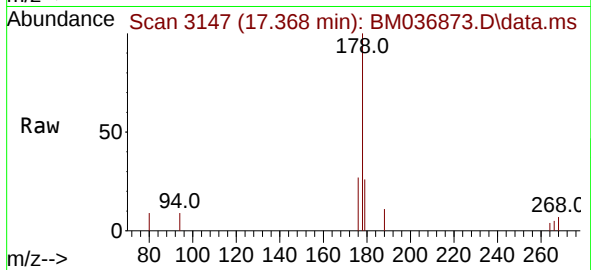




Tgt Ion:178 Resp: 1629

Ion Ratio Lower Upper

178 100

179 25.7 13.0 19.6#

176 27.0 15.6 23.4#

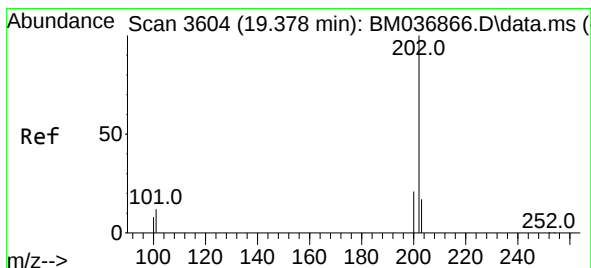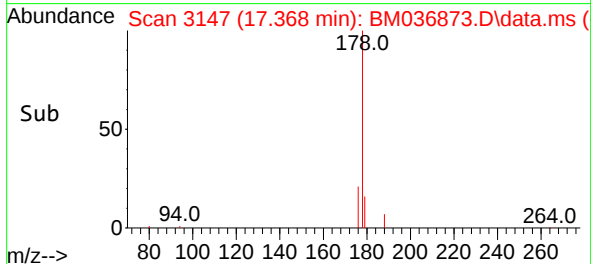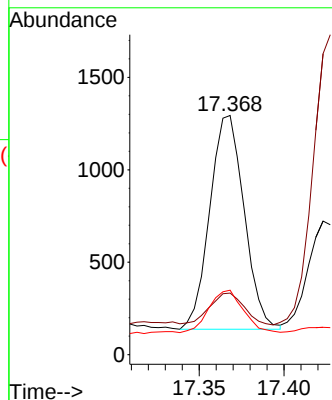

#19

Fluoranthene

Concen: 0.020 ng/ul

RT: 19.373 min Scan# 3603

Delta R.T. -0.006 min

Lab File: BM036873.D

Acq: 08 Oct 2022 00:54

Tgt Ion:202 Resp: 1575

Ion Ratio Lower Upper

202 100

101 21.7 10.1 15.1#

100 17.5 7.9 11.9#

