

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036893.D
 Acq On : 08 Oct 2022 13:19
 Operator : CG/JU
 Sample : N4873-14
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ59

Quant Time: Oct 10 01:25:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 10 00:54:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.959	152	6825	0.400	ng/ul	0.00
4) Naphthalene-d8	10.765	136	24554	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.584	164	16211	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.322	188	33395	0.400	ng/ul	0.00
17) Chrysene-d12	21.488	240	23176	0.400	ng/ul	0.00
23) Perylene-d12	23.888	264	18542	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	36323	3.774	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.349	152	13591	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.340	212	33468	0.483	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.386	88	13053	1.387	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036893.D
Acq On : 08 Oct 2022 13:19
Operator : CG/JU
Sample : N4873-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ59


Quant Time: Oct 10 01:25:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 00:54:15 2022
Response via : Initial Calibration

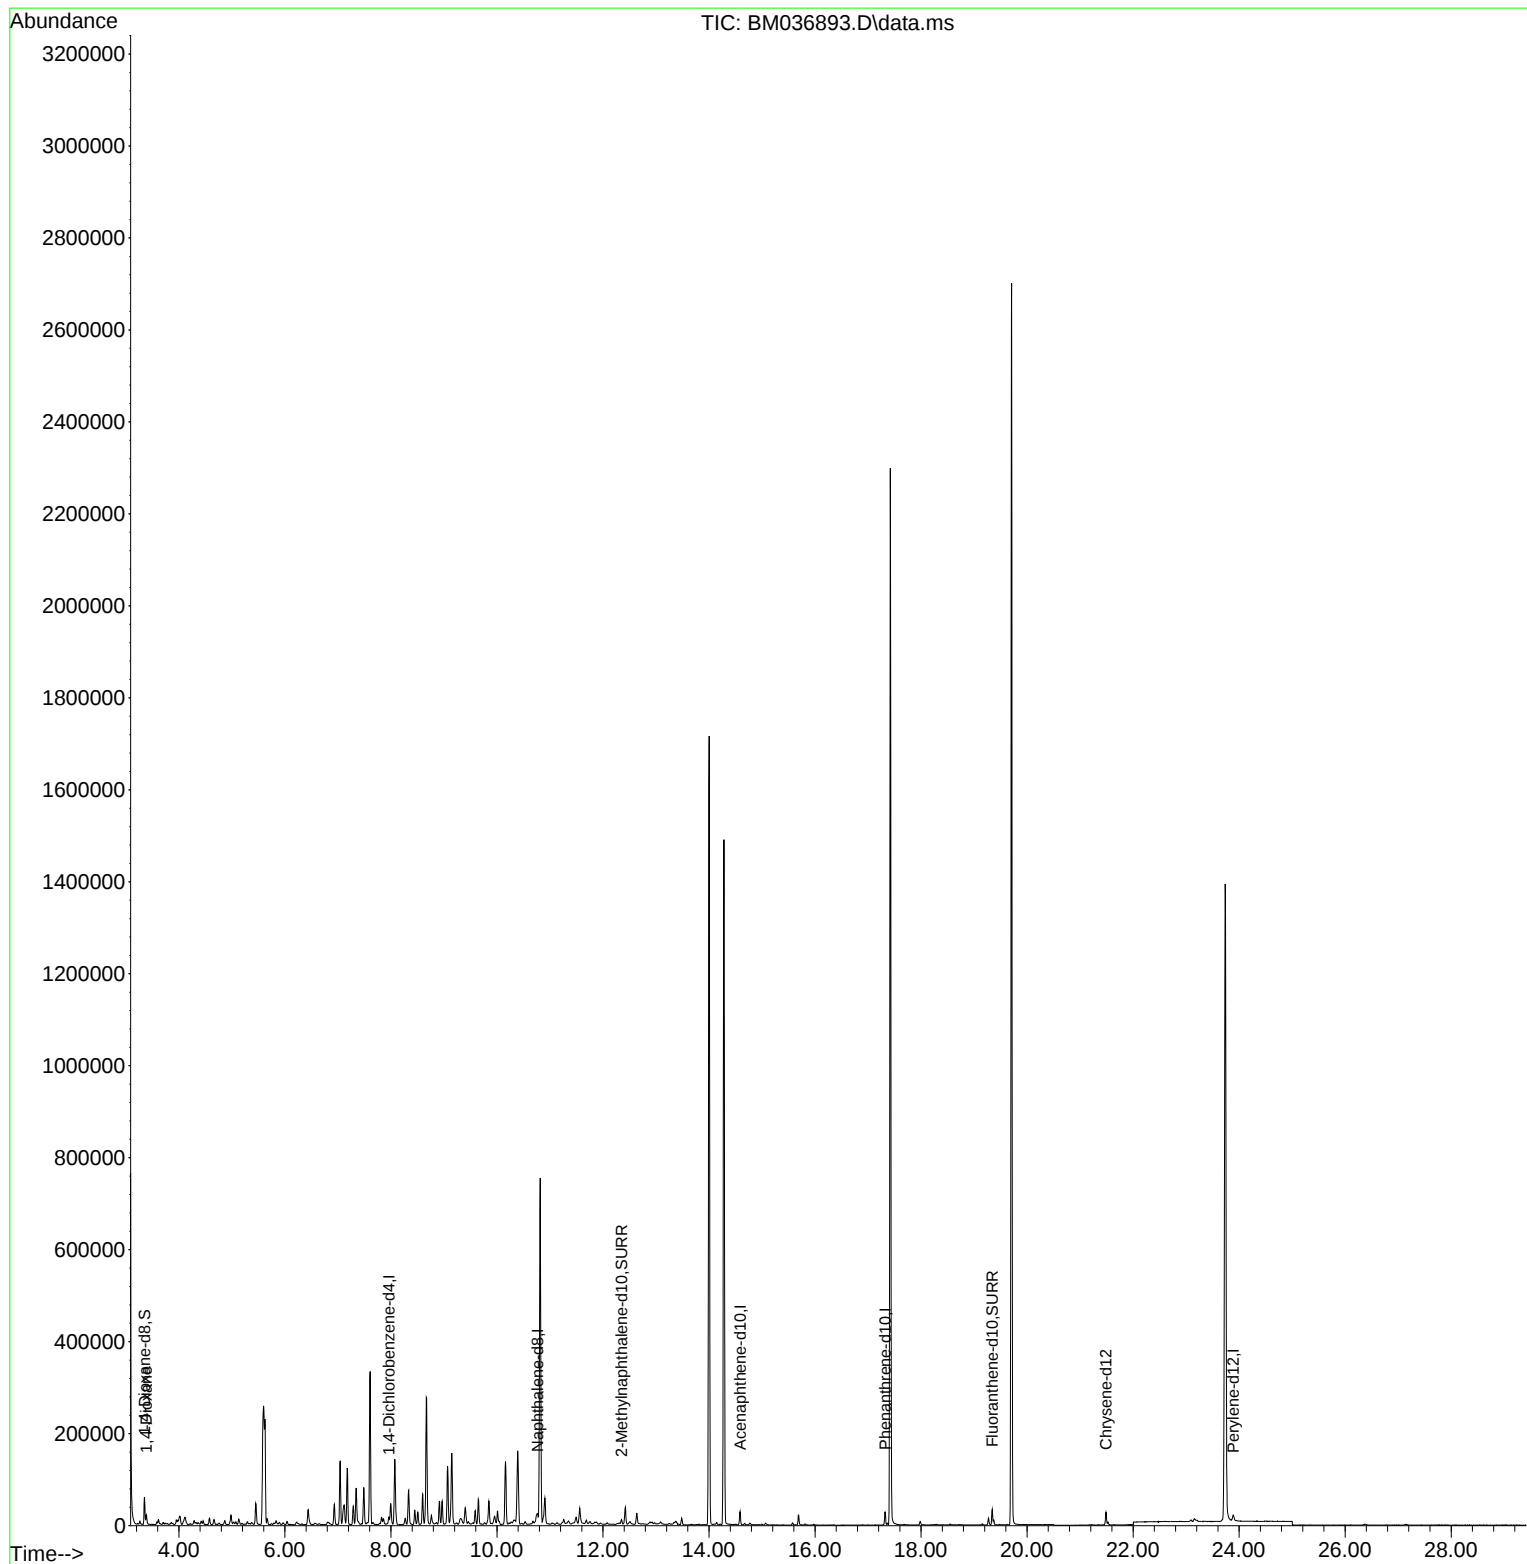

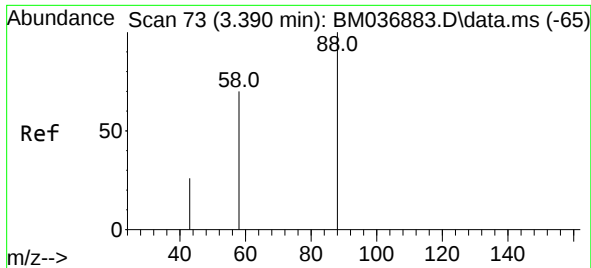

#2
 1,4-Dioxane
 Concen: 1.387 ng/ul
 RT: 3.386 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM036893.D
 Acq: 08 Oct 2022 13:19

Instrument :
 BNA_M
 ClientSampleId :
 EXZ59

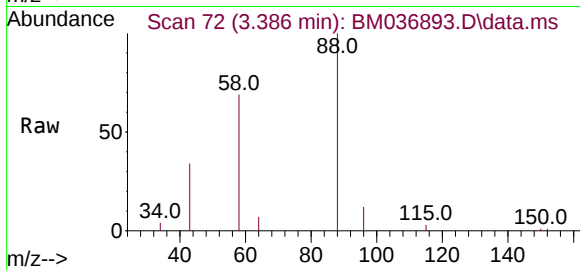

Tgt Ion: 88 Resp: 13053
 Ion Ratio Lower Upper
 88 100
 43 34.0 37.8 56.6#
 58 68.9 42.6 63.8#

