

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036895.D
 Acq On : 08 Oct 2022 14:31
 Operator : CG/JU
 Sample : N4873-16
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ61

Quant Time: Oct 10 01:26:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 10 00:54:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.959	152	6879	0.400	ng/ul	0.00
4) Naphthalene-d8	10.765	136	25712	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.585	164	18823	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.323	188	33184	0.400	ng/ul	0.00
17) Chrysene-d12	21.487	240	25189	0.400	ng/ul	0.00
23) Perylene-d12	23.890	264	21115	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	32442	3.344	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.349	152	13706	0.353	ng/ul	0.00
18) Fluoranthene-d10	19.341	212	32681	0.434	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.386	88	1751	0.185	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036895.D
Acq On : 08 Oct 2022 14:31
Operator : CG/JU
Sample : N4873-16
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ61


Quant Time: Oct 10 01:26:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 00:54:15 2022
Response via : Initial Calibration

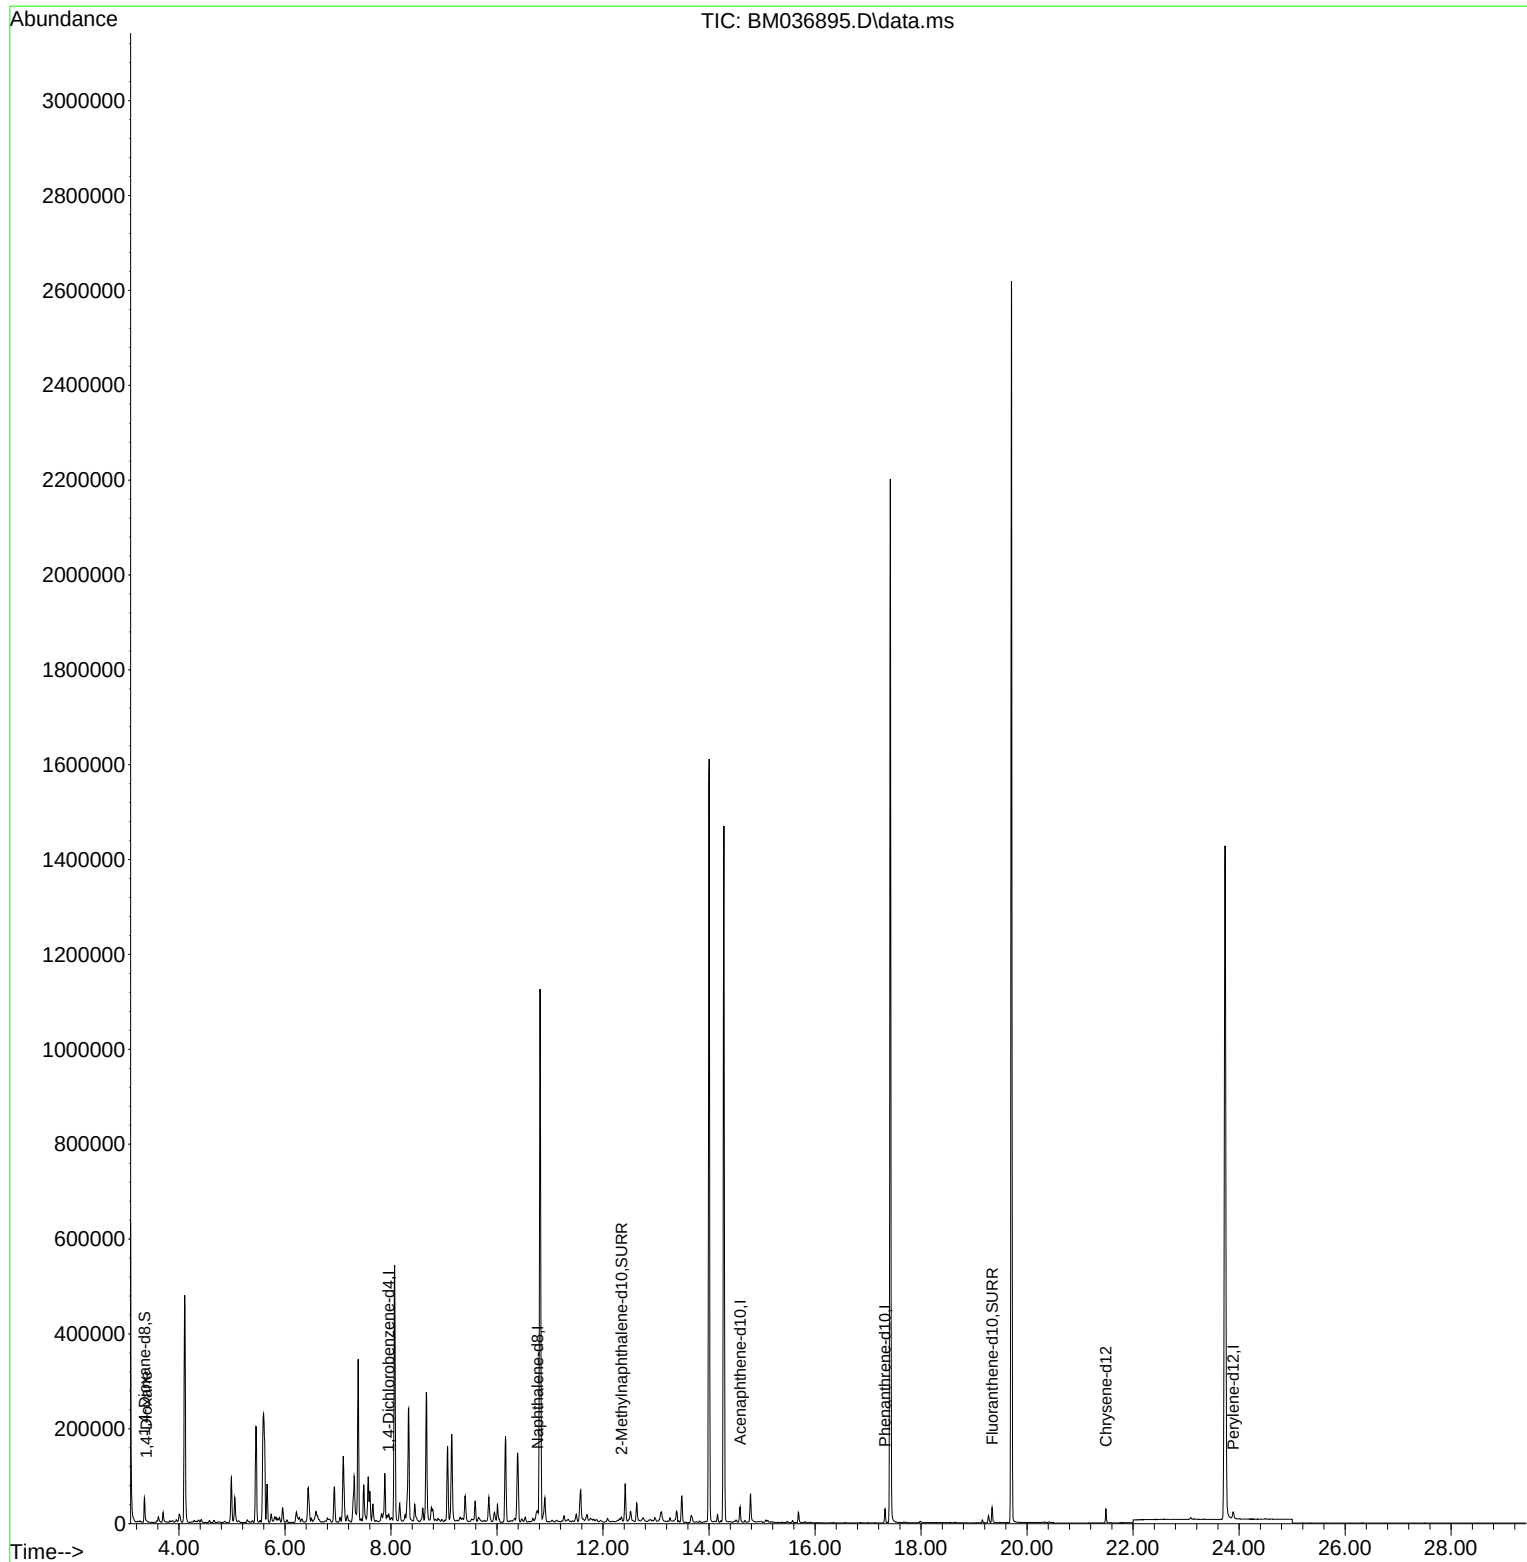

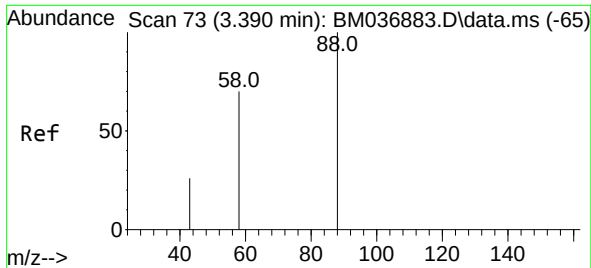

#2
 1,4-Dioxane
 Concen: 0.185 ng/ul
 RT: 3.386 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM036895.D
 Acq: 08 Oct 2022 14:31

Instrument :
 BNA_M
 ClientSampleId :
 EXZ61

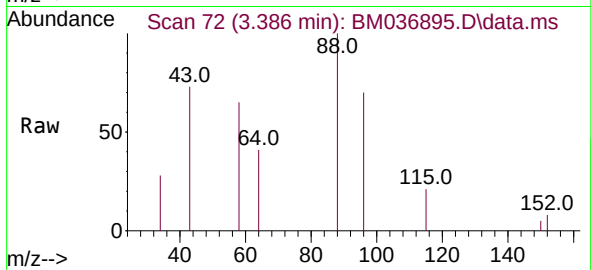

Tgt Ion: 88 Resp: 1751

Ion	Ratio	Lower	Upper
88	100		
43	73.1	37.8	56.6#
58	65.0	42.6	63.8#

