

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
 Data File : BM036897.D
 Acq On : 08 Oct 2022 15:42
 Operator : CG/JU
 Sample : N4873-18
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ63

Quant Time: Oct 10 01:26:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 10 00:54:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.959	152	7182	0.400	ng/u1	0.00
4) Naphthalene-d8	10.765	136	25495	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.585	164	14952	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.323	188	31888	0.400	ng/u1	0.00
17) Chrysene-d12	21.490	240	25402	0.400	ng/u1	0.00
23) Perylene-d12	23.890	264	20960	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	33606	3.318	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.349	152	12836	0.333	ng/u1	0.00
18) Fluoranthene-d10	19.341	212	32971	0.434	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.394	88	2136	0.216	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100722\
Data File : BM036897.D
Acq On : 08 Oct 2022 15:42
Operator : CG/JU
Sample : N4873-18
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ63


Quant Time: Oct 10 01:26:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 00:54:15 2022
Response via : Initial Calibration

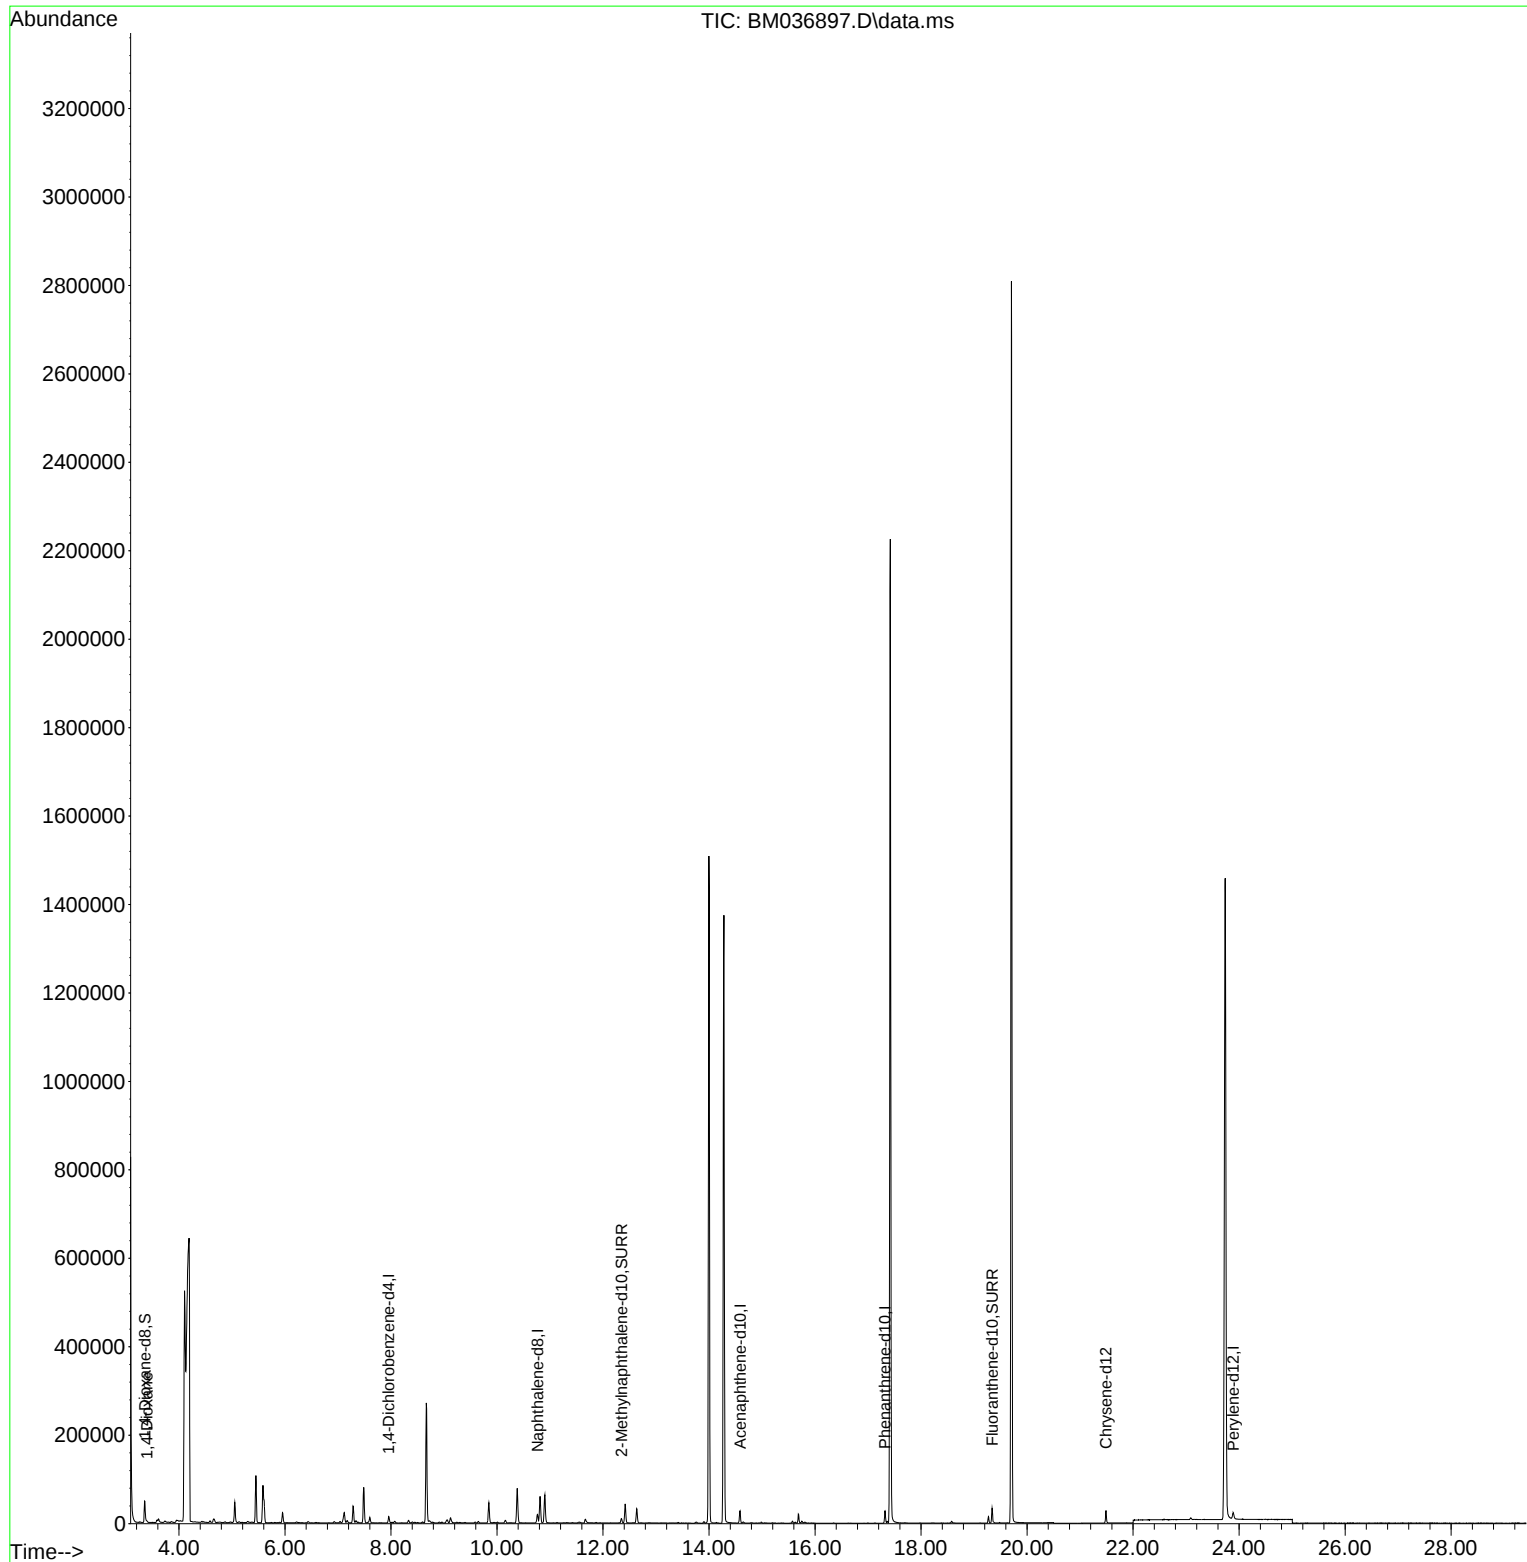

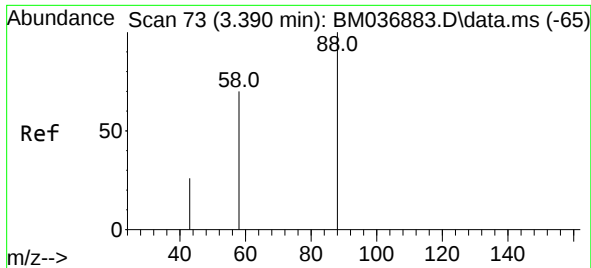

#2
 1,4-Dioxane
 Concen: 0.216 ng/ul
 RT: 3.394 min Scan# 74
 Delta R.T. 0.004 min
 Lab File: BM036897.D
 Acq: 08 Oct 2022 15:42

Instrument :
 BNA_M
 ClientSampleId :
 EXZ63

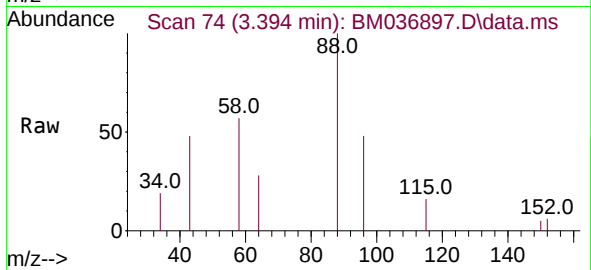

Tgt Ion:	88	Resp:	2136
Ion	Ratio	Lower	Upper
88	100		
43	48.1	37.8	56.6
58	56.7	42.6	63.8

