
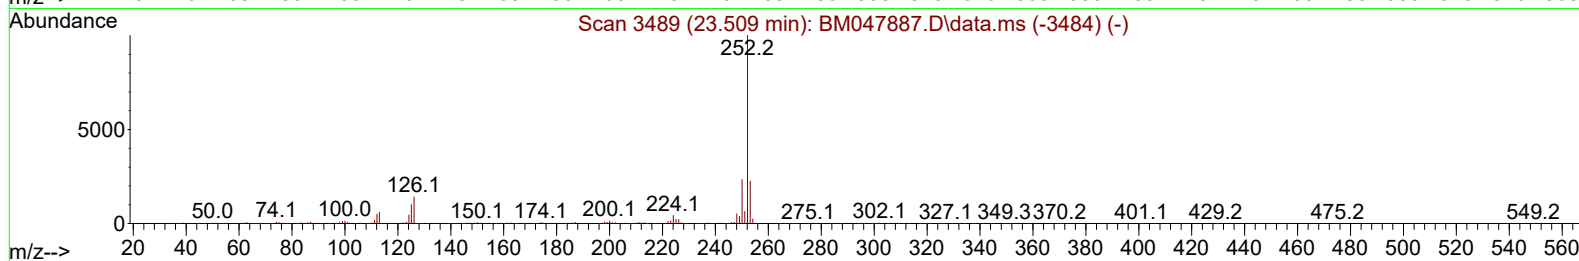
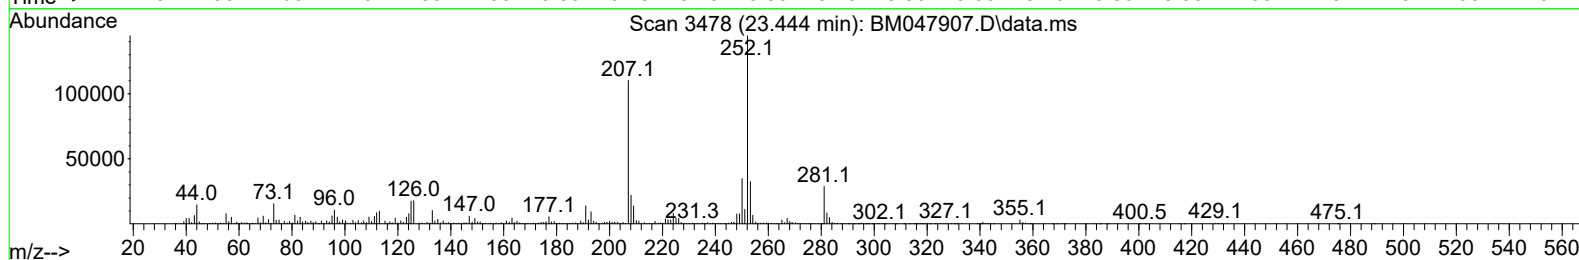


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047907.D
Acq On : 08 Oct 2024 06:55
Operator : RC/JU
Sample : P4131-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Oct 08 07:29:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration

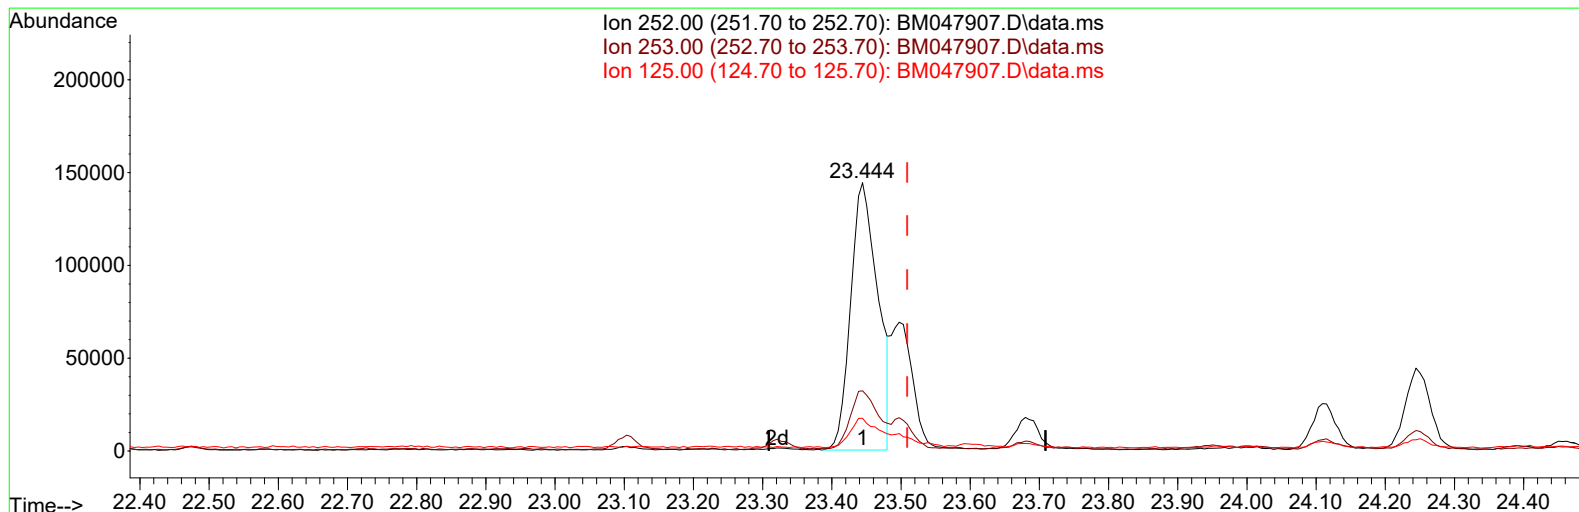

TIC: BM047907.D\data.ms

(91) Benzo(k)fluoranthene

23.444min (-0.064) 3.49 ng/uI

response 391385

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	22.44
125.00	11.10	12.16
0.00	0.00	0.00