




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047903.D
 Acq On : 08 Oct 2024 04:17
 Operator : RC/JU
 Sample : PB163648BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK648

Manual IntegrationsAPPROVED

Quant Time: Oct 08 04:52:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 08:32:31 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/11/2024

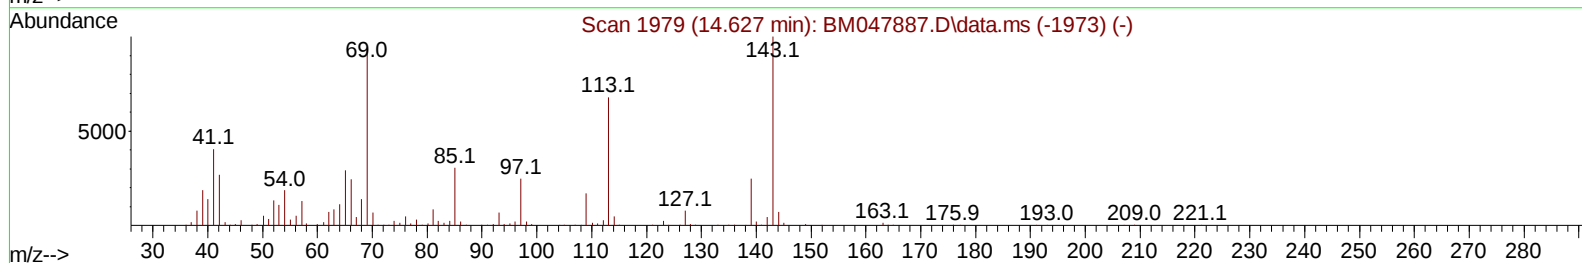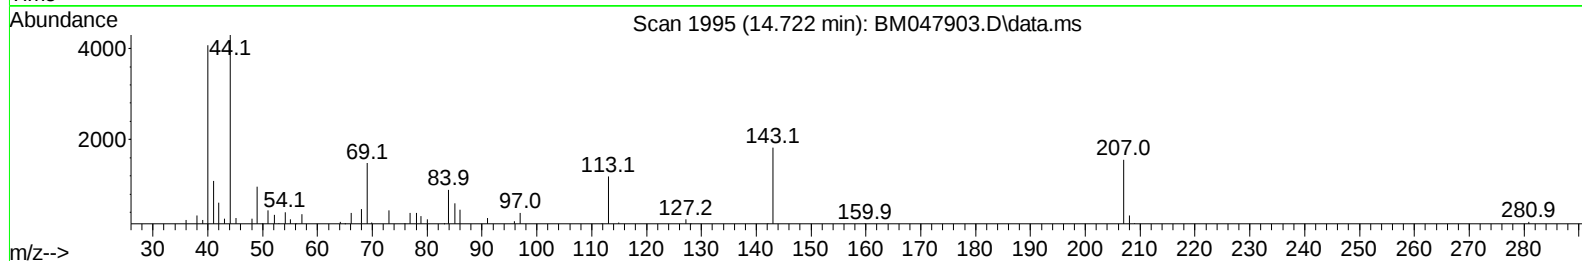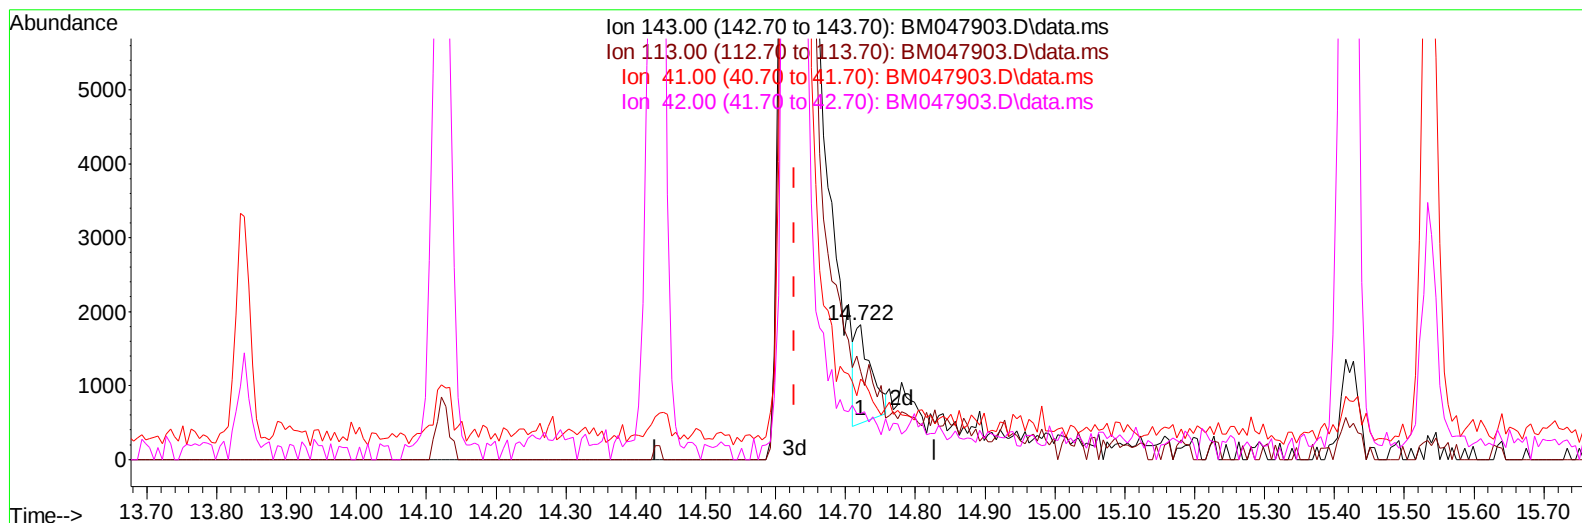

TIC: BM047903.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (+ 0.095) 0.19 ng/u1

response 2102

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.20	65.13
41.00	60.00	59.61
42.00	40.50	33.72




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047903.D
Acq On : 08 Oct 2024 04:17
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Manual IntegrationsAPPROVED

Quant Time: Oct 08 04:52:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024

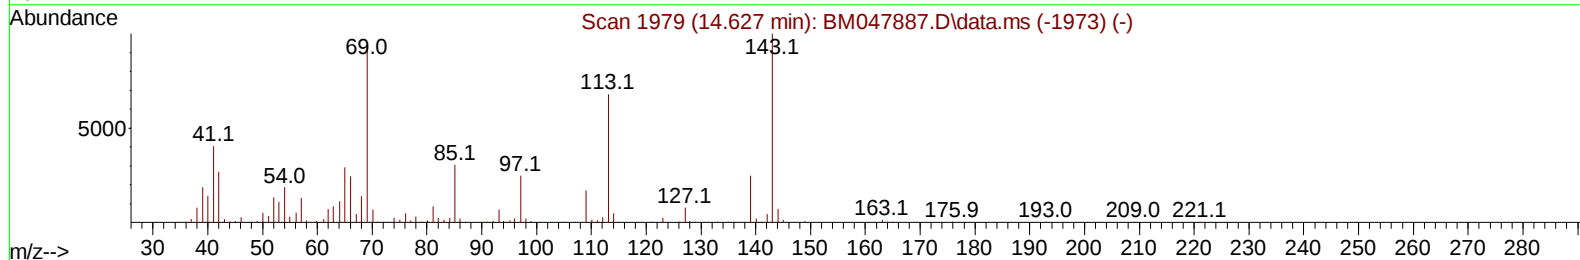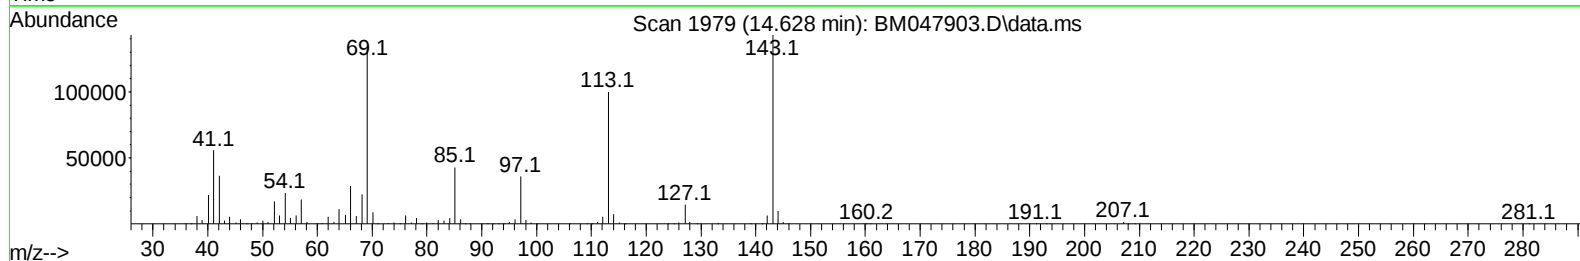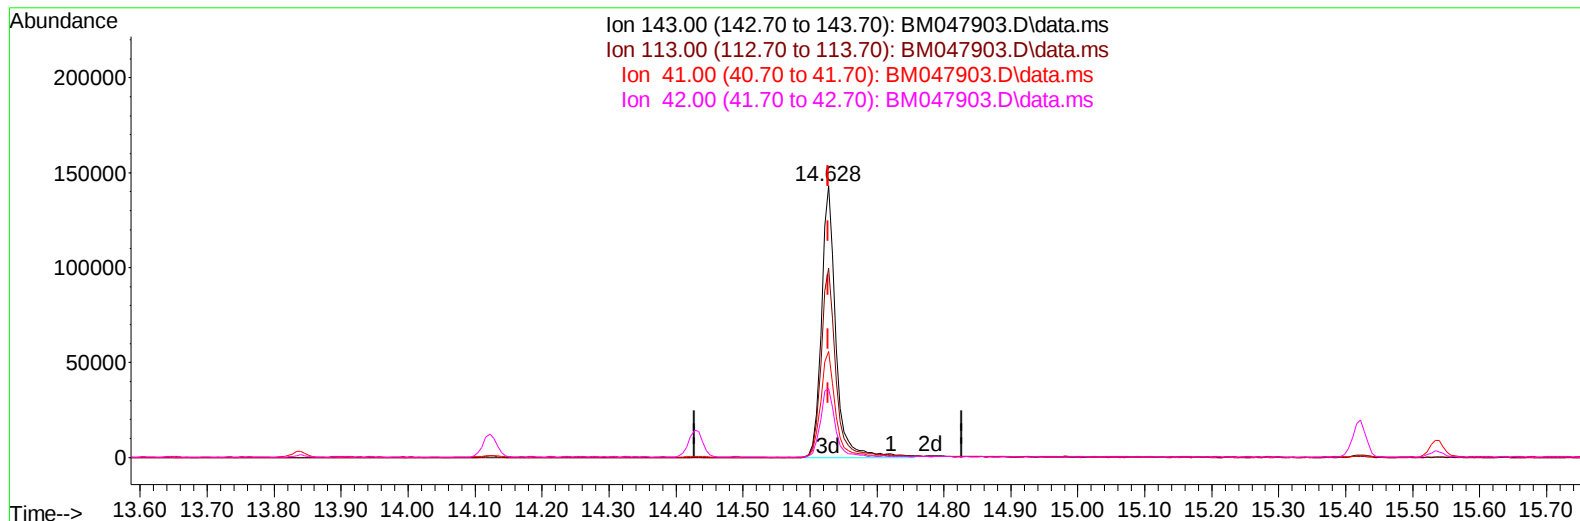

TIC: BM047903.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.628min (+ 0.001) 19.83 ng/ul m

response 215508

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.20	69.74
41.00	60.00	39.00#
42.00	40.50	25.43#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047903.D
 Acq On : 08 Oct 2024 04:17
 Operator : RC/JU
 Sample : PB163648BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK648

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/11/2024

Quant Time: Oct 08 04:56:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 08:32:31 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.793	152		304615	20.000	ng/ul	0.00
20) Naphthalene-d8	10.587	136		1224626	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.428	164		752769	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.169	188		1524528	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240		1397593	20.000	ng/ul	0.00
88) Perylene-d12	24.392	264		1581742	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.246	96		36449	3.867	ng/uL	0.00
4) Pyridine-d5	3.664	84		533149	19.317	ng/ul	0.00
7) Phenol-d5	6.964	99		612255	21.256	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67		377596	18.474	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132		522921	24.952	ng/ul	0.00
15) 4-Methylphenol-d8	8.499	113		478589	22.347	ng/ul	0.00
21) Nitrobenzene-d5	8.952	128		243118	24.934	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143		257982	27.610	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.210	165		468633	25.106	ng/ul	0.00
31) 4-Chloroaniline-d4	10.722	131		678941	23.527	ng/ul	0.00
46) Dimethylphthalate-d6	13.840	166		1312320	24.046	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160		1588265	24.545	ng/ul	0.00
54) 4-Nitrophenol-d4	14.628	143		215508m	19.833	ng/ul	0.00
60) Fluorene-d10	15.422	176		1171379	24.779	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.539	200		144817	16.233	ng/ul	0.00
73) Anthracene-d10	17.269	188		1798323	23.990	ng/ul	0.00
81) Pyrene-d10	19.557	212		2040465	25.724	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.186	264		2057253	25.068	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047903.D
Acq On : 08 Oct 2024 04:17
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Manual IntegrationsAPPROVED

Quant Time: Oct 08 04:56:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024

