

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047890.D
 Acq On : 07 Oct 2024 19:04
 Operator : RC/JU
 Sample : P4083-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4EK3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/08/2024
 Supervised By :mohammad ahmed 10/11/2024

Quant Time: Oct 07 23:25:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 08:32:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.798	152	207306	20.000	ng/u1	0.00
20) Naphthalene-d8	10.586	136	832026	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.433	164	508165	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.168	188	1024306	20.000	ng/u1	0.00
79) Chrysene-d12	21.397	240	964716	20.000	ng/u1	0.00
88) Perylene-d12	24.397	264	1073152	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	7998	1.247	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.963	99	209658	10.695	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	151195	10.869	ng/u1	0.00
11) 2-Chlorophenol-d4	7.328	132	186712	13.091	ng/u1	0.00
15) 4-Methylphenol-d8	8.504	113	114502	7.856	ng/u1	0.00
21) Nitrobenzene-d5	8.951	128	94712	14.297	ng/u1	0.00
24) 2-Nitrophenol-d4	9.669	143	100839	15.884	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.210	165	184389	14.540	ng/u1	0.00
31) 4-Chloroaniline-d4	10.722	131	133398	6.804	ng/u1	0.00
46) Dimethylphthalate-d6	13.839	166	573685	15.571	ng/u1	0.00
49) Acenaphthylene-d8	14.121	160	663147	15.181	ng/u1	0.00
54) 4-Nitrophenol-d4	14.627	143	70339	9.589	ng/u1	0.00
60) Fluorene-d10	15.421	176	518474	16.247	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.539	200	49139	8.198	ng/u1	0.00
73) Anthracene-d10	17.268	188	729022	14.474	ng/u1	0.00
81) Pyrene-d10	19.556	212	804251	14.689	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.185	264	657635	11.811	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.616	105	70530	2.828	ng/u1	92
72) Phenanthrene	17.209	178	250510	4.170	ng/u1	99
80) Fluoranthene	19.221	202	531146	8.237	ng/u1	97
82) Pyrene	19.586	202	323979	4.514	ng/u1#	95
85) Benzo(a)anthracene	21.380	228	231470	3.427	ng/u1	98
86) Bis(2-ethylhexyl)phtha...	21.303	149	139776	3.669	ng/u1#	99
87) Chrysene	21.439	228	268181m	4.073	ng/u1	
90) Benzo(b)fluoranthene	23.450	252	337161	5.038	ng/u1	97
91) Benzo(k)fluoranthene	23.503	252	127519m	1.863	ng/u1	
93) Benzo(a)pyrene	24.250	252	89728	1.412	ng/u1	95
94) Indeno(1,2,3-cd)pyrene	27.773	276	97449	1.196	ng/u1	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047890.D
Acq On : 07 Oct 2024 19:04
Operator : RC/JU
Sample : P4083-08
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4EK3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024


Quant Time: Oct 07 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration

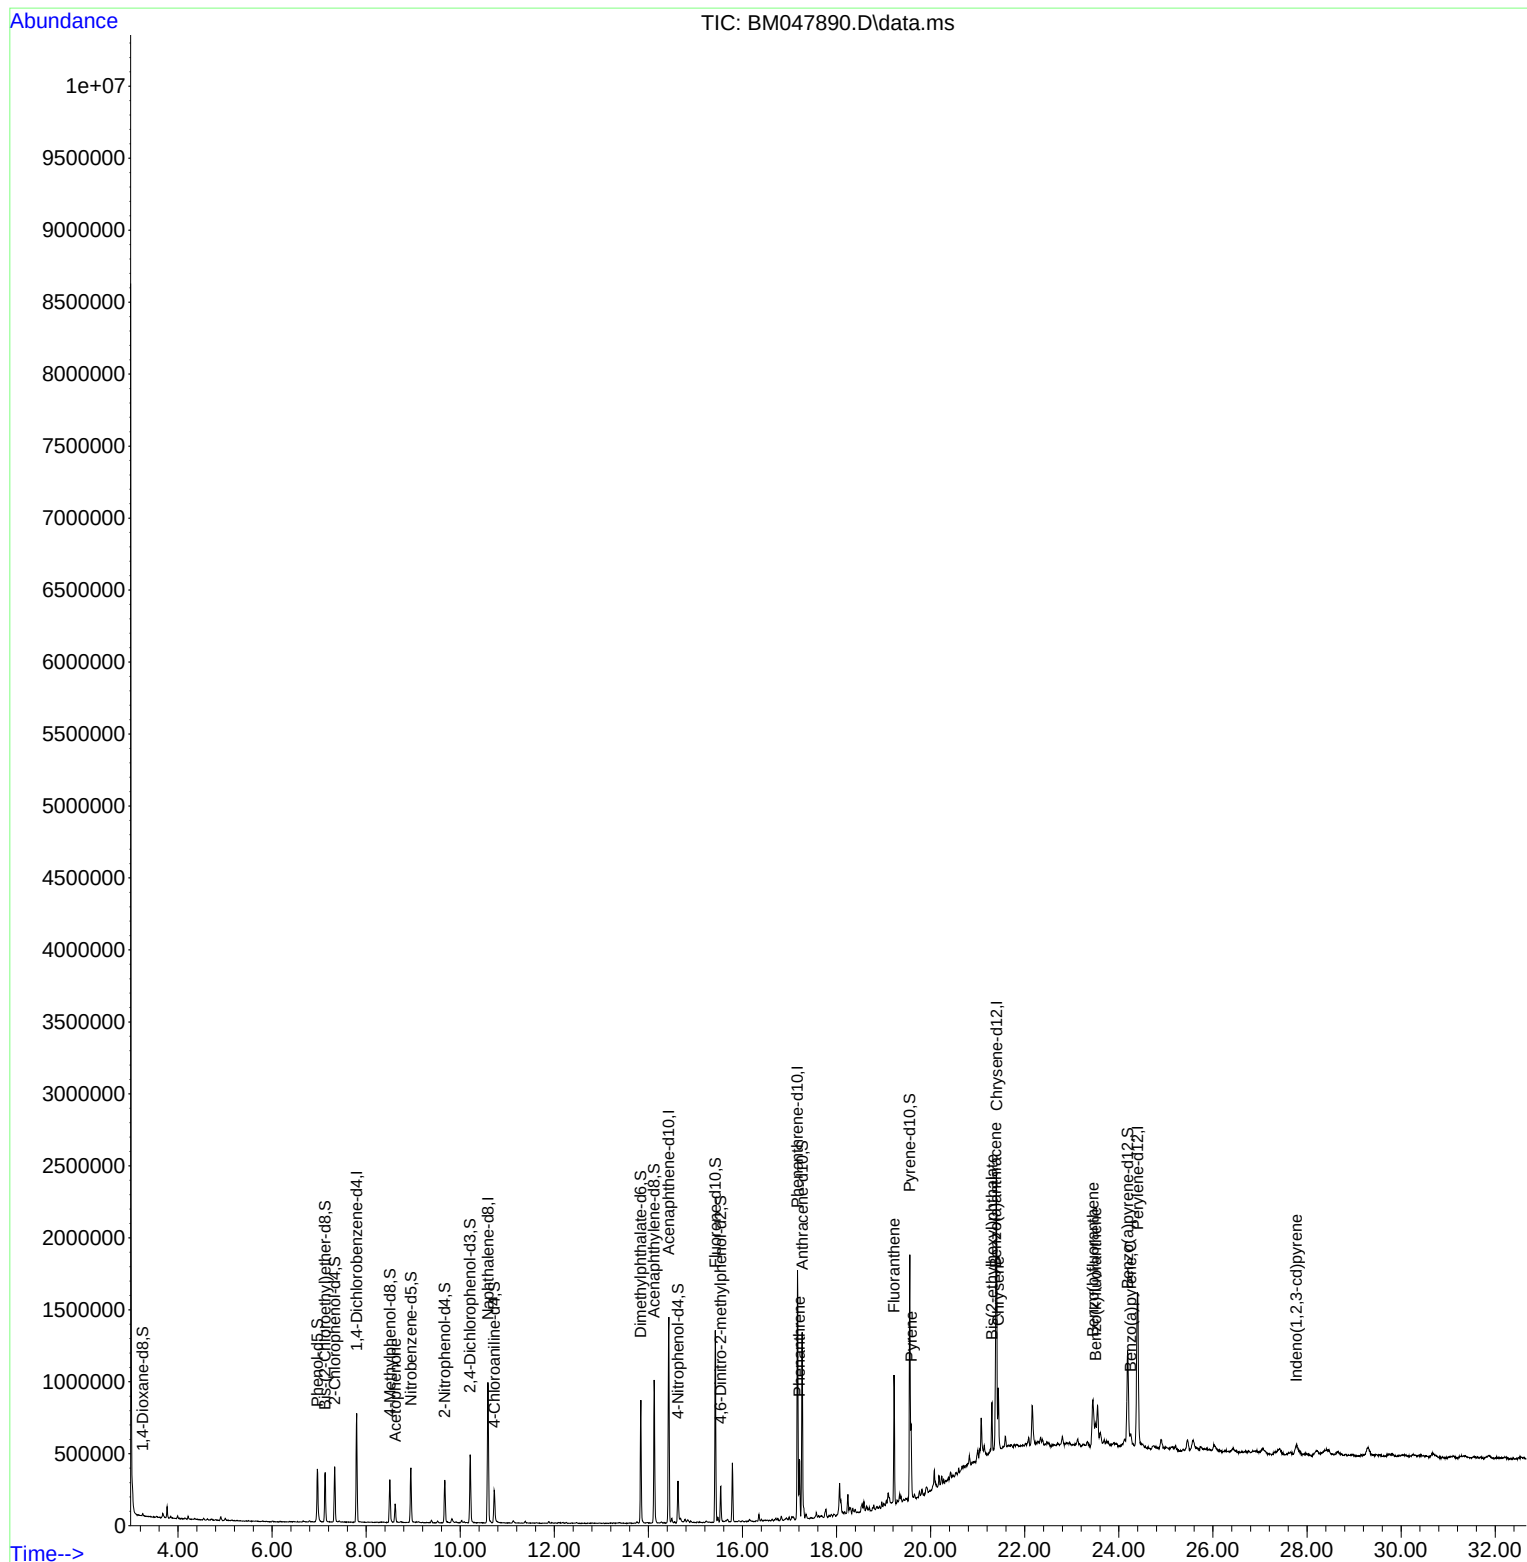



#16
Acetophenone
Concen: 2.828 ng/ul
RT: 8.616 min Scan# 957
Delta R.T. -0.006 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04




Instrument :
BNA_M
ClientSampleId :
A4EK3

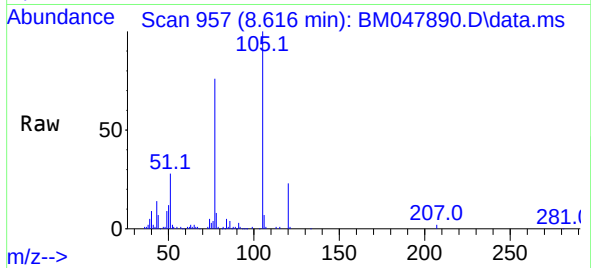

Tgt Ion:105 Resp: 70530
Ion Ratio Lower Upper
105 100
77 76.4 66.6 100.0
51 28.3 27.0 40.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024

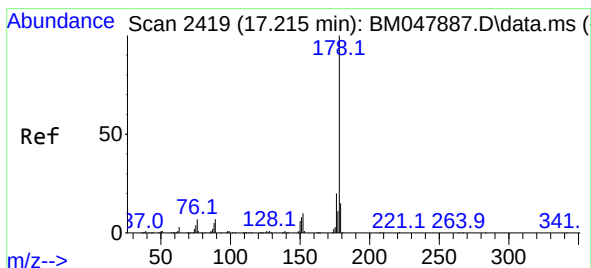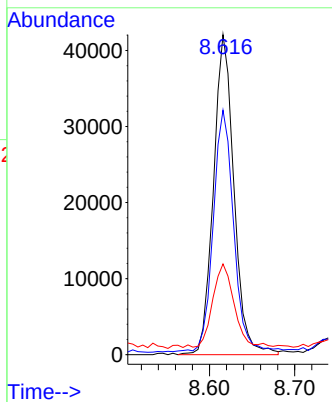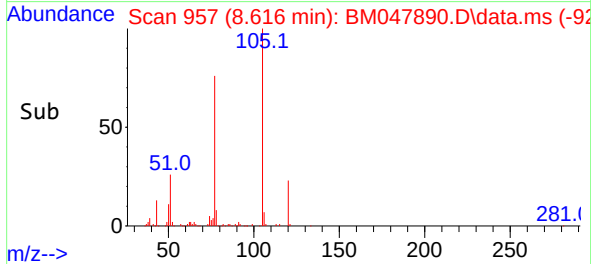

#72
Phenanthrene
Concen: 4.170 ng/ul
RT: 17.209 min Scan# 2418
Delta R.T. -0.006 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04


Tgt Ion:178 Resp: 250510
Ion Ratio Lower Upper
178 100
179 15.2 12.0 18.0
176 19.7 15.4 23.0

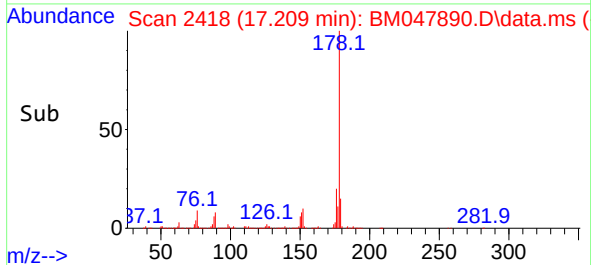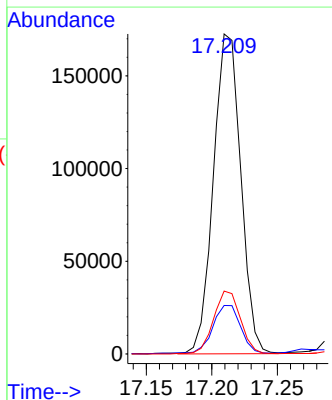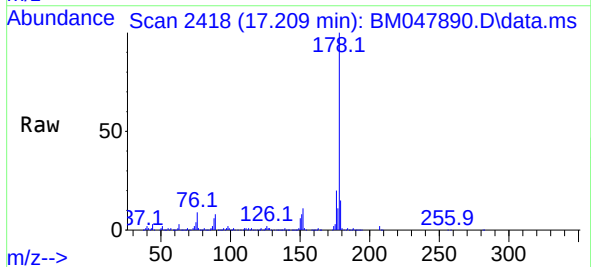



#80
Fluoranthene
Concen: 8.237 ng/u1
RT: 19.221 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04




Instrument :
BNA_M
ClientSampleId :
A4EK3

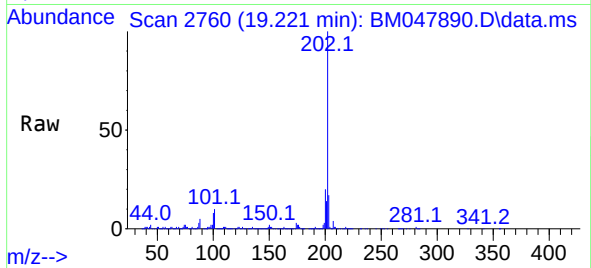

Tgt Ion:202 Resp: 531140
Ion Ratio Lower Upper
202 100
101 10.1 9.0 13.4
100 7.6 6.8 10.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024

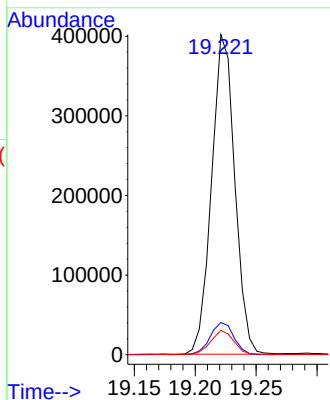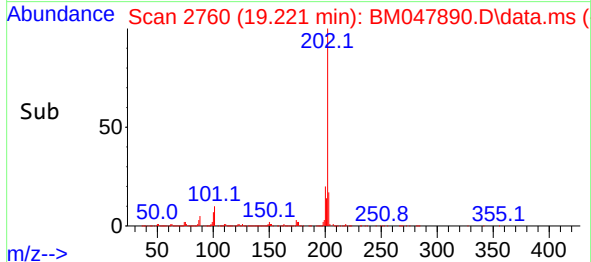

#82
Pyrene
Concen: 4.514 ng/u1
RT: 19.586 min Scan# 2822
Delta R.T. 0.000 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04


Tgt Ion:202 Resp: 323979
Ion Ratio Lower Upper
202 100
101 11.9 10.9 16.3
100 9.4 9.4 14.2#

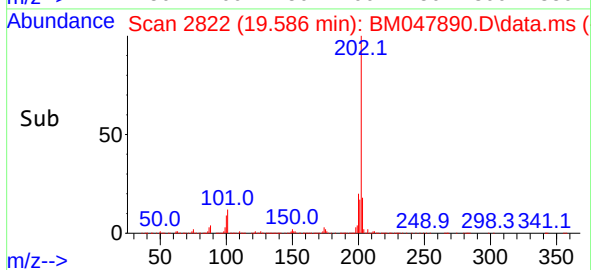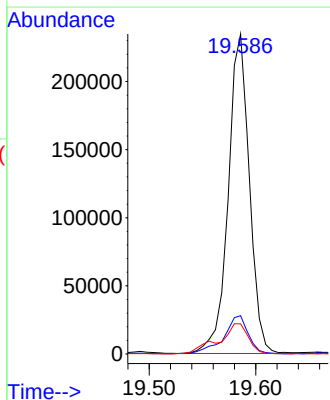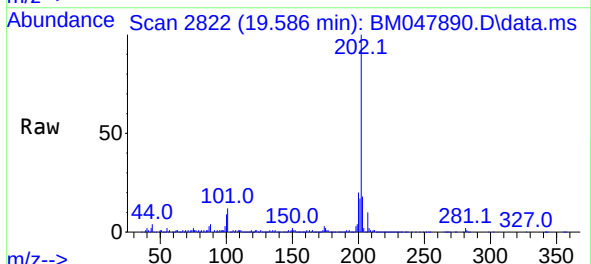



#85
Benzo(a)anthracene
Concen: 3.427 ng/ul
RT: 21.380 min Scan# 3127
Delta R.T. 0.000 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04




Instrument :
BNA_M
ClientSampleId :
A4EK3



Tgt Ion:228 Resp: 231470
Ion Ratio Lower Upper
228 100
229 21.0 15.6 23.4
226 28.2 21.9 32.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024

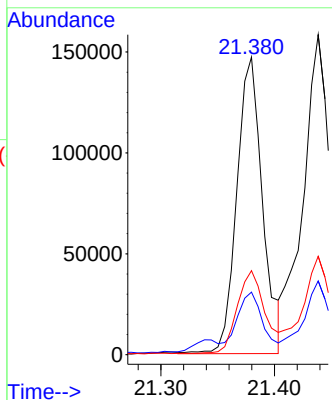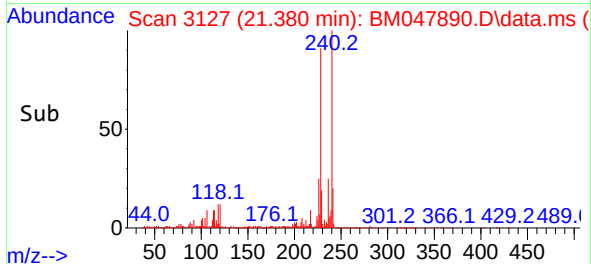

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.669 ng/ul
RT: 21.303 min Scan# 3114
Delta R.T. 0.000 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04


Tgt Ion:149 Resp: 139776
Ion Ratio Lower Upper
149 100
167 26.8 21.3 31.9
279 4.6 2.7 4.1#

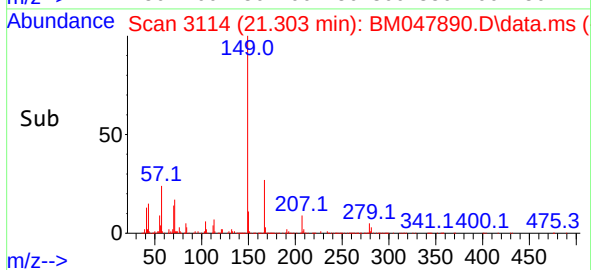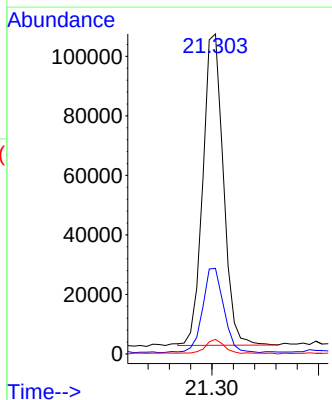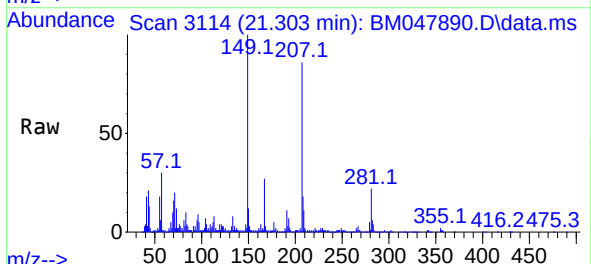



#87
Chrysene
Concen: 4.073 ng/ul m
RT: 21.439 min Scan# 3138
Delta R.T. 0.000 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04




Instrument :
BNA_M
ClientSampleId :
A4EK3



Tgt Ion:228 Resp: 26818
Ion Ratio Lower Upper
228 100
226 30.8 23.6 35.4
229 23.0 15.3 22.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024

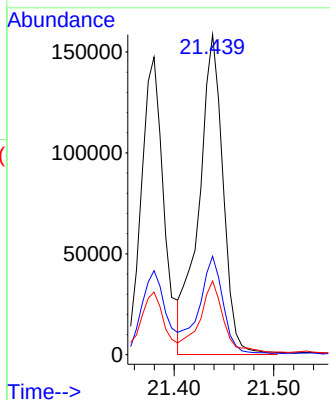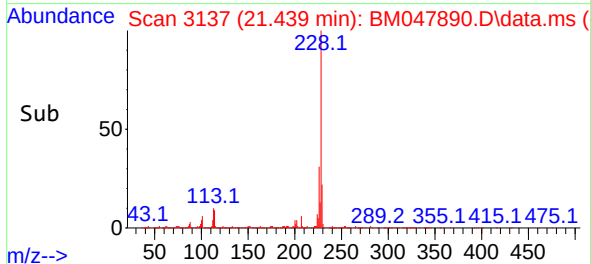

#90
Benzo(b)fluoranthene
Concen: 5.038 ng/ul
RT: 23.450 min Scan# 3479
Delta R.T. 0.000 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04


Tgt Ion:252 Resp: 337161
Ion Ratio Lower Upper
252 100
253 23.7 17.4 26.2
125 11.7 9.0 13.4

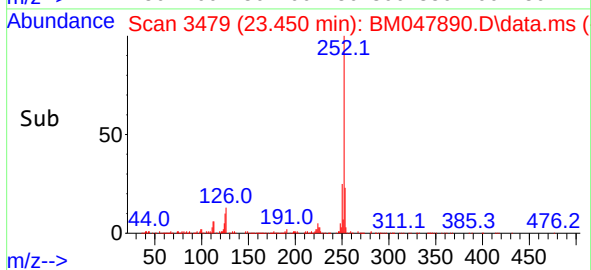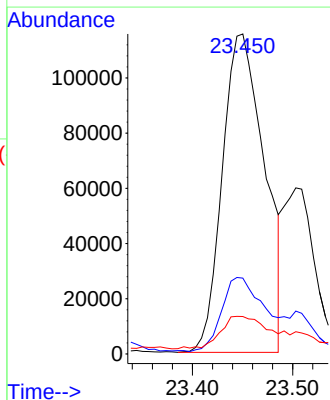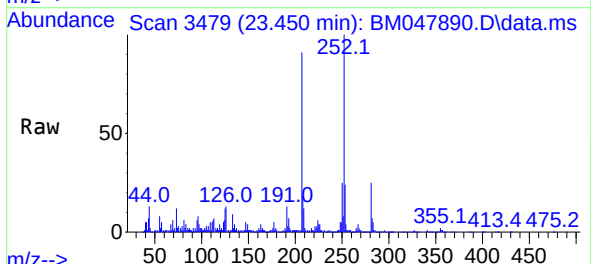



#91
Benzo(k)fluoranthene
Concen: 1.863 ng/ul m
RT: 23.503 min Scan# 3489
Delta R.T. -0.006 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04




Instrument :
BNA_M
ClientSampleId :
A4EK3



Tgt Ion:252 Resp: 127519
Ion Ratio Lower Upper
252 100
253 25.9 17.5 26.3
125 13.4 8.9 13.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024

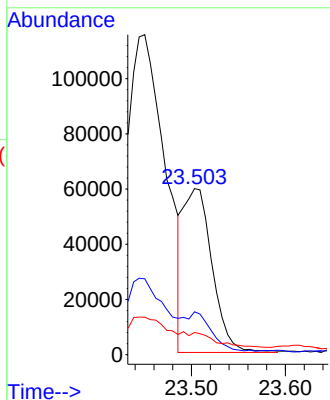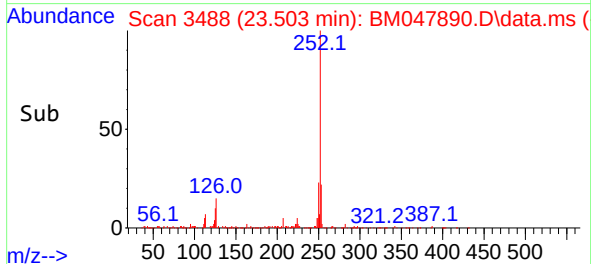

#93
Benzo(a)pyrene
Concen: 1.412 ng/ul
RT: 24.250 min Scan# 3615
Delta R.T. -0.006 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04


Tgt Ion:252 Resp: 89728
Ion Ratio Lower Upper
252 100
253 23.7 17.2 25.8
125 14.7 10.1 15.1

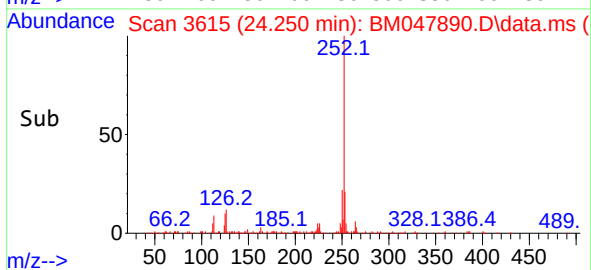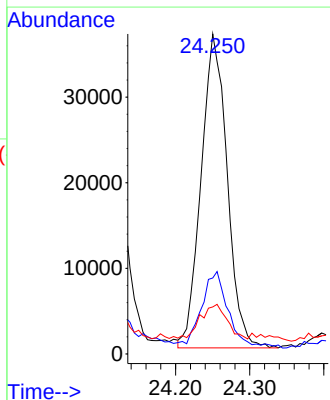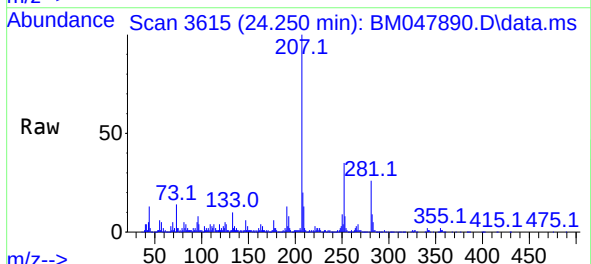

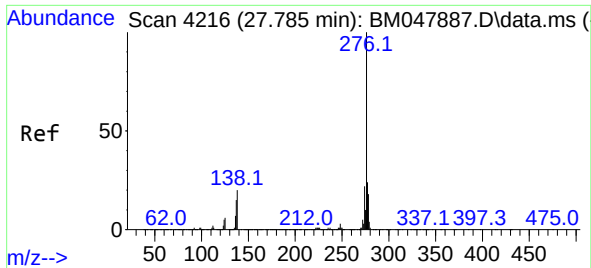

#94
Indeno(1,2,3-cd)pyrene
Concen: 1.196 ng/ul
RT: 27.773 min Scan# 41
Delta R.T. -0.006 min
Lab File: BM047890.D
Acq: 07 Oct 2024 19:04

Instrument :
BNA_M
ClientSampleId :
A4EK3



Tgt Ion:276 Resp: 97449
Ion Ratio Lower Upper
276 100
138 24.1 16.9 25.3
277 27.4 18.9 28.3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/08/2024
Supervised By :mohammad ahmed 10/11/2024

