

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047880.D
 Acq On : 07 Oct 2024 10:39
 Operator : RC/JU
 Sample : PB163718BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK718

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	41	44	50	rVB	68394	92084	1.96%	0.166%
2	3.663	111	115	129	rBV	860519	1309910	27.81%	2.367%
3	3.993	169	171	178	rVB2	14389	20474	0.43%	0.037%
4	6.963	670	676	687	rBV	900419	1465592	31.12%	2.648%
5	7.128	698	704	714	rVB	760696	1170230	24.85%	2.114%
6	7.334	731	739	748	rBV	937584	1534042	32.57%	2.771%
7	7.798	811	818	827	rVB	957255	1505121	31.96%	2.719%
8	7.892	832	834	839	rVB6	4443	5906	0.13%	0.011%
9	8.504	931	938	952	rBV	1105984	1792003	38.05%	3.237%
10	8.951	1006	1014	1025	rBV	854068	1400886	29.75%	2.531%
11	9.675	1127	1137	1145	rBV	672392	1135572	24.11%	2.052%
12	10.210	1221	1228	1239	rBV	1035455	1791082	38.03%	3.236%
13	10.592	1285	1293	1300	rBV	1262239	2113951	44.89%	3.819%
14	10.722	1308	1315	1328	rBV	1036071	1829684	38.85%	3.306%
15	12.180	1558	1563	1568	rBV6	15520	31244	0.66%	0.056%
16	12.398	1596	1600	1603	rBV4	4256	4988	0.11%	0.009%
17	13.839	1838	1845	1854	rBV	1738311	2385425	50.65%	4.310%
18	14.127	1887	1894	1903	rBV	2025217	3060714	64.99%	5.530%
19	14.433	1939	1946	1955	rBV	1879816	2730920	57.99%	4.934%
20	14.627	1973	1979	1996	rBV	727127	1166108	24.76%	2.107%
21	15.421	2107	2114	2123	rBV	2573028	3680773	78.16%	6.650%
22	15.539	2128	2134	2144	rBV	693349	932760	19.81%	1.685%
23	15.663	2151	2155	2160	rVB4	12178	19743	0.42%	0.036%
24	15.998	2207	2212	2215	rVB6	2994	5053	0.11%	0.009%
25	16.957	2372	2375	2380	rVV5	4548	7897	0.17%	0.014%
26	17.174	2405	2412	2420	rBV	2214496	3181035	67.55%	5.747%
27	17.268	2422	2428	2440	rVV2	2781487	3983911	84.60%	7.197%
28	19.121	2740	2743	2750	rVB3	34306	47465	1.01%	0.086%
29	19.192	2752	2755	2761	rVV	34560	46230	0.98%	0.084%
30	19.556	2811	2817	2826	rBV	3603063	4686937	99.52%	8.468%
31	21.397	3124	3130	3136	rBV2	2401363	3566006	75.72%	6.442%
32	24.191	3597	3605	3616	rVB	1921047	4709368	100.00%	8.508%
33	24.397	3632	3640	3652	rVB	1549885	3938934	83.64%	7.116%




Sum of corrected areas: 55352048

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047880.D
Acq On : 07 Oct 2024 10:39
Operator : RC/JU
Sample : PB163718BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK718

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

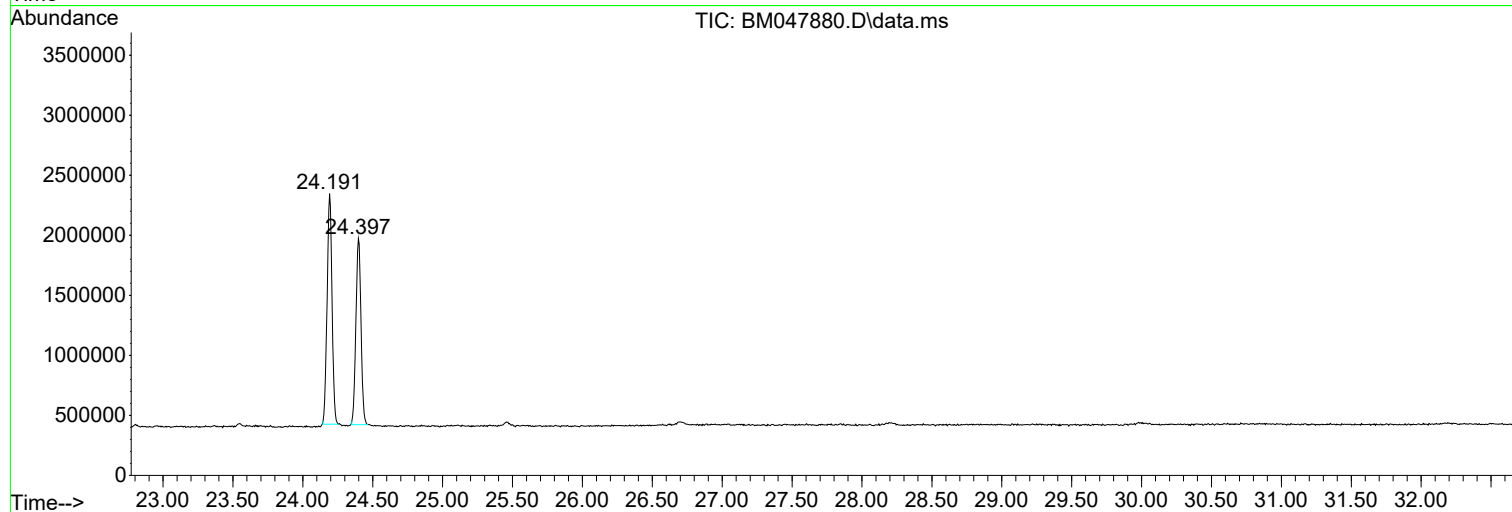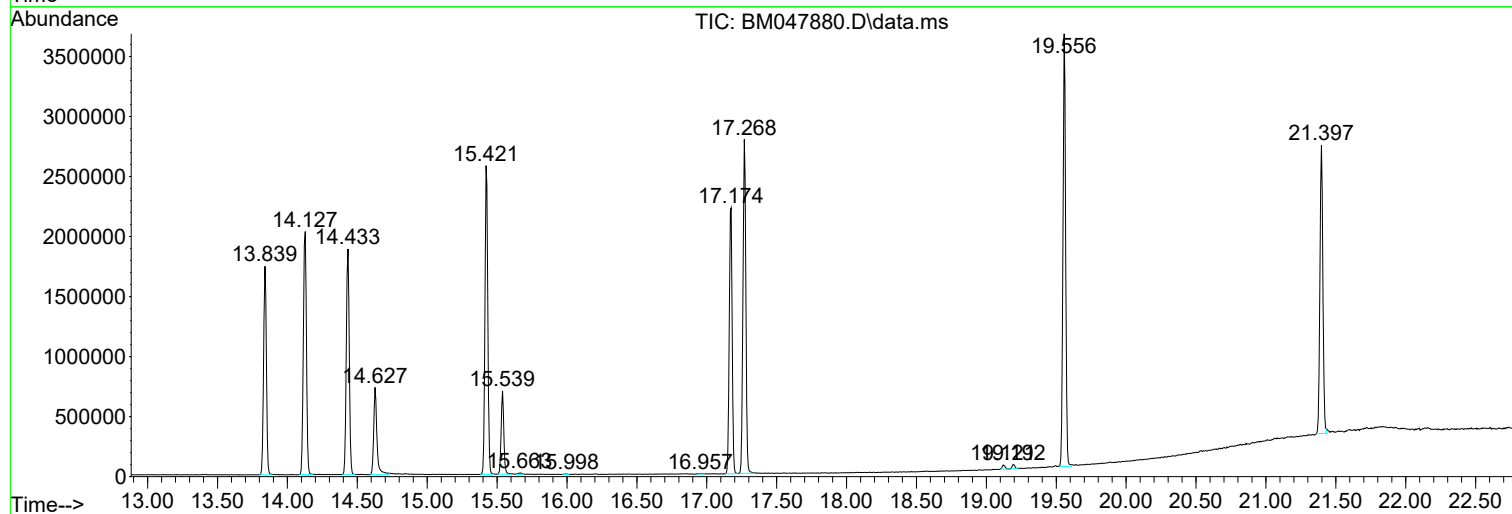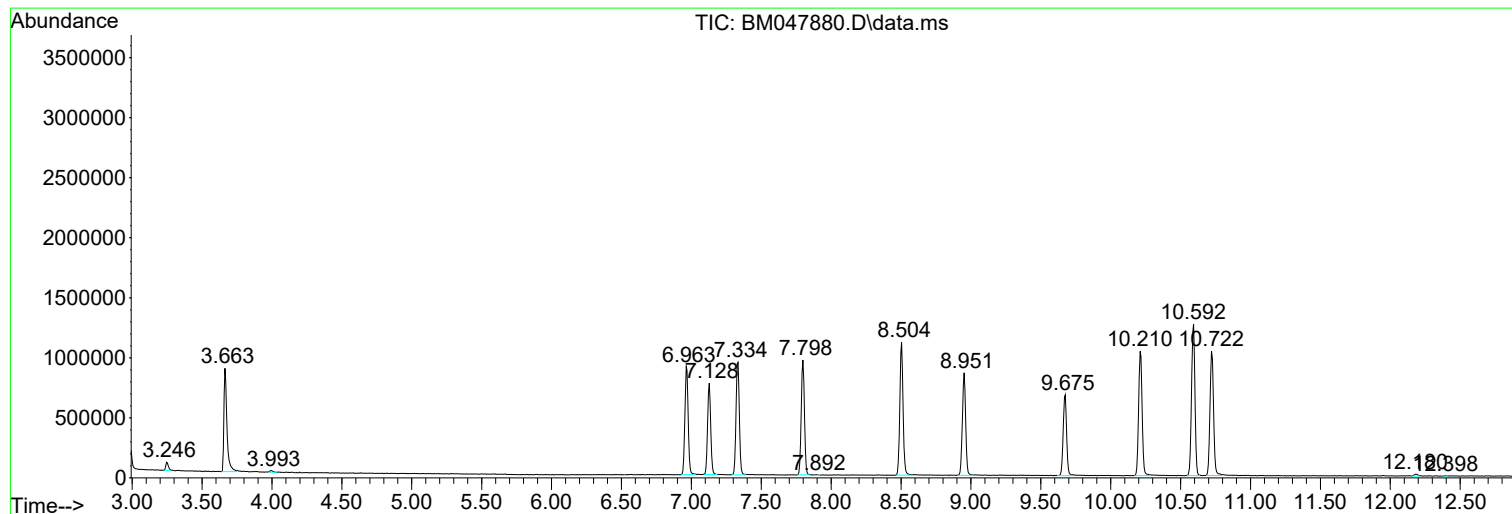

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047880.D
Acq On : 07 Oct 2024 10:39
Operator : RC/JU
Sample : PB163718BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK718

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047880.D
Acq On : 07 Oct 2024 10:39
Operator : RC/JU
Sample : PB163718BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK718

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc