

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047898.D
 Acq On : 08 Oct 2024 00:21
 Operator : RC/JU
 Sample : P4109-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4ET9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	42	45	53	rVB3	23175	33924	0.72%	0.102%
2	3.681	115	118	129	rVB3	29571	54644	1.16%	0.164%
3	3.769	130	133	139	rVB2	26553	34982	0.74%	0.105%
4	3.993	168	171	177	rVB5	20605	27901	0.59%	0.084%
5	4.910	322	327	331	rBV2	32537	50684	1.08%	0.152%
6	6.963	666	676	690	rBV	258730	464457	9.89%	1.395%
7	7.128	698	704	711	rBV	197210	315833	6.72%	0.948%
8	7.328	731	738	748	rBV	264946	437444	9.31%	1.313%
9	7.428	752	755	758	rVB4	7372	9946	0.21%	0.030%
10	7.798	811	818	825	rBV	1154185	1829851	38.95%	5.494%
11	8.504	931	938	951	rBV	252364	436045	9.28%	1.309%
12	8.616	951	957	965	rVB	76827	130550	2.78%	0.392%
13	8.740	973	978	986	rVB10	5872	12633	0.27%	0.038%
14	8.945	1005	1013	1022	rBV	212020	376921	8.02%	1.132%
15	9.387	1083	1088	1094	rVB8	6327	11009	0.23%	0.033%
16	9.516	1105	1110	1117	rVB4	25915	45148	0.96%	0.136%
17	9.669	1127	1136	1151	rBV	168975	309240	6.58%	0.929%
18	9.822	1156	1162	1171	rBV5	11309	27687	0.59%	0.083%
19	10.022	1191	1196	1198	rBV6	7597	12655	0.27%	0.038%
20	10.210	1221	1228	1238	rBV	299261	528904	11.26%	1.588%
21	10.586	1283	1292	1302	rBV	1513856	2618673	55.74%	7.863%
22	10.722	1308	1315	1325	rBV	148288	296739	6.32%	0.891%
23	11.133	1380	1385	1389	rBV8	12474	21096	0.45%	0.063%
24	11.375	1423	1426	1428	rBV4	7727	9736	0.21%	0.029%
25	12.186	1556	1564	1568	rVB7	5737	12967	0.28%	0.039%
26	13.263	1743	1747	1751	rBV5	6213	8656	0.18%	0.026%
27	13.757	1827	1831	1835	rVB6	7443	10481	0.22%	0.031%
28	13.839	1838	1845	1852	rBV	544382	765551	16.30%	2.299%
29	14.122	1882	1893	1902	rBV	613066	942160	20.05%	2.829%
30	14.269	1915	1918	1926	rVB8	7477	12592	0.27%	0.038%
31	14.433	1936	1946	1953	rBV	2258763	3393390	72.23%	10.189%
32	14.498	1953	1957	1962	rVB3	14574	22263	0.47%	0.067%
33	14.557	1964	1967	1973	rVB8	6166	8990	0.19%	0.027%
34	14.627	1973	1979	1988	rBV	140989	266470	5.67%	0.800%
35	14.751	1994	2000	2002	rBV3	10532	14696	0.31%	0.044%
36	14.851	2010	2017	2021	rVB10	9430	18130	0.39%	0.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047898.D
 Acq On : 08 Oct 2024 00:21
 Operator : RC/JU
 Sample : P4109-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4ET9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	15.227	2077	2081	2086	rBV6	13989	22040	0.47%	0.066%
38	15.421	2107	2114	2120	rBV	840181	1205682	25.66%	3.620%
39	15.480	2120	2124	2127	rVB4	13518	18180	0.39%	0.055%
40	15.533	2127	2133	2140	rBV	122089	190203	4.05%	0.571%
41	15.786	2170	2176	2183	rBV	199451	272523	5.80%	0.818%
42	15.992	2209	2211	2218	rVB8	6996	13834	0.29%	0.042%
43	16.151	2235	2238	2245	rBV8	8588	16076	0.34%	0.048%
44	16.527	2299	2302	2306	rVB6	6871	11169	0.24%	0.034%
45	16.586	2306	2312	2314	rBV6	8621	15013	0.32%	0.045%
46	16.710	2330	2333	2337	rVB6	7166	9610	0.20%	0.029%
47	16.774	2341	2344	2349	rVB3	11114	16583	0.35%	0.050%
48	16.827	2349	2353	2359	rVB7	14653	25406	0.54%	0.076%
49	16.886	2359	2363	2367	rBV7	13477	21055	0.45%	0.063%
50	17.086	2395	2397	2401	rVB5	8729	9181	0.20%	0.028%
51	17.168	2403	2411	2416	rBV	2722987	4007104	85.30%	12.032%
52	17.210	2416	2418	2422	rVV	185777	223611	4.76%	0.671%
53	17.268	2422	2428	2439	rVV	861832	1306691	27.81%	3.924%
54	17.351	2439	2442	2448	rVB8	14023	30374	0.65%	0.091%
55	17.751	2507	2510	2519	rBV8	19444	49013	1.04%	0.147%
56	18.015	2550	2555	2557	rBV4	31004	45810	0.98%	0.138%
57	18.062	2558	2563	2566	rBV3	122141	179345	3.82%	0.539%
58	18.239	2588	2593	2597	rBV3	49477	80591	1.72%	0.242%
59	18.474	2629	2633	2638	rBV3	45407	63739	1.36%	0.191%
60	18.633	2657	2660	2664	rBV3	17716	24941	0.53%	0.075%
61	18.957	2713	2715	2719	rVB3	23310	25328	0.54%	0.076%
62	19.004	2719	2723	2729	rBV7	61747	113334	2.41%	0.340%
63	19.221	2756	2760	2765	rVB	370301	458404	9.76%	1.376%
64	19.280	2767	2770	2775	rVB2	48433	60623	1.29%	0.182%
65	19.556	2811	2817	2820	rBV	919719	1367988	29.12%	4.108%
66	21.398	3123	3130	3135	rBV	2886684	4536750	96.57%	13.622%
67	24.186	3600	3604	3611	rVB	306413	612696	13.04%	1.840%
68	24.391	3631	3639	3653	rVB	1875864	4697882	100.00%	14.106%




Sum of corrected areas: 33303827

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047898.D
Acq On : 08 Oct 2024 00:21
Operator : RC/JU
Sample : P4109-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4ET9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

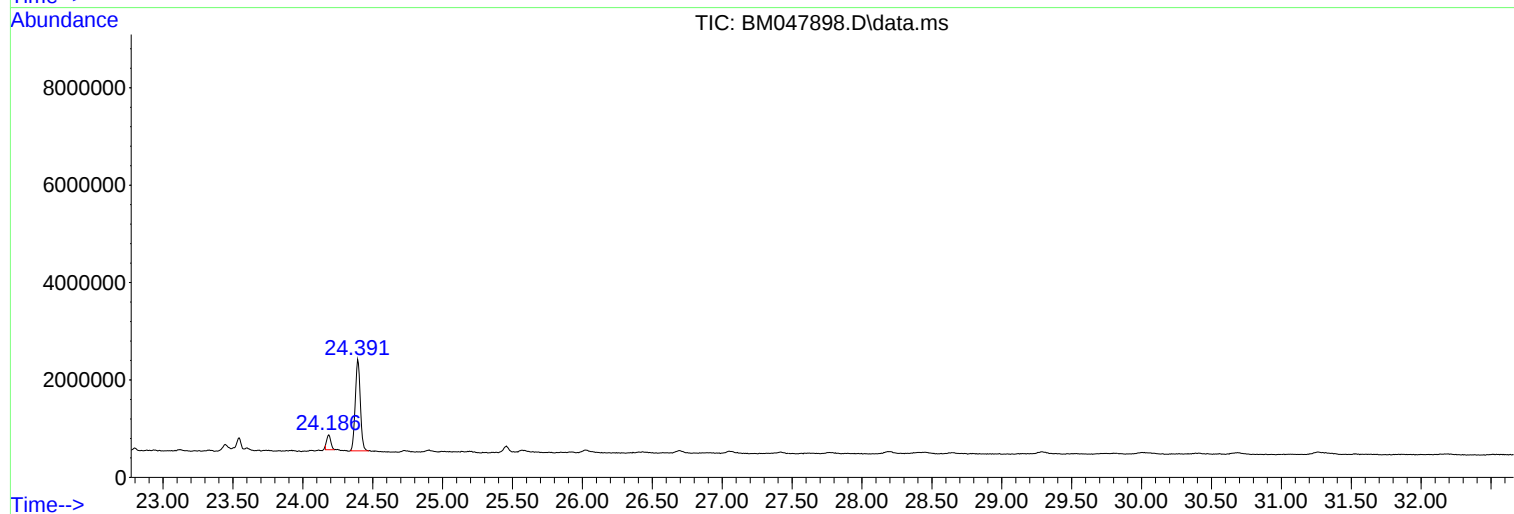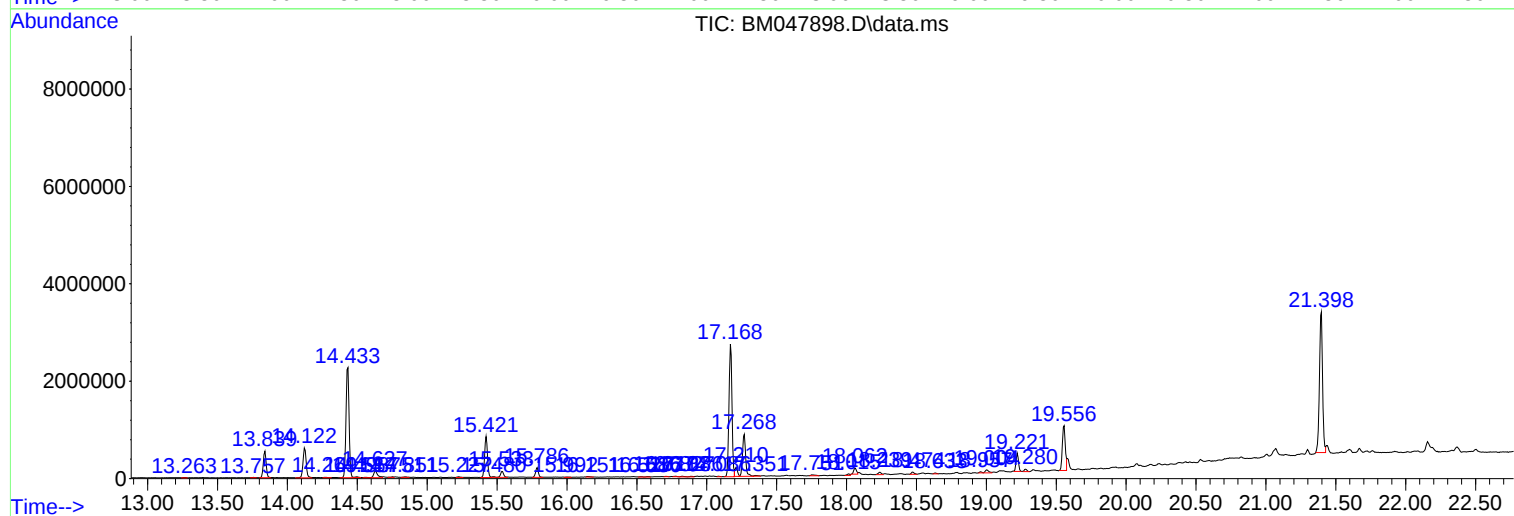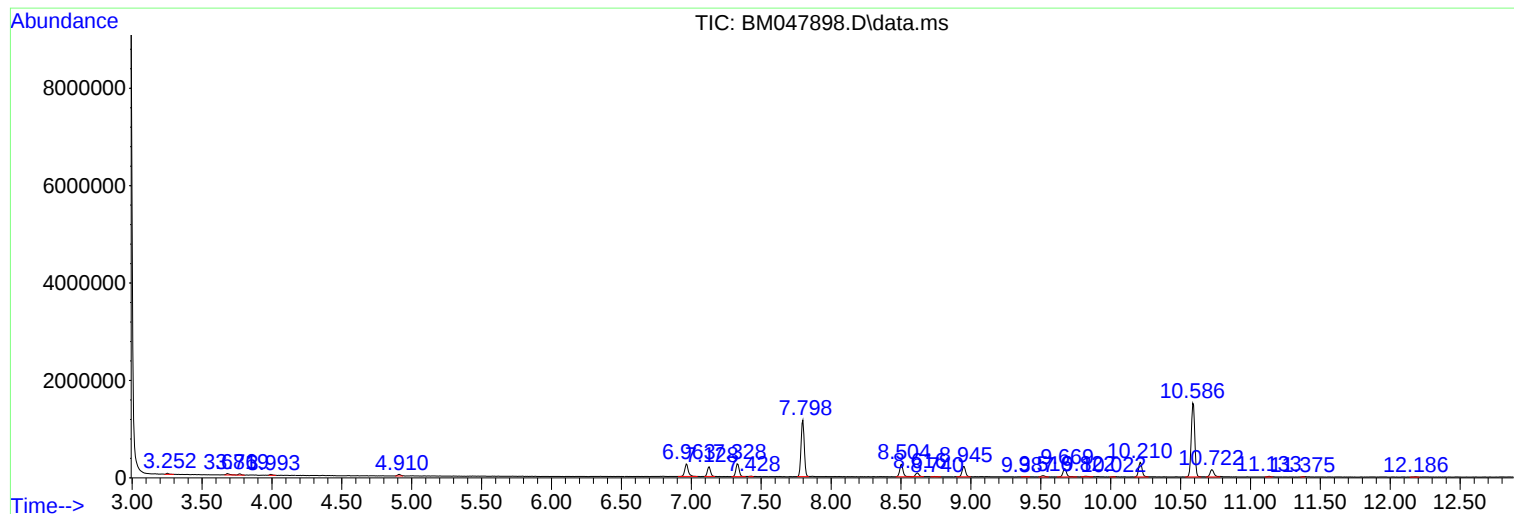

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047898.D
Acq On : 08 Oct 2024 00:21
Operator : RC/JU
Sample : P4109-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4ET9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047898.D
Acq On : 08 Oct 2024 00:21
Operator : RC/JU
Sample : P4109-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4ET9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc