

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047903.D
 Acq On : 08 Oct 2024 04:17
 Operator : RC/JU
 Sample : PB163648BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK648

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	41	44	51	rVB	81459	106287	2.07%	0.170%
2	3.664	111	115	132	rBV	971832	1468152	28.65%	2.349%
3	3.993	167	171	176	rVB2	17228	22326	0.44%	0.036%
4	5.640	448	451	453	rBV4	4913	6960	0.14%	0.011%
5	6.964	669	676	688	rBV	1061841	1680540	32.80%	2.689%
6	7.128	697	704	714	rBV	833531	1350509	26.36%	2.161%
7	7.328	731	738	746	rBV	1124137	1755755	34.27%	2.809%
8	7.793	810	817	829	rBV	1079467	1738451	33.93%	2.781%
9	8.499	930	937	948	rBV	1260959	2060165	40.21%	3.296%
10	8.946	1006	1013	1022	rBV	954500	1615118	31.52%	2.584%
11	9.669	1128	1136	1150	rBV	769963	1308856	25.55%	2.094%
12	10.210	1220	1228	1246	rBV	1228392	2100120	40.99%	3.360%
13	10.587	1284	1292	1303	rVB	1463782	2451176	47.84%	3.922%
14	10.722	1307	1315	1337	rBV	1216568	2138481	41.74%	3.421%
15	12.181	1556	1563	1571	rBV2	18041	35632	0.70%	0.057%
16	13.840	1838	1845	1853	rBV	2049366	2726883	53.22%	4.363%
17	14.122	1884	1893	1902	rVV	2443156	3559081	69.47%	5.694%
18	14.428	1938	1945	1953	rBV	2128849	3147866	61.44%	5.036%
19	14.628	1973	1979	1995	rBV	849143	1341532	26.18%	2.146%
20	14.792	2004	2007	2011	rVB5	4712	6581	0.13%	0.011%
21	14.845	2013	2016	2019	rVB4	4509	6208	0.12%	0.010%
22	15.422	2107	2114	2127	rBV	2949752	4259682	83.14%	6.815%
23	15.534	2127	2133	2143	rBV	706937	1001221	19.54%	1.602%
24	15.663	2151	2155	2162	rVB4	13539	21700	0.42%	0.035%
25	15.975	2206	2208	2212	rVB4	4365	5348	0.10%	0.009%
26	16.598	2310	2314	2317	rBV4	3300	5299	0.10%	0.008%
27	16.851	2354	2357	2363	rVB8	4616	7184	0.14%	0.011%
28	16.951	2373	2374	2379	rVB4	4840	5779	0.11%	0.009%
29	17.169	2404	2411	2421	rBV	2540373	3612991	70.52%	5.780%
30	17.269	2421	2428	2439	rVV2	3117726	4500496	87.84%	7.200%
31	17.428	2450	2455	2458	rBV7	4679	8510	0.17%	0.014%
32	17.545	2473	2475	2480	rBV6	5056	7431	0.15%	0.012%
33	18.069	2561	2564	2566	rBV4	5613	6251	0.12%	0.010%
34	19.122	2739	2743	2747	rBV3	40312	51471	1.00%	0.082%
35	19.192	2751	2755	2760	rVB	36240	46957	0.92%	0.075%
36	19.557	2811	2817	2825	rBV	3856779	5123557	100.00%	8.197%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047903.D
Acq On : 08 Oct 2024 04:17
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	21.392	3123	3129	3140	rBV2	2609950	3888366	75.89%	6.221%
38	24.186	3595	3604	3617	rVB	2051372	5072027	98.99%	8.114%
39	24.392	3631	3639	3651	rVB2	1586832	4255013	83.05%	6.807%




Sum of corrected areas: 62505962

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047903.D
Acq On : 08 Oct 2024 04:17
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

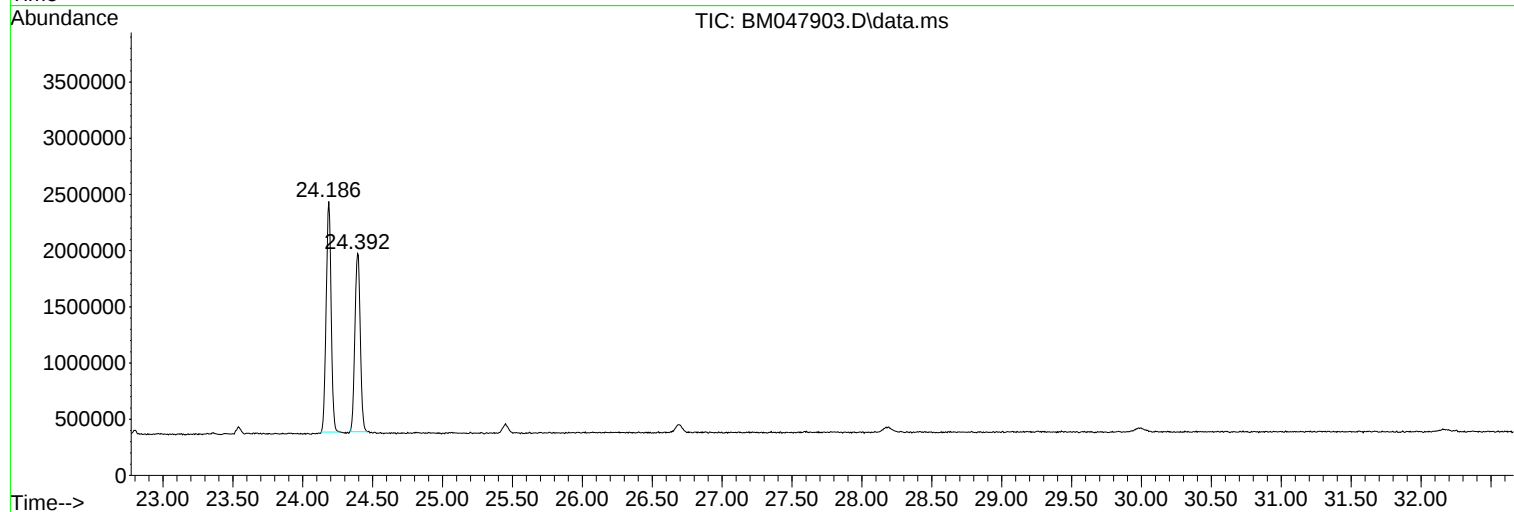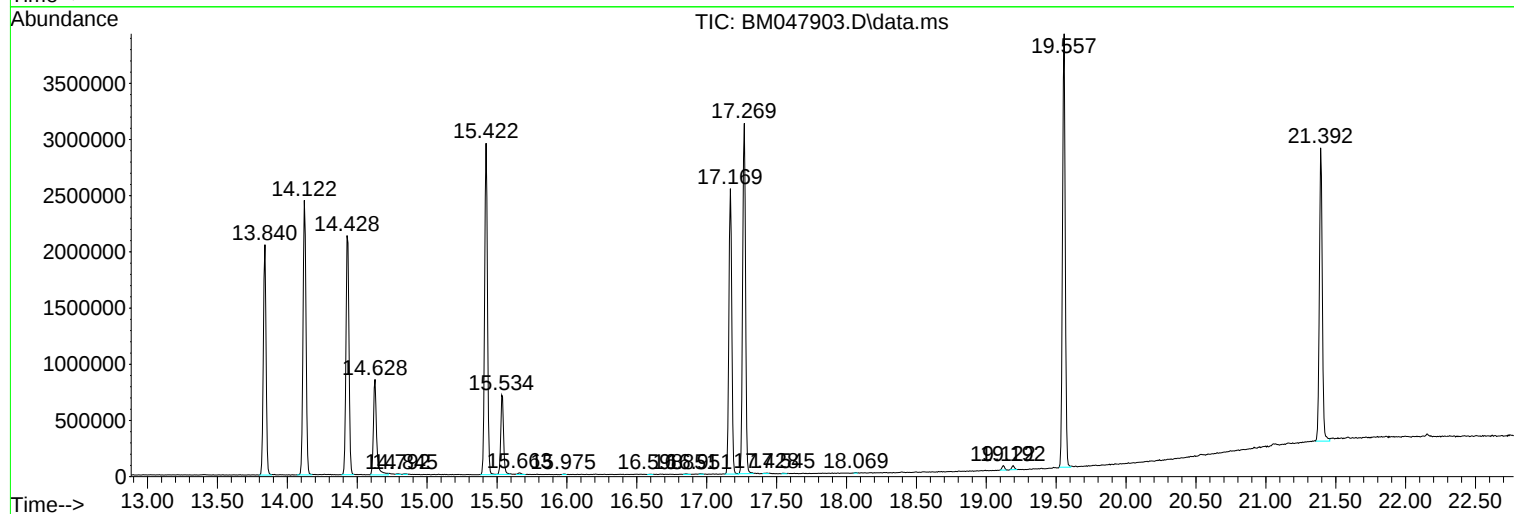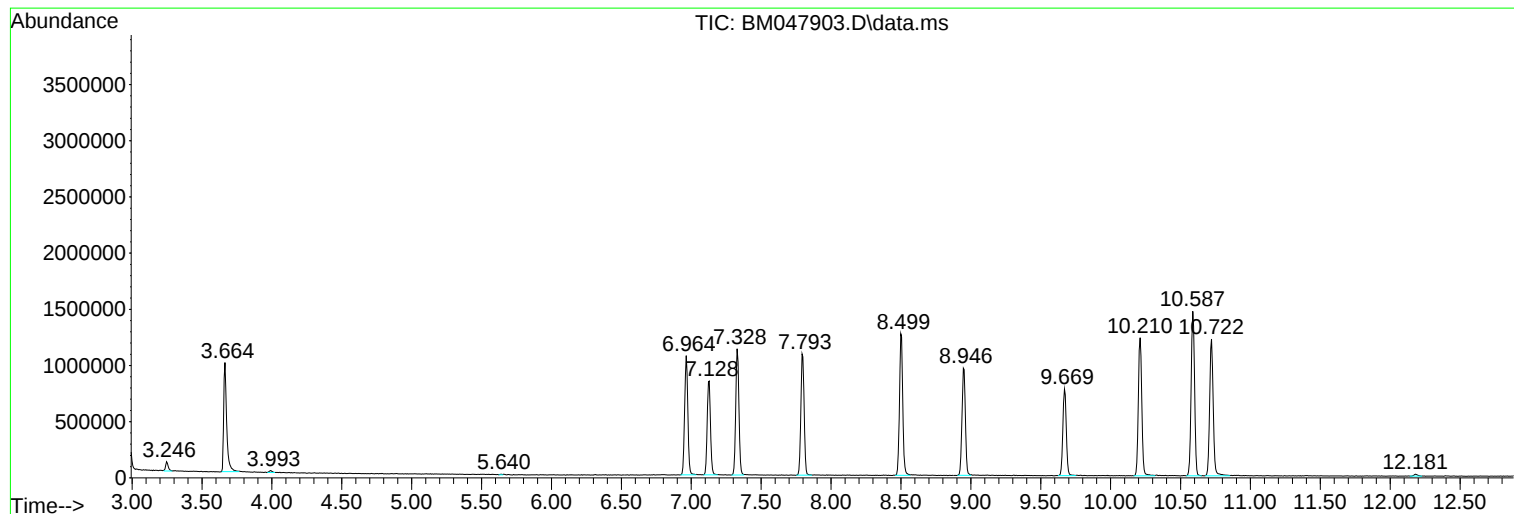

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047903.D
Acq On : 08 Oct 2024 04:17
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047903.D
Acq On : 08 Oct 2024 04:17
Operator : RC/JU
Sample : PB163648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc