

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047910.D
 Acq On : 08 Oct 2024 08:54
 Operator : RC/JU
 Sample : P4131-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4EX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	52	rVB	40959	55513	1.21%	0.111%
2	3.663	112	115	129	rBV	407781	672190	14.70%	1.349%
3	3.993	167	171	177	rVB2	21456	34317	0.75%	0.069%
4	6.022	514	516	520	rBV4	4036	5142	0.11%	0.010%
5	6.963	669	676	686	rBV	617097	1005677	21.99%	2.018%
6	7.122	697	703	717	rVB	485928	781899	17.10%	1.569%
7	7.328	732	738	748	rBV	638607	1004382	21.97%	2.015%
8	7.792	810	817	825	rBV	1155912	1872471	40.95%	3.757%
9	7.863	825	829	833	rVB7	8056	12798	0.28%	0.026%
10	8.357	911	913	918	rVB6	3047	4663	0.10%	0.009%
11	8.498	931	937	948	rBV	753722	1231660	26.94%	2.471%
12	8.945	1006	1013	1022	rBV	558980	925903	20.25%	1.858%
13	9.122	1040	1043	1045	rBV4	4871	4790	0.10%	0.010%
14	9.381	1084	1087	1092	rVB5	7681	13034	0.29%	0.026%
15	9.516	1104	1110	1117	rVB2	43287	75762	1.66%	0.152%
16	9.669	1126	1136	1146	rBV	448296	757806	16.57%	1.521%
17	9.910	1174	1177	1181	rBV5	3632	5343	0.12%	0.011%
18	10.210	1220	1228	1243	rBV	745858	1269885	27.77%	2.548%
19	10.586	1284	1292	1302	rBV	1595756	2663726	58.25%	5.345%
20	10.722	1307	1315	1325	rBV	694714	1242096	27.16%	2.492%
21	11.133	1380	1385	1394	rVB8	14374	31020	0.68%	0.062%
22	11.339	1415	1420	1422	rBV6	2842	4713	0.10%	0.009%
23	12.174	1557	1562	1568	rBV2	12316	24378	0.53%	0.049%
24	13.039	1706	1709	1713	rBV6	3279	5532	0.12%	0.011%
25	13.121	1720	1723	1727	rBV4	7232	10908	0.24%	0.022%
26	13.204	1732	1737	1742	rVV7	15020	25182	0.55%	0.051%
27	13.263	1744	1747	1752	rVV5	11723	17372	0.38%	0.035%
28	13.763	1827	1832	1838	rVV7	6805	12726	0.28%	0.026%
29	13.839	1838	1845	1855	rVV	1261792	1778217	38.89%	3.568%
30	13.921	1857	1859	1862	rVV4	4258	4708	0.10%	0.009%
31	13.963	1862	1866	1872	rVB7	7179	11214	0.25%	0.023%
32	14.121	1884	1893	1904	rBV	1502610	2236270	48.91%	4.487%
33	14.274	1913	1919	1924	rBV3	31366	48656	1.06%	0.098%
34	14.333	1926	1929	1934	rVB7	6463	10768	0.24%	0.022%
35	14.427	1939	1945	1955	rVV	2336917	3438944	75.21%	6.900%
36	14.498	1955	1957	1963	rVB7	10721	15765	0.34%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047910.D
 Acq On : 08 Oct 2024 08:54
 Operator : RC/JU
 Sample : P4131-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4EX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	14.627	1972	1979	1985	rBV	420251	683200	14.94%	1.371%
38	14.686	1985	1989	1997	rVV	51305	102953	2.25%	0.207%
39	14.751	1997	2000	2006	rVB2	10935	18741	0.41%	0.038%
40	14.851	2013	2017	2022	rVB6	9399	16274	0.36%	0.033%
41	14.963	2033	2036	2041	rVB6	4914	5735	0.13%	0.012%
42	15.274	2086	2089	2093	rBV6	2806	5002	0.11%	0.010%
43	15.421	2106	2114	2123	rBV	1932229	2760459	60.37%	5.539%
44	15.533	2126	2133	2145	rVV	353036	515055	11.26%	1.033%
45	15.657	2150	2154	2162	rVB8	11340	22646	0.50%	0.045%
46	15.786	2168	2176	2183	rBV	747637	1026029	22.44%	2.059%
47	15.998	2206	2212	2217	rBV9	6672	15175	0.33%	0.030%
48	16.139	2235	2236	2244	rVB7	3972	6293	0.14%	0.013%
49	16.351	2267	2272	2278	rVB5	15477	24963	0.55%	0.050%
50	16.962	2371	2376	2378	rVB4	6076	9849	0.22%	0.020%
51	17.092	2394	2398	2401	rVB5	6045	7929	0.17%	0.016%
52	17.168	2404	2411	2417	rBV	2783754	3929283	85.93%	7.884%
53	17.262	2422	2427	2438	rVV	1886699	2867316	62.71%	5.753%
54	17.351	2438	2442	2447	rVB8	12680	23368	0.51%	0.047%
55	17.539	2471	2474	2478	rBV5	8408	12670	0.28%	0.025%
56	17.774	2510	2514	2518	rVB5	18555	26903	0.59%	0.054%
57	17.839	2523	2525	2529	rVB5	8620	10289	0.23%	0.021%
58	17.880	2529	2532	2537	rBV7	6769	13245	0.29%	0.027%
59	18.062	2558	2563	2572	rBV	225305	343714	7.52%	0.690%
60	18.239	2590	2593	2596	rVV5	13960	16463	0.36%	0.033%
61	18.298	2600	2603	2606	rVB5	12625	15523	0.34%	0.031%
62	18.521	2638	2641	2643	rBV3	15113	17242	0.38%	0.035%
63	18.915	2704	2708	2712	rBV5	16329	25879	0.57%	0.052%
64	19.121	2740	2743	2747	rVB4	26189	35532	0.78%	0.071%
65	19.192	2751	2755	2758	rBV	34399	54734	1.20%	0.110%
66	19.333	2776	2779	2788	rBV5	48774	89433	1.96%	0.179%
67	19.556	2811	2817	2824	rBV	2566247	3460339	75.68%	6.943%
68	21.068	3070	3074	3083	rBV2	266323	401691	8.78%	0.806%
69	21.392	3124	3129	3140	rBV	2790852	4158221	90.94%	8.344%
70	24.185	3596	3604	3614	rVB2	1314773	3226396	70.56%	6.474%
71	24.391	3631	3639	3652	rVB	1787957	4572618	100.00%	9.175%




Sum of corrected areas: 49836592

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047910.D
Acq On : 08 Oct 2024 08:54
Operator : RC/JU
Sample : P4131-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4EX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

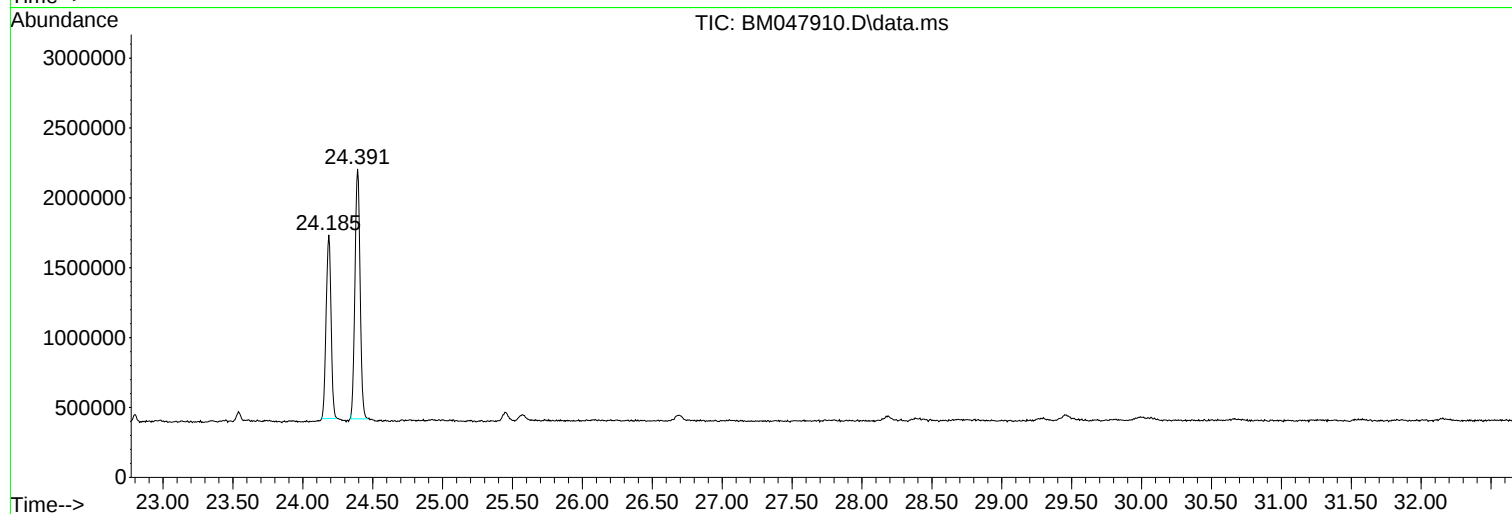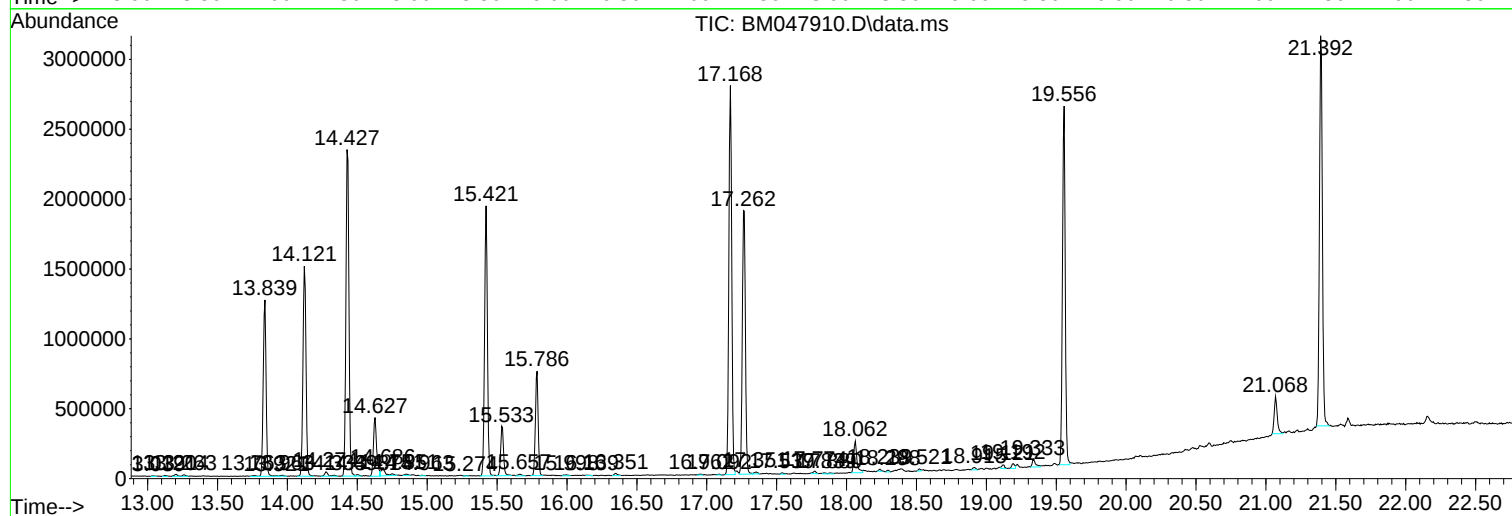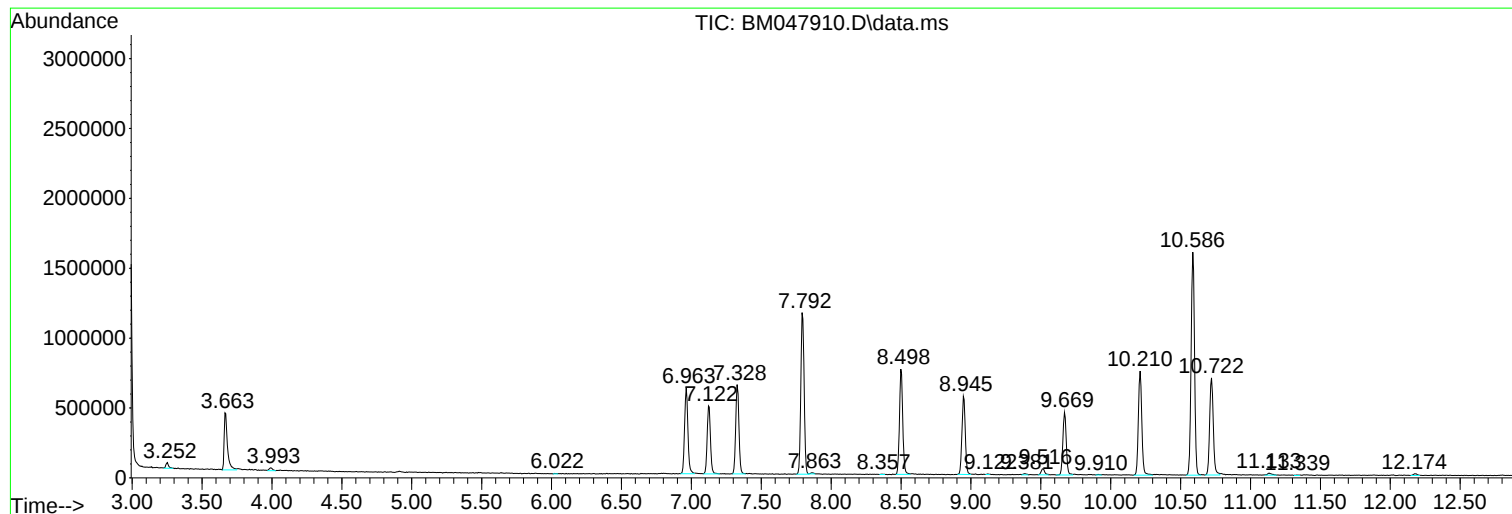

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047910.D
Acq On : 08 Oct 2024 08:54
Operator : RC/JU
Sample : P4131-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4EX9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.786	5.97 ng/ul	1026030	Acenaphthene-d10	14.427

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	94
4			Benzophenone	182	C13H10O	000119-61-9	93
5			Benzeneacetic acid, .alpha.-oxo-...	164	C9H8O3	015206-55-0	53

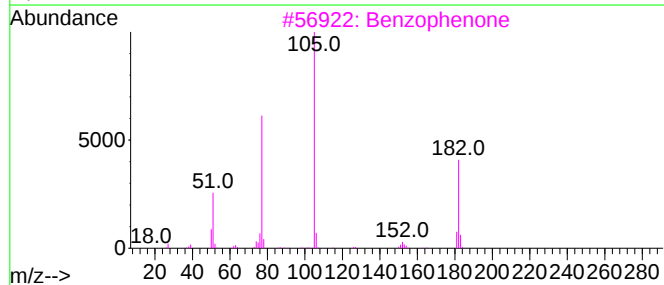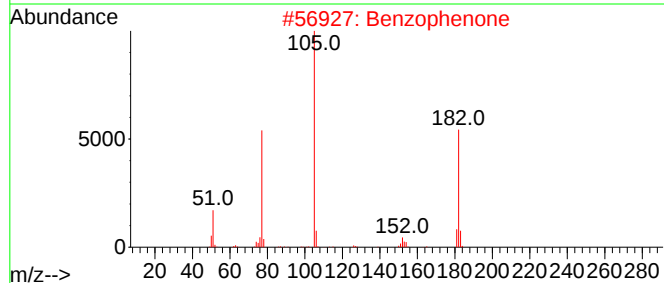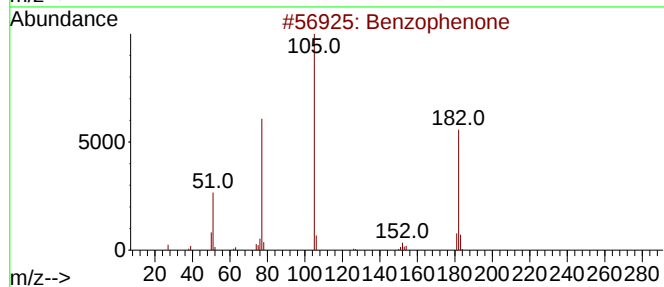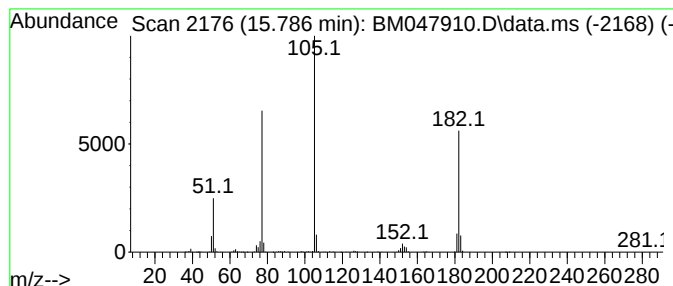

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047910.D
Acq On : 08 Oct 2024 08:54
Operator : RC/JU
Sample : P4131-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4EX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.786	6.0	ng/ul	1026030	3	14.427	3438940	20.0