

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047914.D
 Acq On : 08 Oct 2024 15:08
 Operator : RC/JU
 Sample : P4109-17
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4ET9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	42	45	50	rVB3	18944	28283	0.63%	0.069%
2	3.681	114	118	122	rBV5	22498	35158	0.78%	0.085%
3	3.769	130	133	138	rVB2	29942	38366	0.86%	0.093%
4	3.993	168	171	177	rVB	20027	25981	0.58%	0.063%
5	4.904	321	326	333	rBV	30557	51354	1.15%	0.125%
6	6.963	668	676	686	rBV	473100	794131	17.71%	1.926%
7	7.122	697	703	712	rBV	385000	604490	13.48%	1.466%
8	7.328	732	738	749	rBV	487637	768105	17.13%	1.863%
9	7.416	751	753	757	rVB4	7049	8965	0.20%	0.022%
10	7.792	810	817	826	rBV	1145337	1826601	40.73%	4.429%
11	7.863	826	829	837	rVB9	7215	13718	0.31%	0.033%
12	8.498	930	937	947	rBV	521555	849548	18.94%	2.060%
13	8.616	951	957	964	rVB	80634	140104	3.12%	0.340%
14	8.945	1005	1013	1024	rBV	427331	714254	15.93%	1.732%
15	9.116	1037	1042	1047	rVB9	7090	10338	0.23%	0.025%
16	9.386	1083	1088	1093	rVB4	8218	13417	0.30%	0.033%
17	9.516	1104	1110	1116	rBV3	28600	49253	1.10%	0.119%
18	9.669	1129	1136	1147	rBV	326471	556345	12.41%	1.349%
19	9.822	1156	1162	1167	rBV6	10183	21376	0.48%	0.052%
20	10.028	1191	1197	1204	rVB7	9043	17920	0.40%	0.043%
21	10.210	1220	1228	1239	rBV	551676	954255	21.28%	2.314%
22	10.586	1285	1292	1299	rBV	1534112	2594543	57.86%	6.292%
23	10.722	1307	1315	1331	rBV	365370	693943	15.47%	1.683%
24	11.127	1380	1384	1389	rBV7	11337	18614	0.42%	0.045%
25	11.375	1425	1426	1433	rVB7	6733	8871	0.20%	0.022%
26	13.757	1827	1831	1833	rBV4	7381	10030	0.22%	0.024%
27	13.833	1838	1844	1855	rVB	907055	1319975	29.43%	3.201%
28	14.121	1886	1893	1905	rBV	1118127	1638861	36.55%	3.974%
29	14.427	1937	1945	1952	rBV	2309716	3335266	74.38%	8.088%
30	14.492	1952	1956	1964	rVB5	16691	28264	0.63%	0.069%
31	14.627	1972	1979	1986	rBV	289513	486705	10.85%	1.180%
32	14.745	1996	1999	2003	rBV3	7962	12065	0.27%	0.029%
33	14.839	2011	2015	2022	rVB7	13237	23595	0.53%	0.057%
34	15.086	2052	2057	2061	rBV8	4485	9131	0.20%	0.022%
35	15.221	2075	2080	2086	rBV9	14562	25796	0.58%	0.063%
36	15.421	2107	2114	2120	rBV	1405327	2060863	45.96%	4.997%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047914.D
 Acq On : 08 Oct 2024 15:08
 Operator : RC/JU
 Sample : P4109-17
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4ET9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	15.474	2120	2123	2128	rVV4	16003	23287	0.52%	0.056%
38	15.533	2128	2133	2141	rVB	267771	377046	8.41%	0.914%
39	15.662	2148	2155	2156	rBV6	7541	13172	0.29%	0.032%
40	15.780	2170	2175	2181	rVB	190352	271191	6.05%	0.658%
41	16.145	2233	2237	2243	rVB9	10612	20816	0.46%	0.050%
42	16.521	2297	2301	2306	rVB7	7770	11901	0.27%	0.029%
43	16.709	2329	2333	2336	rVB6	8350	13544	0.30%	0.033%
44	16.821	2348	2352	2359	rBV4	10341	16545	0.37%	0.040%
45	17.168	2404	2411	2416	rBV	2747140	3832149	85.46%	9.293%
46	17.209	2416	2418	2422	rVV	171506	202433	4.51%	0.491%
47	17.262	2422	2427	2438	rVV	1439234	2140422	47.73%	5.190%
48	17.345	2439	2441	2448	rVB8	11742	25190	0.56%	0.061%
49	17.574	2478	2480	2484	rVB4	15067	13263	0.30%	0.032%
50	18.015	2550	2555	2557	rBV2	25016	39554	0.88%	0.096%
51	18.056	2557	2562	2566	rBV2	118708	185479	4.14%	0.450%
52	18.239	2588	2593	2596	rBV3	45758	71751	1.60%	0.174%
53	18.468	2629	2632	2637	rBV	46004	60781	1.36%	0.147%
54	18.780	2683	2685	2690	rVB5	26840	31685	0.71%	0.077%
55	18.998	2719	2722	2730	rBV10	48293	76985	1.72%	0.187%
56	19.221	2755	2760	2766	rVB	333507	442372	9.86%	1.073%
57	19.280	2767	2770	2774	rVB3	49505	58669	1.31%	0.142%
58	19.339	2777	2780	2783	rBV4	27585	31437	0.70%	0.076%
59	19.550	2811	2816	2830	rBV2	1640217	2624638	58.53%	6.365%
60	21.392	3123	3129	3134	rBV2	2671429	4157717	92.72%	10.082%
61	22.156	3256	3259	3264	rBV	153624	210192	4.69%	0.510%
62	23.544	3491	3495	3501	rVB	242345	445984	9.95%	1.081%
63	24.185	3597	3604	3613	rVB	665507	1566936	34.94%	3.800%
64	24.397	3631	3640	3653	rVB	1699393	4484388	100.00%	10.874%




Sum of corrected areas: 41238011

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047914.D
Acq On : 08 Oct 2024 15:08
Operator : RC/JU
Sample : P4109-17
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4ET9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

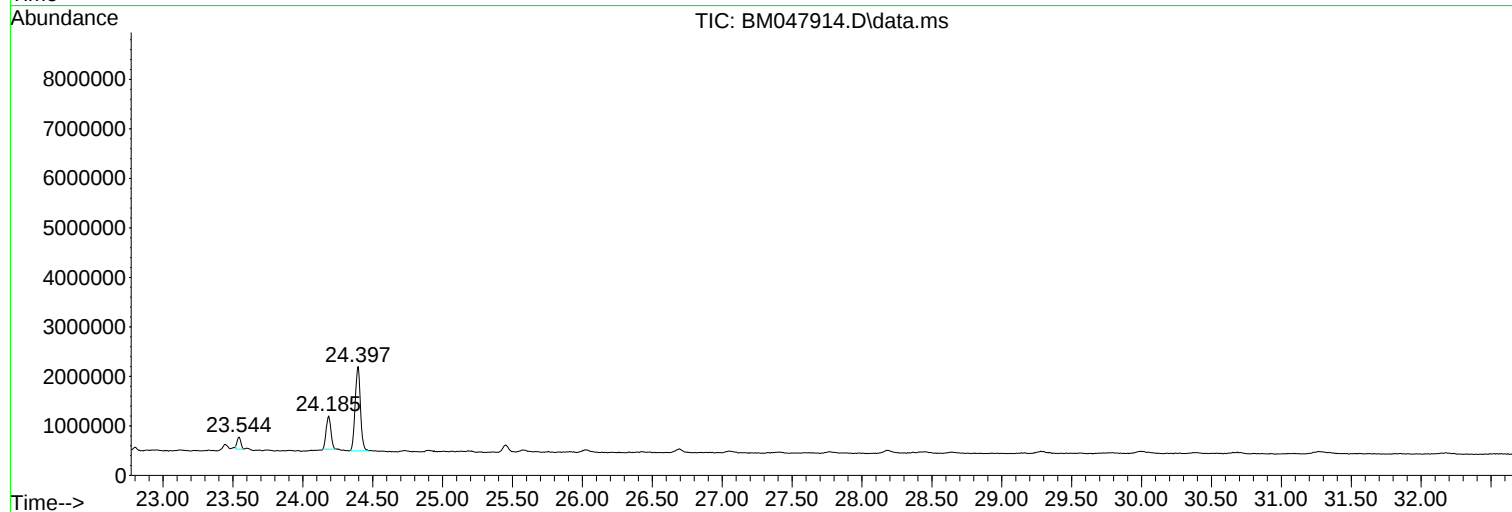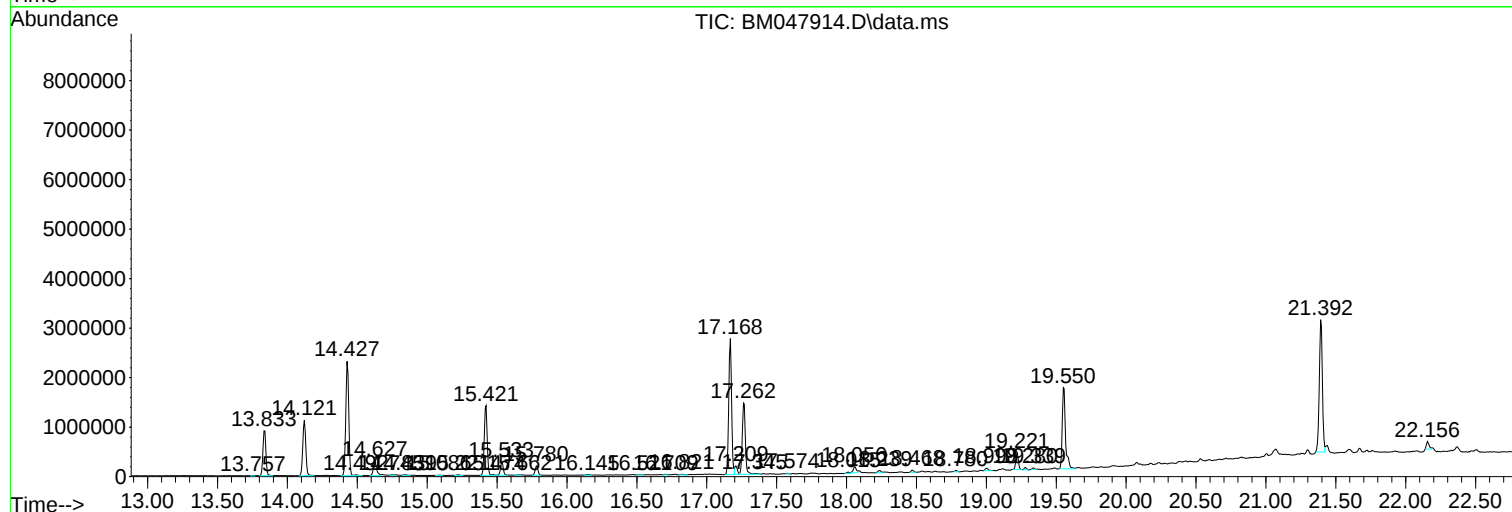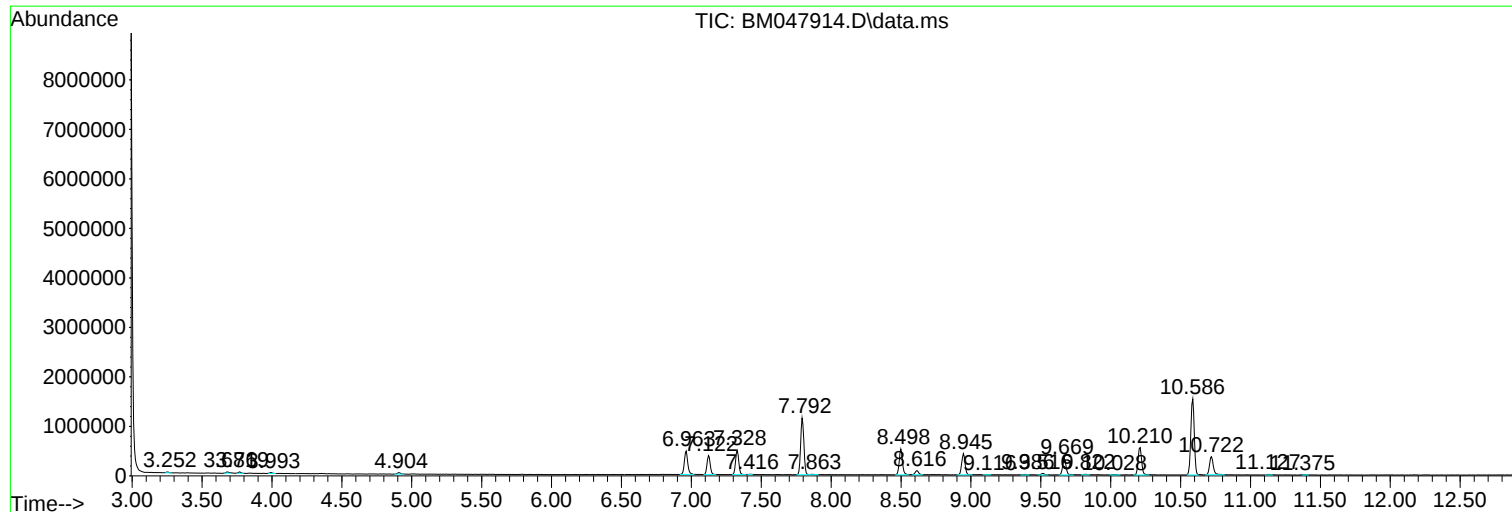

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047914.D
Acq On : 08 Oct 2024 15:08
Operator : RC/JU
Sample : P4109-17
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4ET9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047914.D
Acq On : 08 Oct 2024 15:08
Operator : RC/JU
Sample : P4109-17
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4ET9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------