

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047917.D
 Acq On : 08 Oct 2024 17:46
 Operator : RC/JU
 Sample : PB163712BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK712

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	52	rVB	64708	93031	2.22%	0.179%
2	3.663	112	115	130	rBV	751555	1204455	28.71%	2.316%
3	3.993	168	171	176	rVB	18709	26597	0.63%	0.051%
4	5.316	393	396	398	rBV3	4986	4958	0.12%	0.010%
5	6.963	669	676	687	rBV	858833	1354634	32.29%	2.605%
6	7.122	697	703	712	rBV	684561	1099090	26.20%	2.114%
7	7.328	731	738	750	rBV	895976	1411374	33.64%	2.714%
8	7.792	810	817	825	rBV	987917	1569557	37.41%	3.019%
9	8.498	929	937	955	rBV	1028918	1679022	40.02%	3.229%
10	8.798	985	988	991	rBV4	3908	5005	0.12%	0.010%
11	8.945	1006	1013	1022	rBV	770416	1290041	30.75%	2.481%
12	9.380	1082	1087	1092	rVV6	9981	16148	0.38%	0.031%
13	9.445	1096	1098	1101	rVB3	4295	4232	0.10%	0.008%
14	9.669	1129	1136	1144	rBV	626997	1031494	24.59%	1.984%
15	10.210	1220	1228	1241	rBV	980849	1657713	39.51%	3.188%
16	10.586	1284	1292	1300	rBV	1299035	2212890	52.75%	4.256%
17	10.722	1306	1315	1335	rBV	953232	1713370	40.84%	3.295%
18	11.880	1507	1512	1515	rBV5	7454	10988	0.26%	0.021%
19	12.186	1559	1564	1571	rVB5	11982	25382	0.60%	0.049%
20	12.798	1665	1668	1671	rBV4	2724	4249	0.10%	0.008%
21	13.310	1751	1755	1759	rVB5	3066	4989	0.12%	0.010%
22	13.839	1838	1845	1855	rBV	1581671	2256463	53.78%	4.340%
23	14.121	1886	1893	1901	rBV	1923727	2808053	66.93%	5.400%
24	14.427	1938	1945	1955	rBV	1904719	2807778	66.92%	5.400%
25	14.627	1972	1979	1994	rBV	596605	1026016	24.46%	1.973%
26	14.786	2004	2006	2012	rVB7	3578	5202	0.12%	0.010%
27	15.421	2106	2114	2122	rBV	2328578	3387011	80.73%	6.514%
28	15.533	2128	2133	2144	rBV	607627	839133	20.00%	1.614%
29	15.662	2151	2155	2159	rVB5	11968	19634	0.47%	0.038%
30	15.815	2179	2181	2185	rBV5	3474	5119	0.12%	0.010%
31	15.980	2207	2209	2212	rBV3	4615	4985	0.12%	0.010%
32	16.198	2245	2246	2250	rVB4	3569	4327	0.10%	0.008%
33	17.104	2397	2400	2404	rBV4	2933	4224	0.10%	0.008%
34	17.168	2404	2411	2420	rBV	2379408	3204345	76.38%	6.163%
35	17.268	2421	2428	2443	rVB	2583160	3669494	87.46%	7.057%
36	19.121	2739	2743	2749	rBV2	31381	41275	0.98%	0.079%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047917.D
Acq On : 08 Oct 2024 17:46
Operator : RC/JU
Sample : PB163712BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK712

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	19.192	2752	2755	2761	rVB	27274	36996	0.88%	0.071%
38	19.556	2811	2817	2827	rBV	3182220	4195447	100.00%	8.069%
39	21.391	3124	3129	3142	rBV	2278997	3383657	80.65%	6.507%
40	24.185	3596	3604	3618	rVB	1682105	4192242	99.92%	8.063%
41	24.391	3631	3639	3652	rVB	1421944	3685737	87.85%	7.088%




Sum of corrected areas: 51996357

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047917.D
Acq On : 08 Oct 2024 17:46
Operator : RC/JU
Sample : PB163712BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK712

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

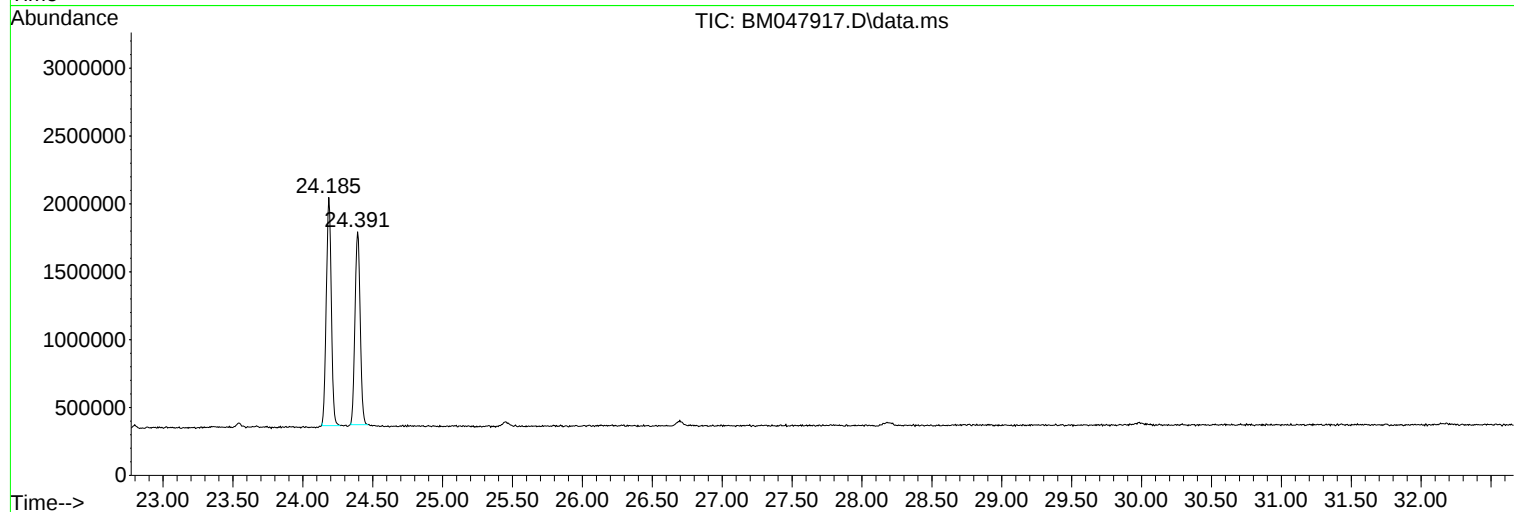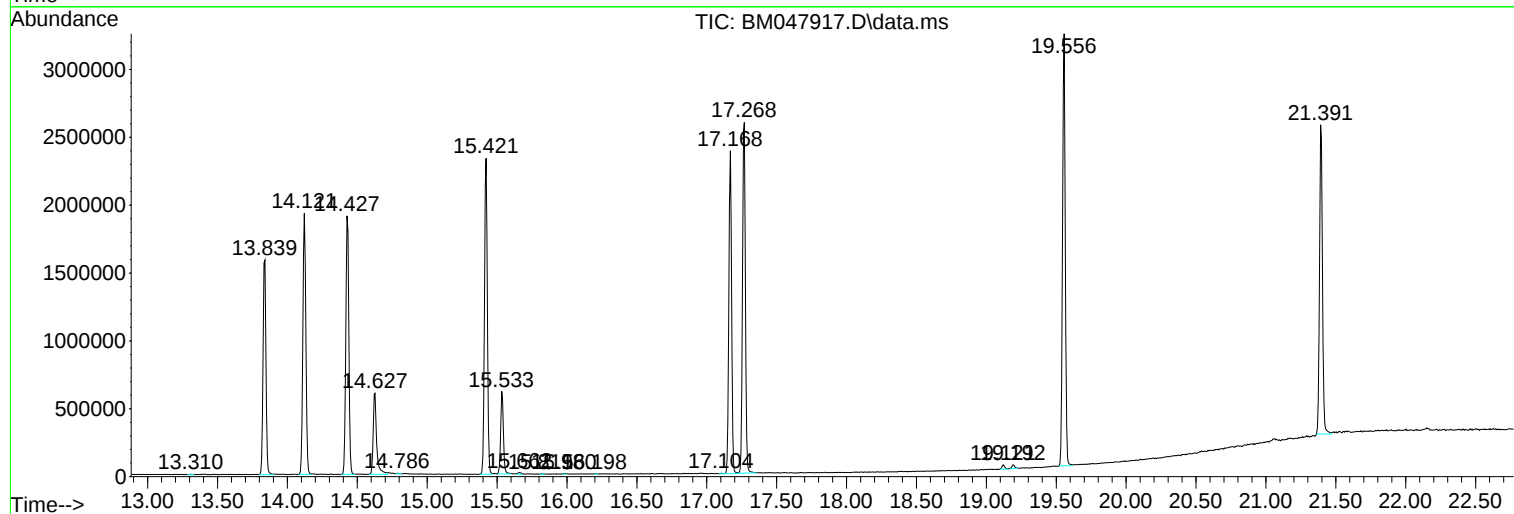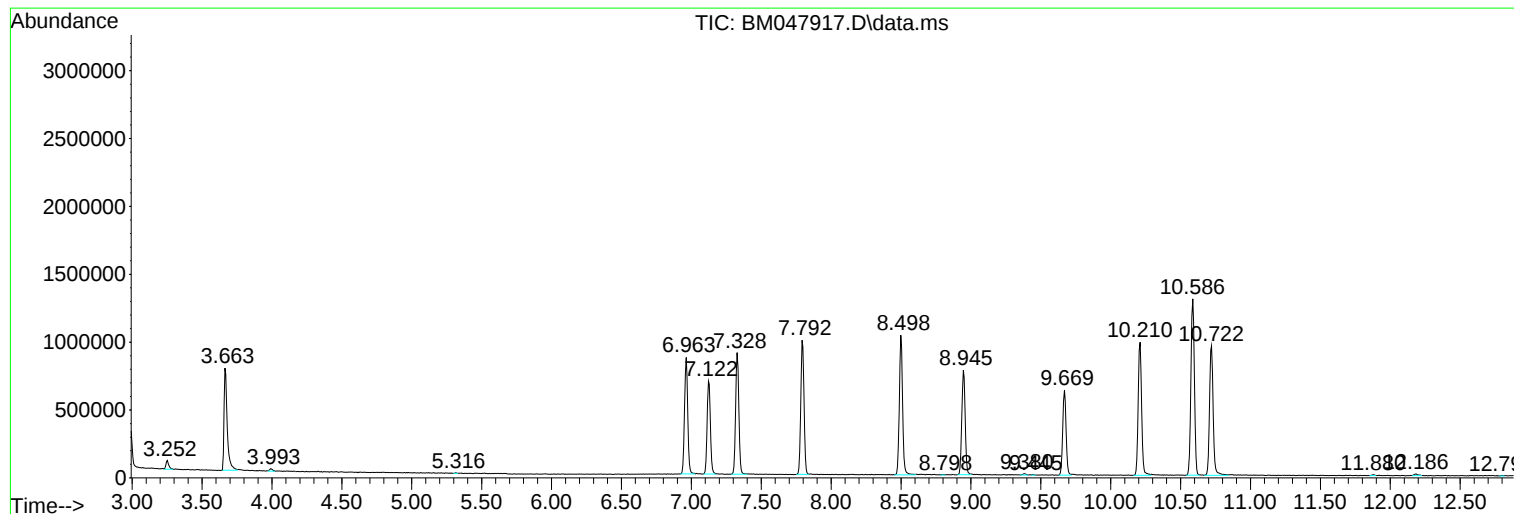

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047917.D
Acq On : 08 Oct 2024 17:46
Operator : RC/JU
Sample : PB163712BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK712

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047917.D
Acq On : 08 Oct 2024 17:46
Operator : RC/JU
Sample : PB163712BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK712

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------