

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047932.D
 Acq On : 09 Oct 2024 04:17
 Operator : RC/JU
 Sample : PB163712BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK712

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	49	rVB	67902	83384	1.93%	0.161%
2	3.663	111	115	131	rBV	772158	1204533	27.91%	2.324%
3	3.987	166	170	175	rVB2	17844	26221	0.61%	0.051%
4	6.963	669	676	683	rBV	832691	1345420	31.18%	2.595%
5	7.122	697	703	712	rVB	680407	1073049	24.87%	2.070%
6	7.328	730	738	748	rBV	877492	1405143	32.56%	2.711%
7	7.792	810	817	825	rBV	945465	1507449	34.93%	2.908%
8	7.857	827	828	833	rBV4	3683	4642	0.11%	0.009%
9	8.498	930	937	948	rBV	1043385	1649133	38.21%	3.181%
10	8.745	976	979	984	rBV6	3192	5006	0.12%	0.010%
11	8.945	1006	1013	1023	rBV	786945	1291038	29.92%	2.490%
12	9.386	1085	1088	1091	rVB3	5793	6189	0.14%	0.012%
13	9.669	1128	1136	1145	rBV	611258	1017751	23.58%	1.963%
14	9.745	1147	1149	1152	rVB3	5051	4451	0.10%	0.009%
15	10.204	1218	1227	1238	rBV	958093	1643278	38.08%	3.170%
16	10.281	1238	1240	1244	rVB5	5406	5622	0.13%	0.011%
17	10.586	1283	1292	1301	rBV	1264508	2111088	48.92%	4.072%
18	10.716	1308	1314	1333	rBV	916759	1673114	38.77%	3.227%
19	11.875	1506	1511	1515	rBV6	6163	7368	0.17%	0.014%
20	12.180	1556	1563	1570	rBV4	13729	27818	0.64%	0.054%
21	13.686	1817	1819	1823	rBV4	2956	4345	0.10%	0.008%
22	13.833	1838	1844	1854	rBV	1588110	2241750	51.95%	4.324%
23	14.121	1886	1893	1902	rBV	1935783	2814340	65.22%	5.429%
24	14.427	1938	1945	1954	rBV	1895571	2707914	62.75%	5.224%
25	14.621	1971	1978	2003	rBV	595698	1082573	25.09%	2.088%
26	14.839	2011	2015	2019	rVB6	3273	6212	0.14%	0.012%
27	15.421	2106	2114	2121	rBV	2366045	3413389	79.10%	6.584%
28	15.468	2121	2122	2126	rVB4	4679	5672	0.13%	0.011%
29	15.533	2126	2133	2146	rBV	617005	857717	19.88%	1.655%
30	15.663	2151	2155	2159	rVB5	12880	19355	0.45%	0.037%
31	16.668	2321	2326	2329	rVB7	4001	6695	0.16%	0.013%
32	16.957	2371	2375	2382	rVB4	4699	7315	0.17%	0.014%
33	17.168	2404	2411	2420	rBV	2106061	3113196	72.14%	6.005%
34	17.262	2420	2427	2440	rVV2	2553690	3728351	86.40%	7.192%
35	19.121	2739	2743	2748	rVB4	30621	39357	0.91%	0.076%
36	19.192	2751	2755	2760	rBV2	30660	41613	0.96%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047932.D
Acq On : 09 Oct 2024 04:17
Operator : RC/JU
Sample : PB163712BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK712

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	19.551	2810	2816	2824	rBV	3202278	4314677	99.98%	8.323%
38	21.392	3123	3129	3138	rBV	2214796	3388524	78.52%	6.537%
39	24.180	3595	3603	3616	rVB	1813029	4315423	100.00%	8.325%
40	24.385	3630	3638	3651	rVB	1441116	3639659	84.34%	7.021%




Sum of corrected areas: 51839774

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047932.D
Acq On : 09 Oct 2024 04:17
Operator : RC/JU
Sample : PB163712BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK712

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

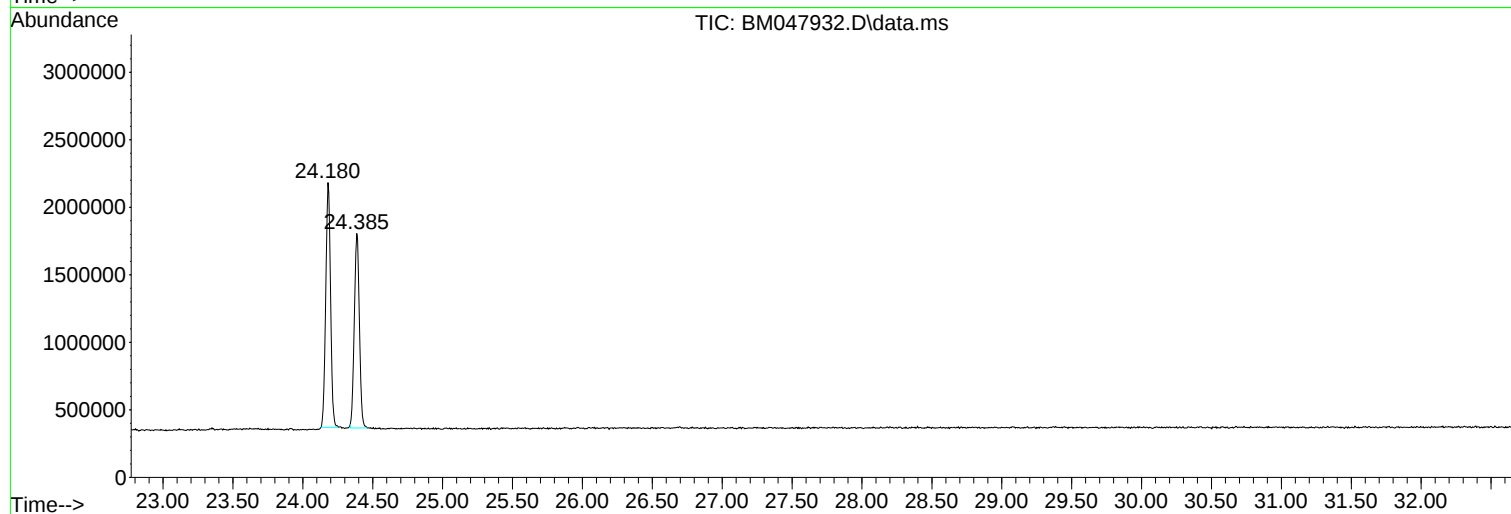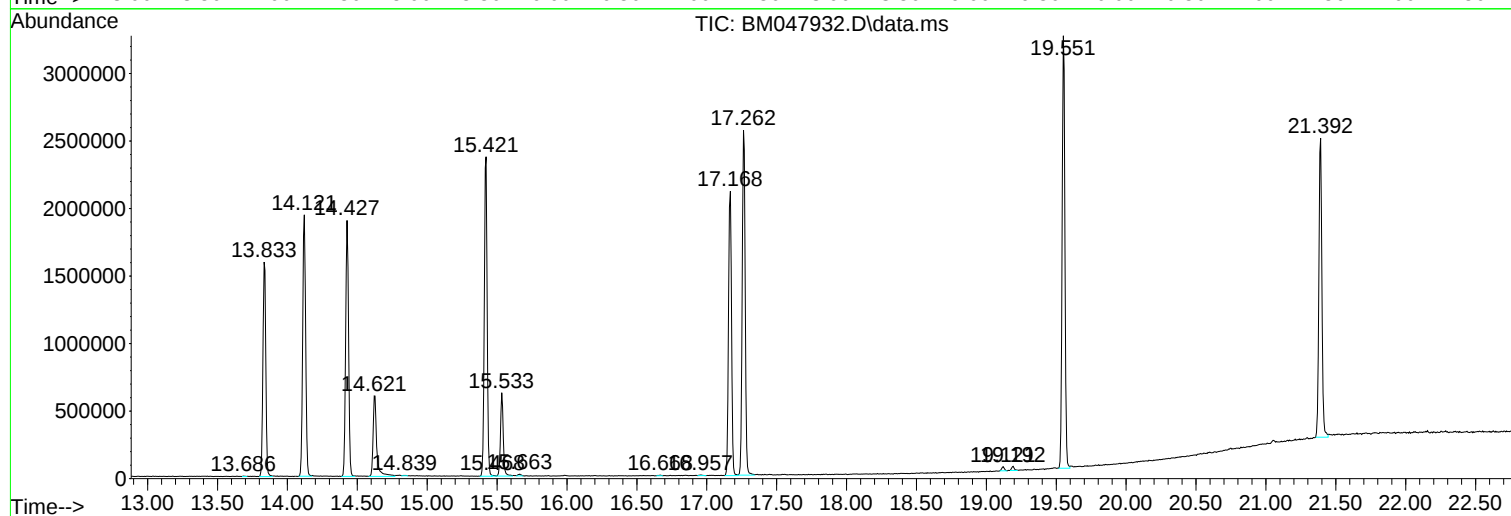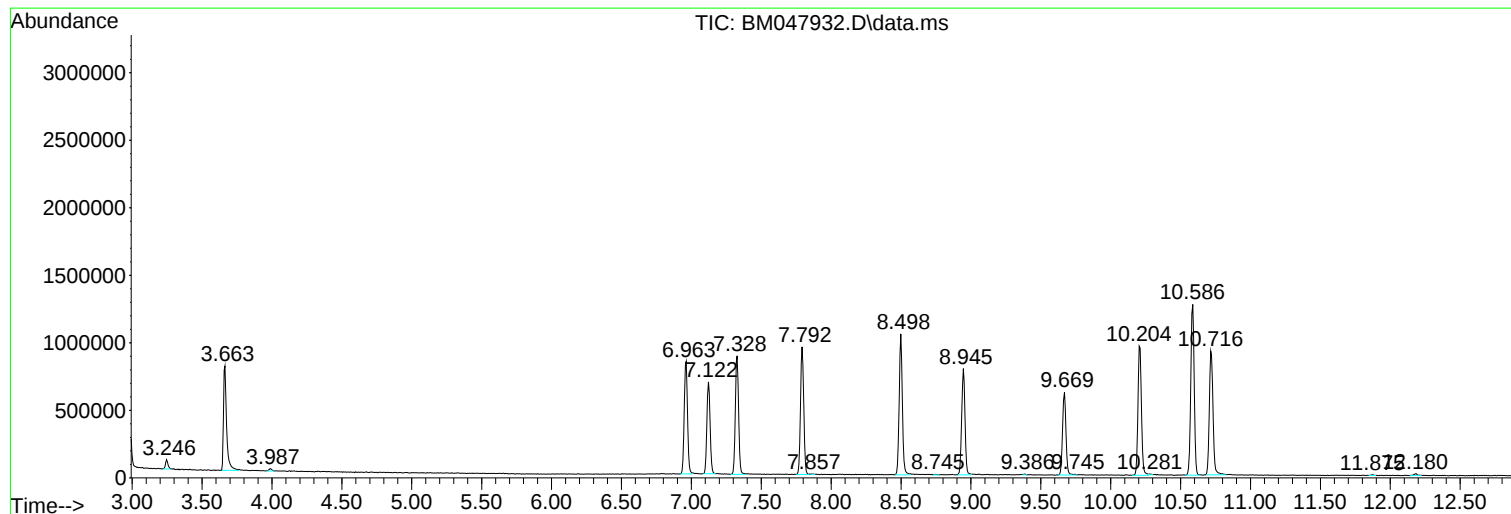

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047932.D
Acq On : 09 Oct 2024 04:17
Operator : RC/JU
Sample : PB163712BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK712

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047932.D
Acq On : 09 Oct 2024 04:17
Operator : RC/JU
Sample : PB163712BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK712

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc