

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
 Data File : BM047939.D
 Acq On : 09 Oct 2024 08:53
 Operator : RC/JU
 Sample : SP6637
 Misc : SFAM SURROGATES
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP6637

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	52	rVB	217305	288295	1.95%	0.196%
2	3.663	110	115	137	rVB	2772205	4323645	29.31%	2.937%
3	3.993	168	171	179	rVB3	20464	28858	0.20%	0.020%
4	6.969	669	677	687	rBV	3055771	4915787	33.33%	3.339%
5	7.128	696	704	715	rVB	2572639	3977752	26.97%	2.702%
6	7.328	731	738	748	rBV	3181192	5103452	34.60%	3.466%
7	7.792	810	817	827	rBV	1066735	1722566	11.68%	1.170%
8	8.504	930	938	950	rBV	3821801	6168379	41.82%	4.190%
9	8.951	1006	1014	1028	rBV	2938441	4863652	32.97%	3.303%
10	9.669	1128	1136	1146	rBV	2403685	4056385	27.50%	2.755%
11	10.210	1220	1228	1240	rBV	3703683	6203250	42.06%	4.213%
12	10.586	1285	1292	1300	rBV	1462691	2458861	16.67%	1.670%
13	10.722	1306	1315	1329	rBV	3783200	6409310	43.45%	4.353%
14	12.175	1557	1562	1568	rVB2	65411	103846	0.70%	0.071%
15	13.398	1765	1770	1775	rVB3	9500	16168	0.11%	0.011%
16	13.839	1836	1845	1855	rBV	5599373	7944392	53.86%	5.396%
17	14.121	1886	1893	1905	rBV	6759178	10513035	71.28%	7.141%
18	14.427	1937	1945	1953	rBV	2178654	3201740	21.71%	2.175%
19	14.516	1956	1960	1966	rBV9	10389	17597	0.12%	0.012%
20	14.633	1973	1980	2000	rBV	2921841	4502433	30.53%	3.058%
21	14.786	2004	2006	2012	rVV6	13586	23700	0.16%	0.016%
22	14.839	2012	2015	2019	rVB4	9160	15474	0.10%	0.011%
23	15.421	2106	2114	2126	rBV	8442096	12210009	82.78%	8.293%
24	15.539	2127	2134	2149	rVV	2559516	3575949	24.24%	2.429%
25	15.663	2150	2155	2161	rVB	46651	75547	0.51%	0.051%
26	15.992	2208	2211	2217	rVB6	12439	18796	0.13%	0.013%
27	16.198	2242	2246	2250	rVB6	11903	16308	0.11%	0.011%
28	16.851	2353	2357	2361	rVB5	12231	17723	0.12%	0.012%
29	17.168	2403	2411	2421	rBV	2652768	3677451	24.93%	2.498%
30	17.268	2421	2428	2436	rBV2	8673040	12986939	88.05%	8.821%
31	17.415	2448	2453	2463	rBV2	50717	103499	0.70%	0.070%
32	17.545	2472	2475	2483	rVB3	13075	26081	0.18%	0.018%
33	19.121	2738	2743	2749	rBV3	127496	181656	1.23%	0.123%
34	19.192	2750	2755	2760	rBV	142937	201313	1.36%	0.137%
35	19.556	2811	2817	2826	rBV	10281176	14749610	100.00%	10.018%
36	21.397	3124	3130	3138	rBV	2568261	3866182	26.21%	2.626%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047939.D
Acq On : 09 Oct 2024 08:53
Operator : RC/JU
Sample : SP6637
Misc : SFAM SURROGATES
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6637

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	24.197	3596	3606	3619	rVB	5652913	14481982	98.19%	9.836%
38	24.397	3632	3640	3650	rVB	1623279	4180119	28.34%	2.839%




Sum of corrected areas: 147227741

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047939.D
Acq On : 09 Oct 2024 08:53
Operator : RC/JU
Sample : SP6637
Misc : SFAM SURROGATES
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6637

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

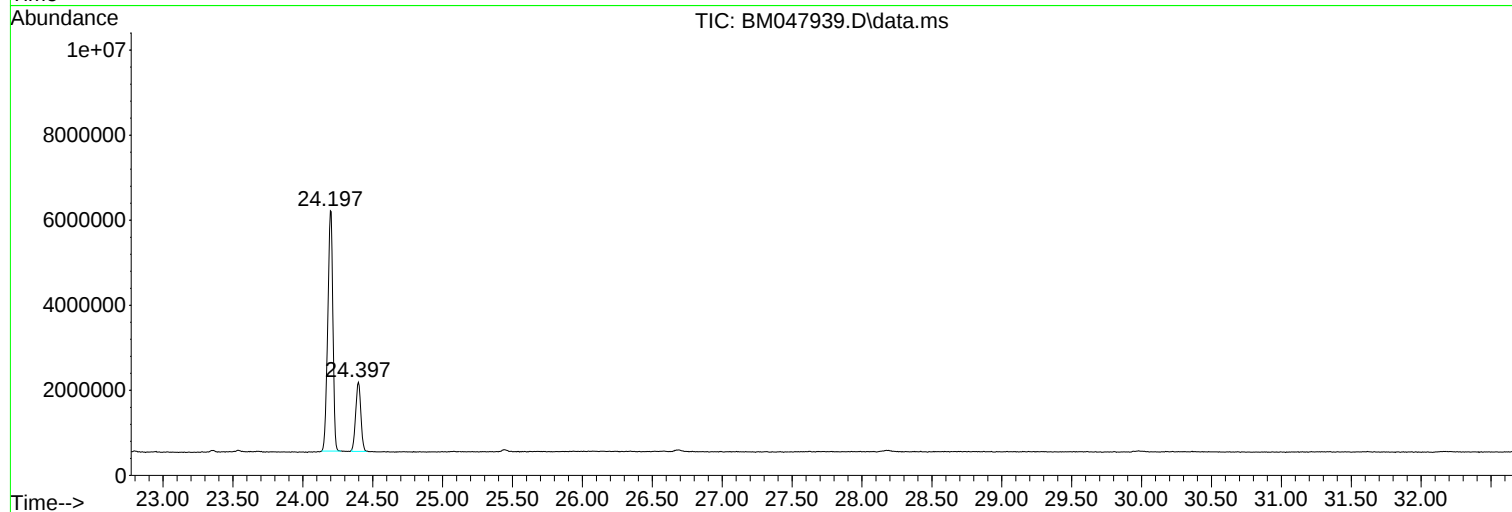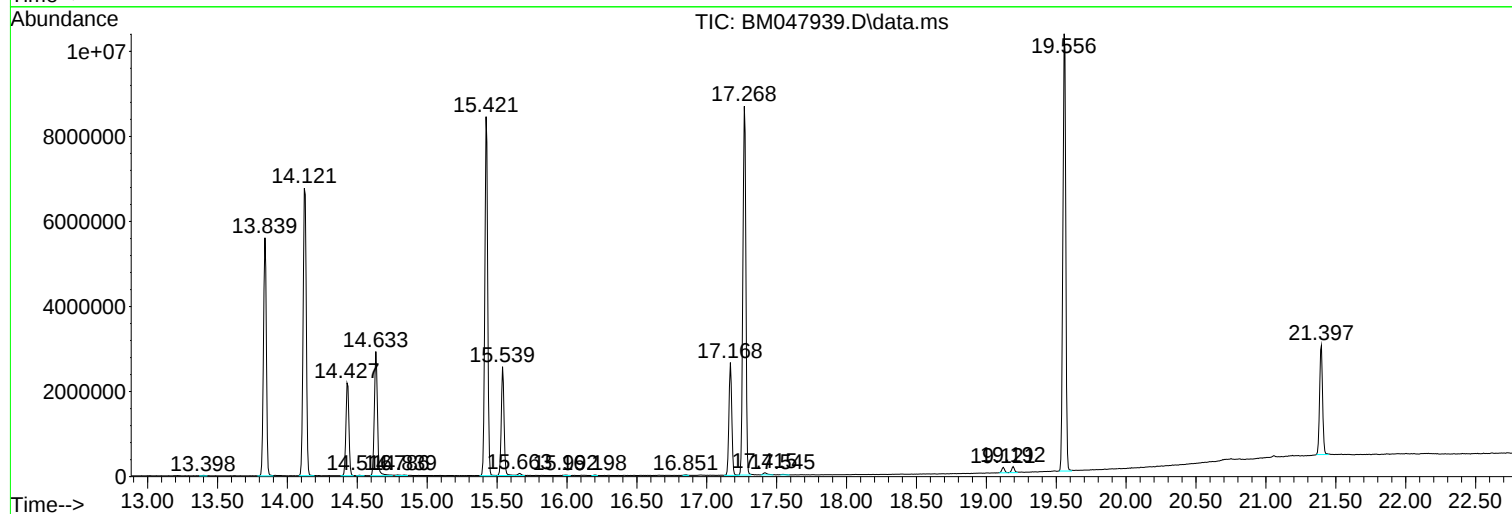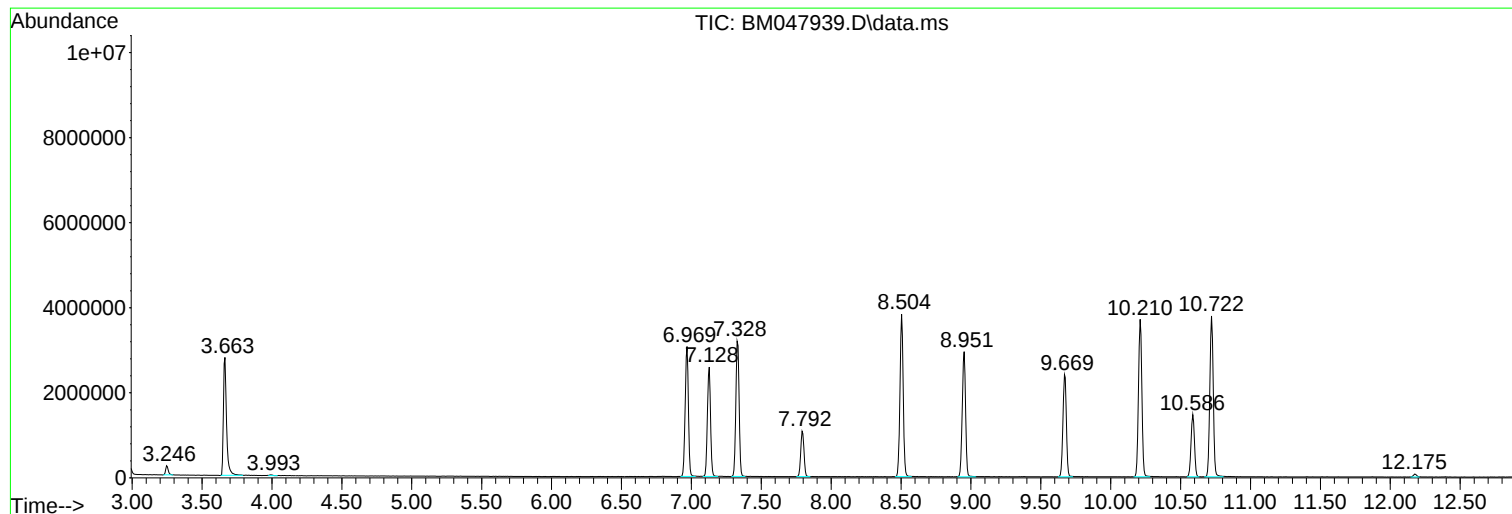

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047939.D
Acq On : 09 Oct 2024 08:53
Operator : RC/JU
Sample : SP6637
Misc : SFAM SURROGATES
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6637

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100724\
Data File : BM047939.D
Acq On : 09 Oct 2024 08:53
Operator : RC/JU
Sample : SP6637
Misc : SFAM SURROGATES
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6637

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------