


Data Path : Z:\HPCHEM1\BNA M\DATA\BM100815\
 Data File : BM002865.D
 Acq On : 08 Oct 2015 16:07
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM100815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 09 06:47:52 2015

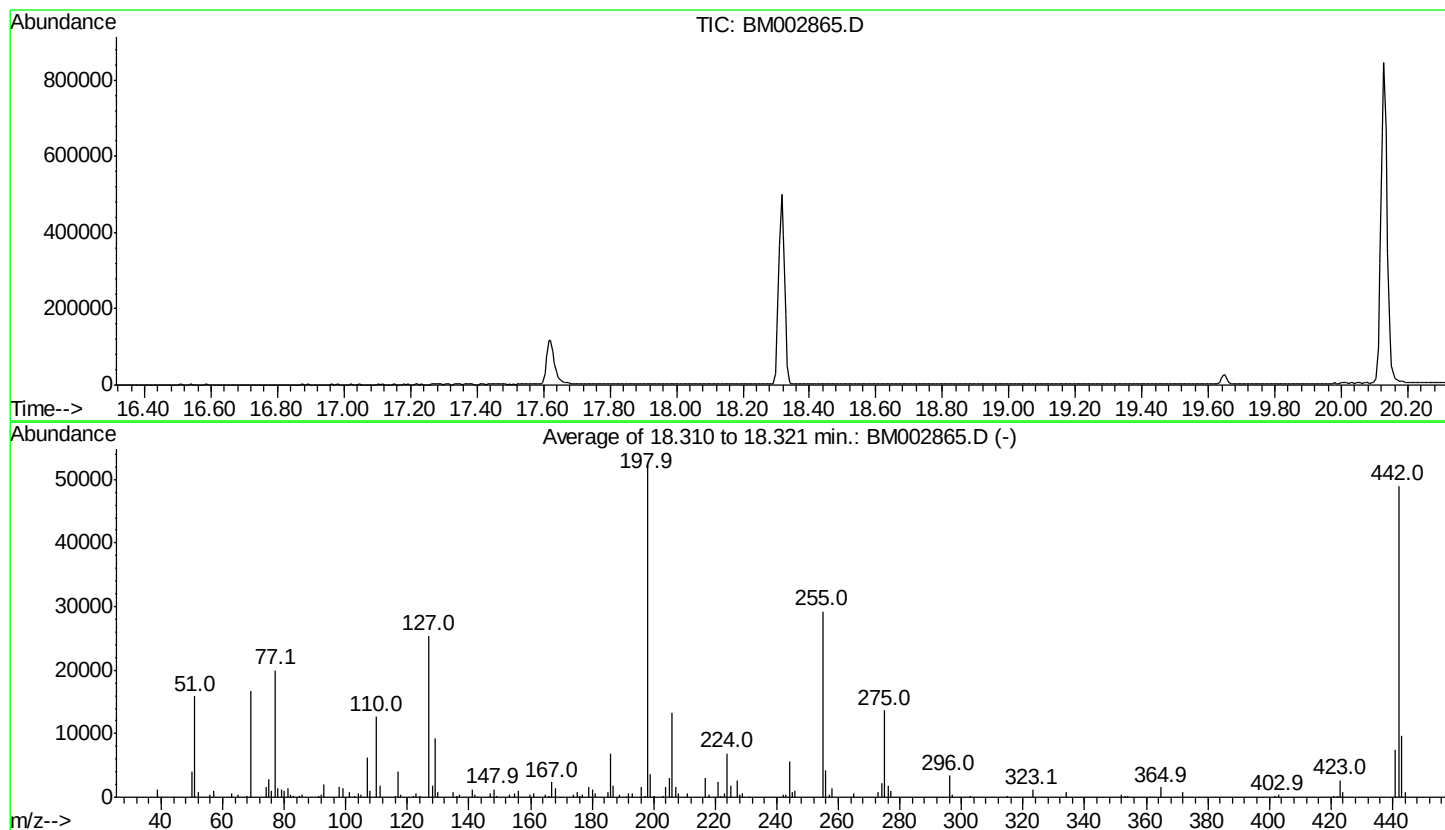

AutoFind: Scans 2588, 2589, 2590; Background Corrected with Scan 2582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	15817	PASS
68	69	0.00	2	1.3	215	PASS
69	198	0.00	100	32.1	16740	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	25384	PASS
197	198	0.00	2	0.4	220	PASS
198	198	100	100	100.0	52162	PASS
199	198	5	9	7.1	3718	PASS
275	198	10	60	26.2	13692	PASS
365	198	1	100	3.0	1562	PASS
441	442	0.01	24	15.4	7529	PASS
442	198	50	100	93.9	48992	PASS
443	442	15	24	19.9	9735	PASS