

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
 Data File : BM012020.D
 Acq On : 09 Oct 2017 19:37
 Operator : SJ/JU
 Sample : I5666-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AD5

Quant Time: Oct 10 01:18:35 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 01:14:20 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	133650	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	611557	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	402808	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	1009334	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	1388202	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	1682645	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	20623	7.30	ng/uL	0.00
5) Phenol-d5	7.01	99	77577	6.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	197036	28.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	229592	24.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	154607	15.55	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	132956	30.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	150185	30.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	282218	28.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.82	131	3309	0.31	ng/ul	0.02
43) Dimethylphthalate-d6	13.90	166	1163686	33.33	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	1346643	32.83	ng/ul	0.00
51) 4-Nitrophenol-d4	14.71	143	13188	2.16	ng/ul	0.01
57) Fluorene-d10	15.49	176	999397	32.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	192032	28.28	ng/ul	0.00
70) Anthracene-d10	17.33	188	1727926	34.74	ng/ul	0.00
76) Pyrene-d10	19.63	212	2207878	35.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.58	264	2789274	34.46	ng/ul	0.00


Target Compounds				Ovalue	
45) 2,6-Dinitrotoluene	13.90	165	7162	1.131	ng/ul# 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
Data File : BM012020.D
Acq On : 09 Oct 2017 19:37
Operator : SJ/JU
Sample : I5666-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AD5

Quant Time: Oct 10 01:18:35 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 01:14:20 2017
Response via : Initial Calibration

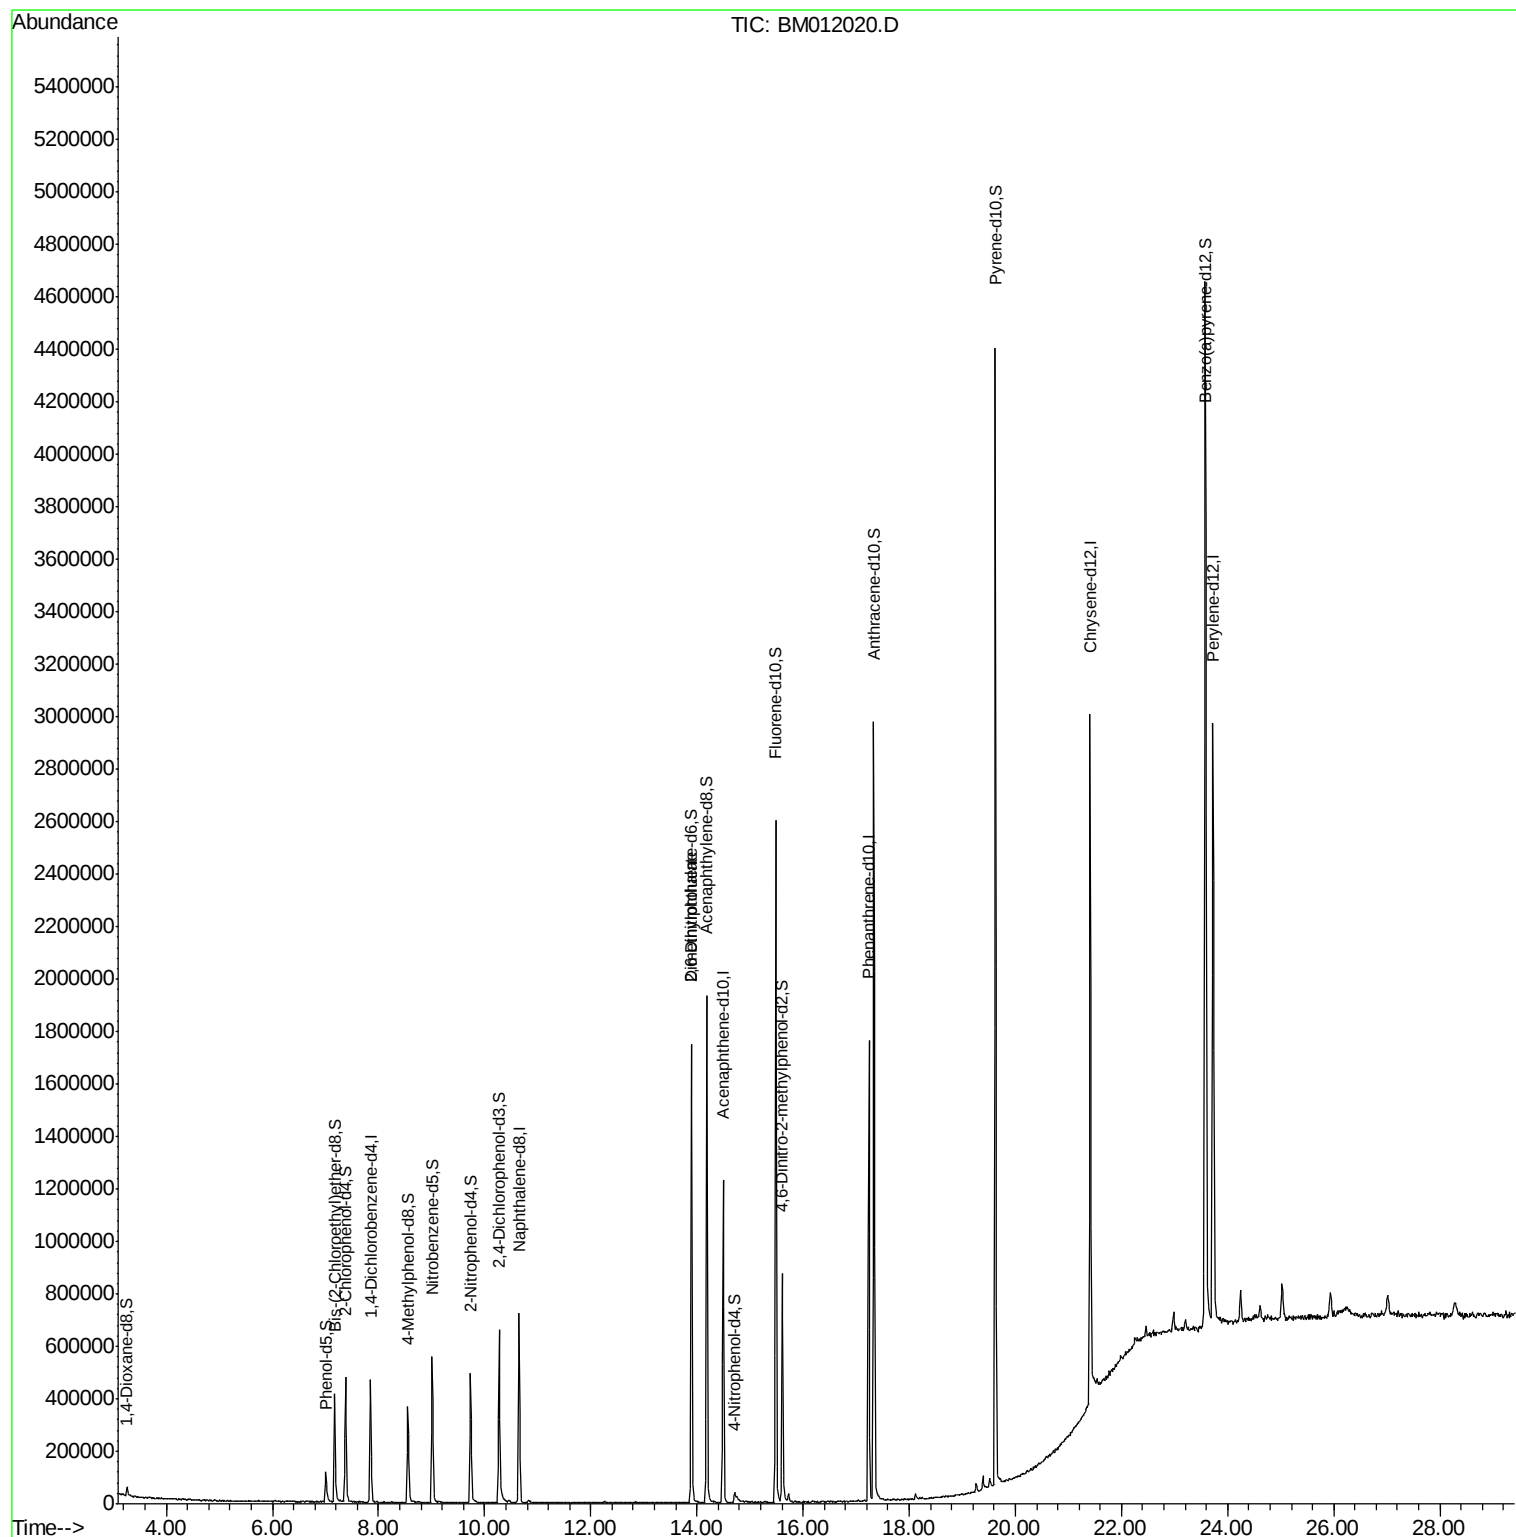

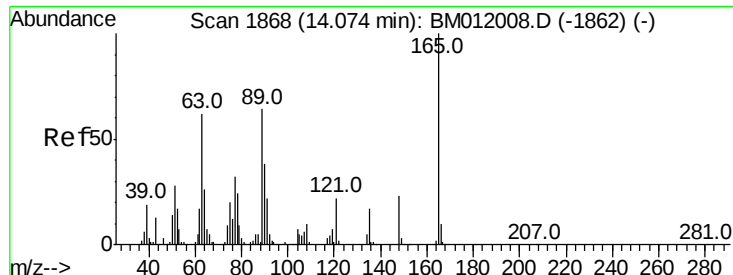

#45

2,6-Dinitrotoluene

Concen: 1.131 ng/ul

RT: 13.90 min Scan# 1839

Delta R.T. -0.17 min

Lab File: BM012020.D

Acq: 09 Oct 2017 19:37

Instrument :

BNA_M

ClientSampleId :

H0AD5


Tot Ion:165 Resp: 7162

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 38.5 14.6 22.0#

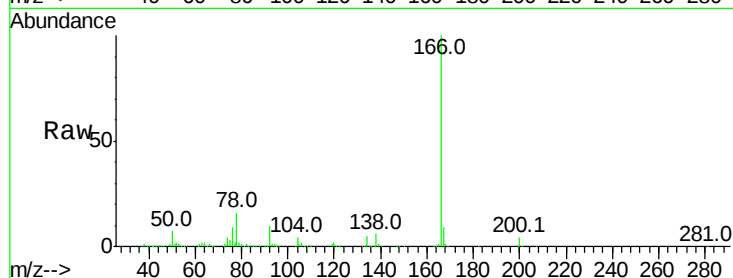

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

