

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
 Data File : BM012025.D
 Acq On : 09 Oct 2017 22:38
 Operator : SJ/JU
 Sample : I5666-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AC9

Quant Time: Oct 10 02:37:28 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 02:27:01 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	166085	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	736796	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	477792	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	1173855	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	1487753	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	1782543	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	22501	6.41	ng/uL	0.00
5) Phenol-d5	7.00	99	81366	5.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	220628	26.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	253395	22.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	170846	13.83	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	146140	27.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	166662	28.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	310097	25.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.80	131	22236	1.71	ng/ul	0.02
43) Dimethylphthalate-d6	13.90	166	1244366	30.05	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	1445922	29.71	ng/ul	0.00
51) 4-Nitrophenol-d4	14.71	143	13779	1.90	ng/ul	0.02
57) Fluorene-d10	15.49	176	1073354	29.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	201243	25.48	ng/ul	0.00
70) Anthracene-d10	17.33	188	1862448	32.20	ng/ul	0.00
76) Pyrene-d10	19.63	212	2359005	35.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.58	264	2710873	31.61	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.95	163	158231	3.972	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
Data File : BM012025.D
Acq On : 09 Oct 2017 22:38
Operator : SJ/JU
Sample : I5666-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AC9

Quant Time: Oct 10 02:37:28 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 02:27:01 2017
Response via : Initial Calibration

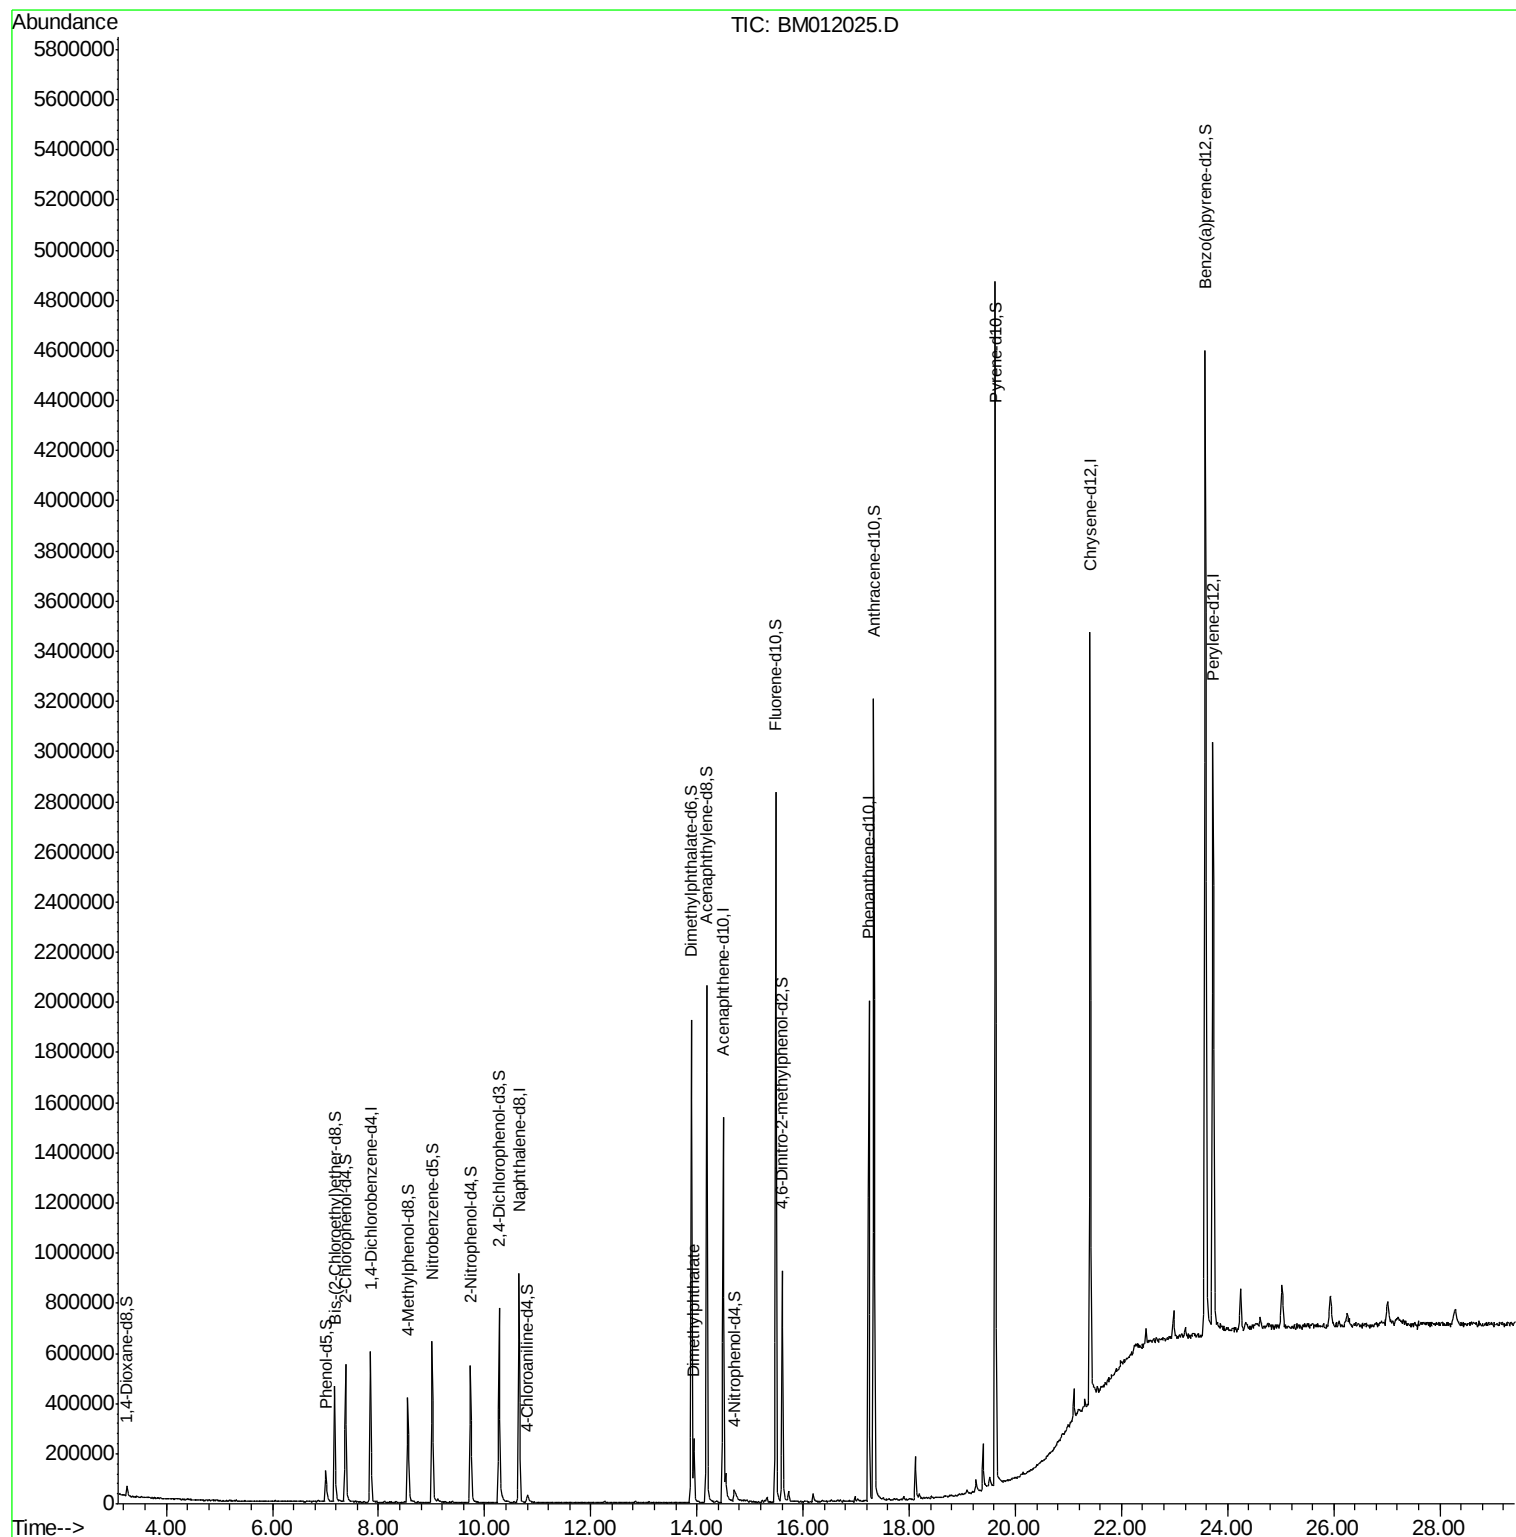

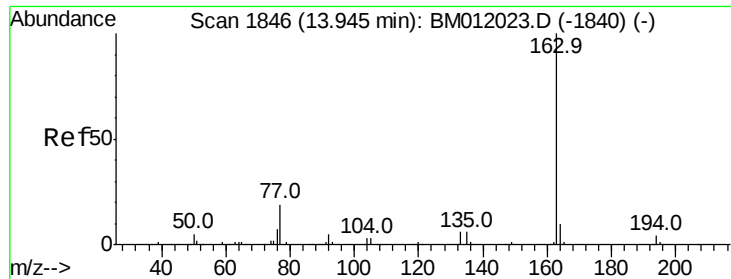

#44

Dimethylphthalate

Concen: 3.972 ng/ul

RT: 13.95 min Scan# 1846

Delta R.T. -0.00 min

Lab File: BM012025.D

Acq: 09 Oct 2017 22:38

Instrument :

BNA_M

ClientSampleId :

H0AC9


Tot Ion:163 Resp: 158231

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 9.9 8.2 12.4

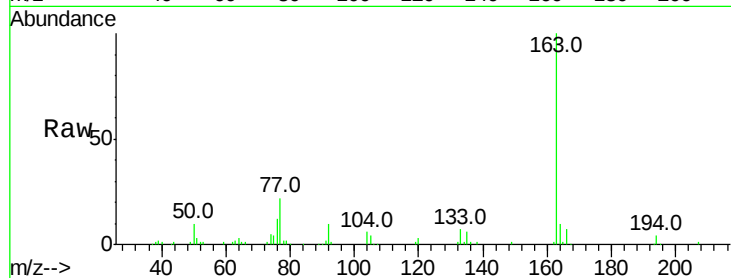

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

