

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
Data File : BM012022.D
Acq On : 09 Oct 2017 20:49
Operator : SJ/JU
Sample : I5666-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 10 01:19:02 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 01:14:20 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
H0AC2

Manual Integrations
APPROVED

Sohil
10/10/2017 5:05:24 PM

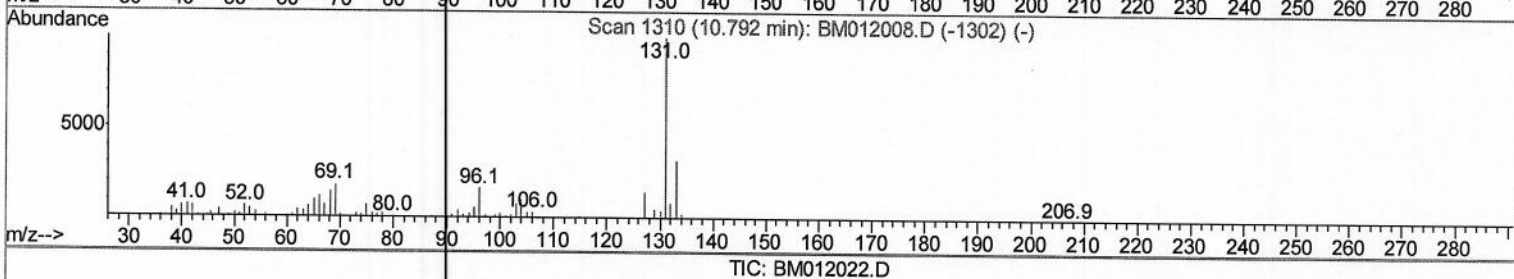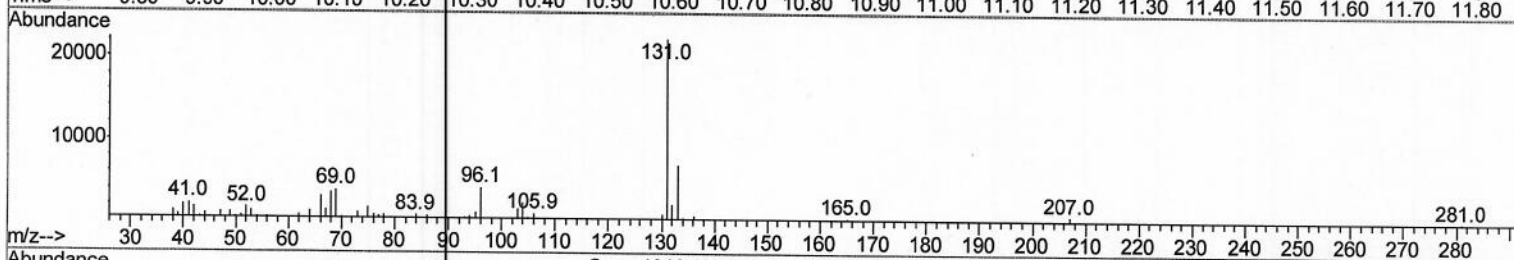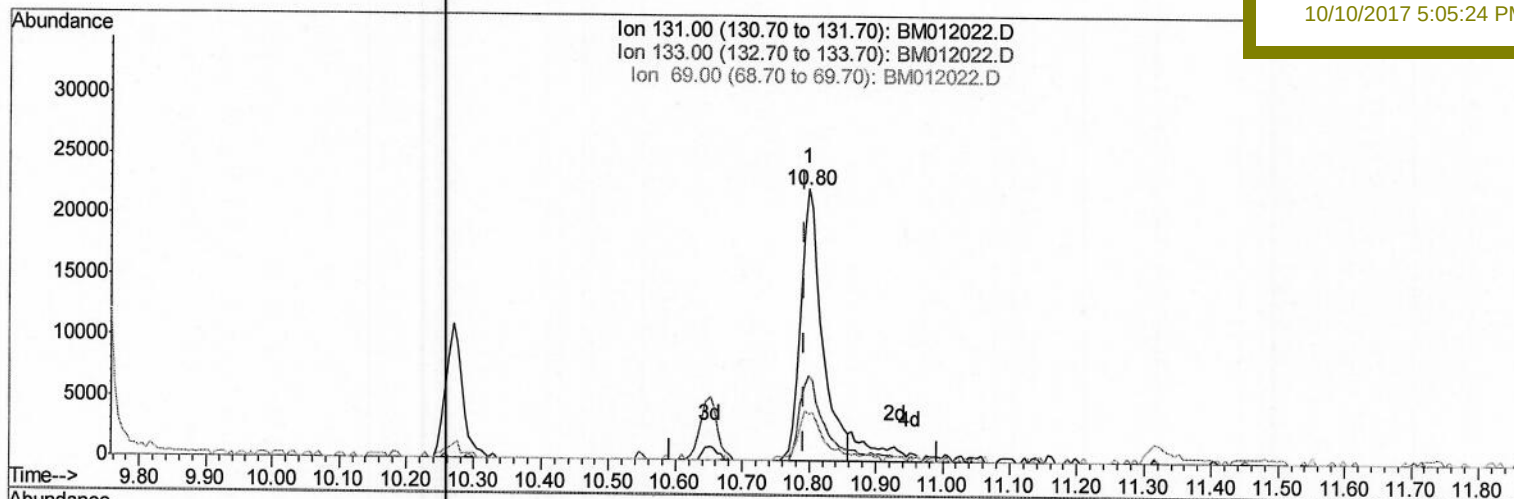

TIC: BM012022.D

(29) 4-Chloroaniline-d4 (S)

10.798min (+0.006) 2.30ng/ul

response 49823

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	31.41
69.00	24.30	17.12#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
 Data File : BM012022.D
 Acq On : 09 Oct 2017 20:49
 Operator : SJ/JU
 Sample : I5666-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 10 01:19:02 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 01:14:20 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 H0AC2

Manual Integrations
 APPROVED

Sohil
 10/10/2017 5:05:24 PM

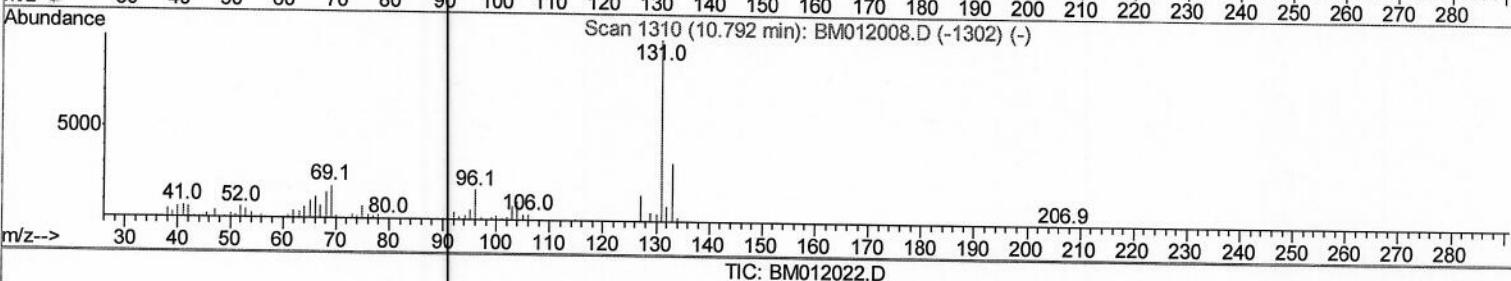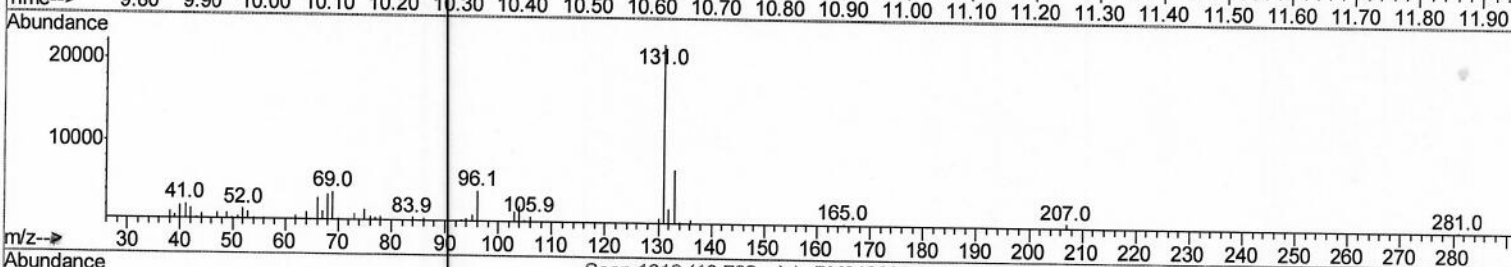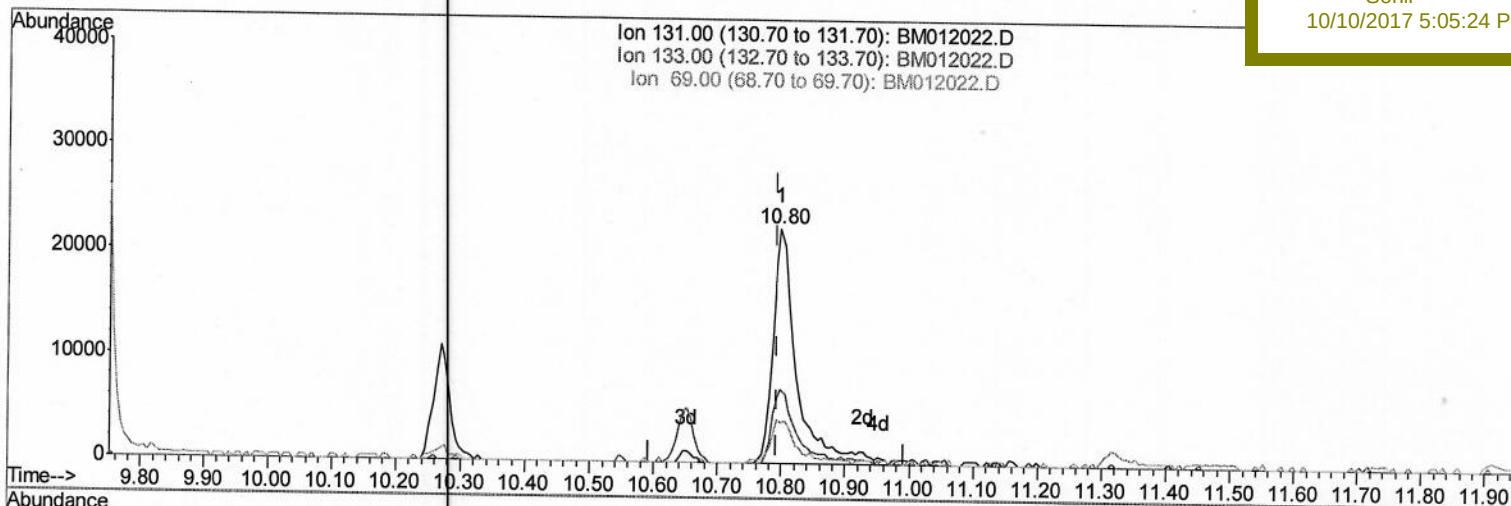

TIC: BM012022.D

(29) 4-Chloroaniline-d4 (S)

10.798min (+0.006) 2.60ng/ul m

response 56285

Ion Exp% Act%

131.00 100 100

133.00 31.40 31.41

69.00 24.30 17.12#

0.00 0.00 0.00

S.J
 10/17/17

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
 Data File : BM012022.D
 Acq On : 09 Oct 2017 20:49
 Operator : SJ/JU
 Sample : I5666-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 10 02:19:01 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 01:14:20 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 H0AC2

Manual Integrations
 APPROVED

Sohil
 10/10/2017 5:05:24 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	276955	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1225905	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	785011	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	1897329	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	2214592	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	2129540	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	33351	5.70	ng/uL	0.00
5) Phenol-d5	7.00	99	156648	6.57	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.17	67	385391	27.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	450728	23.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	319884	15.53	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	268127	30.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	311262	31.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	570919	28.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.80	131	56285m	2.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	2258714	33.20	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	2612266	32.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	67851	5.71	ng/ul	0.00
57) Fluorene-d10	15.49	176	1926297	32.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	398057	31.18	ng/ul	0.00
70) Anthracene-d10	17.34	188	3314855	35.46	ng/ul	0.00
76) Pyrene-d10	19.63	212	4184719	41.89	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.59	264	3788050	36.98	ng/ul	0.00

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.95	163	133053	2.033	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

S.J
 10/17/17

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
Data File : BM012022.D
Acq On : 09 Oct 2017 20:49
Operator : SJ/JU
Sample : I5666-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 10 02:19:01 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 01:14:20 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
H0AC2

Manual Integrations
APPROVED

Sohil
10/10/2017 5:05:24 PM

