

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
 Data File : BM012011.D
 Acq On : 09 Oct 2017 14:11
 Operator : SJ/JU
 Sample : I5522-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE2

Manual Integrations
 APPROVED

Sohil
 10/10/2017 5:05:12 PM

Quant Time: Oct 10 01:33:23 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 01:14:20 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	191961	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	857029	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	547925	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	1304106	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	1510036	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	1650076	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	4536	1.12	ng/uL	0.00
5) Phenol-d5	7.01	99	92071	5.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	40817	4.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.38	132	62110	4.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.56	113	76663	5.37	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	22925m	3.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.74	143	32035	4.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.28	165	68376m	4.92	ng/ul	0.01
29) 4-Chloroaniline-d4	10.80	131	87936m	5.80	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	296076	6.23	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	193947	3.48	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	23326m	2.81	ng/ul	0.02
57) Fluorene-d10	15.49	176	175444	4.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.62	200	29621	3.38	ng/ul	0.00
70) Anthracene-d10	17.34	188	395447	6.15	ng/ul	0.00
76) Pyrene-d10	19.63	212	639887	9.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.59	264	1702880	21.45	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	13.95	163	110030	2.408	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
Data File : BM012011.D
Acq On : 09 Oct 2017 14:11
Operator : SJ/JU
Sample : I5522-13
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AE2

Manual Integrations
APPROVED

Sohil
10/10/2017 5:05:12 PM

Quant Time: Oct 10 01:33:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 01:14:20 2017
Response via : Initial Calibration

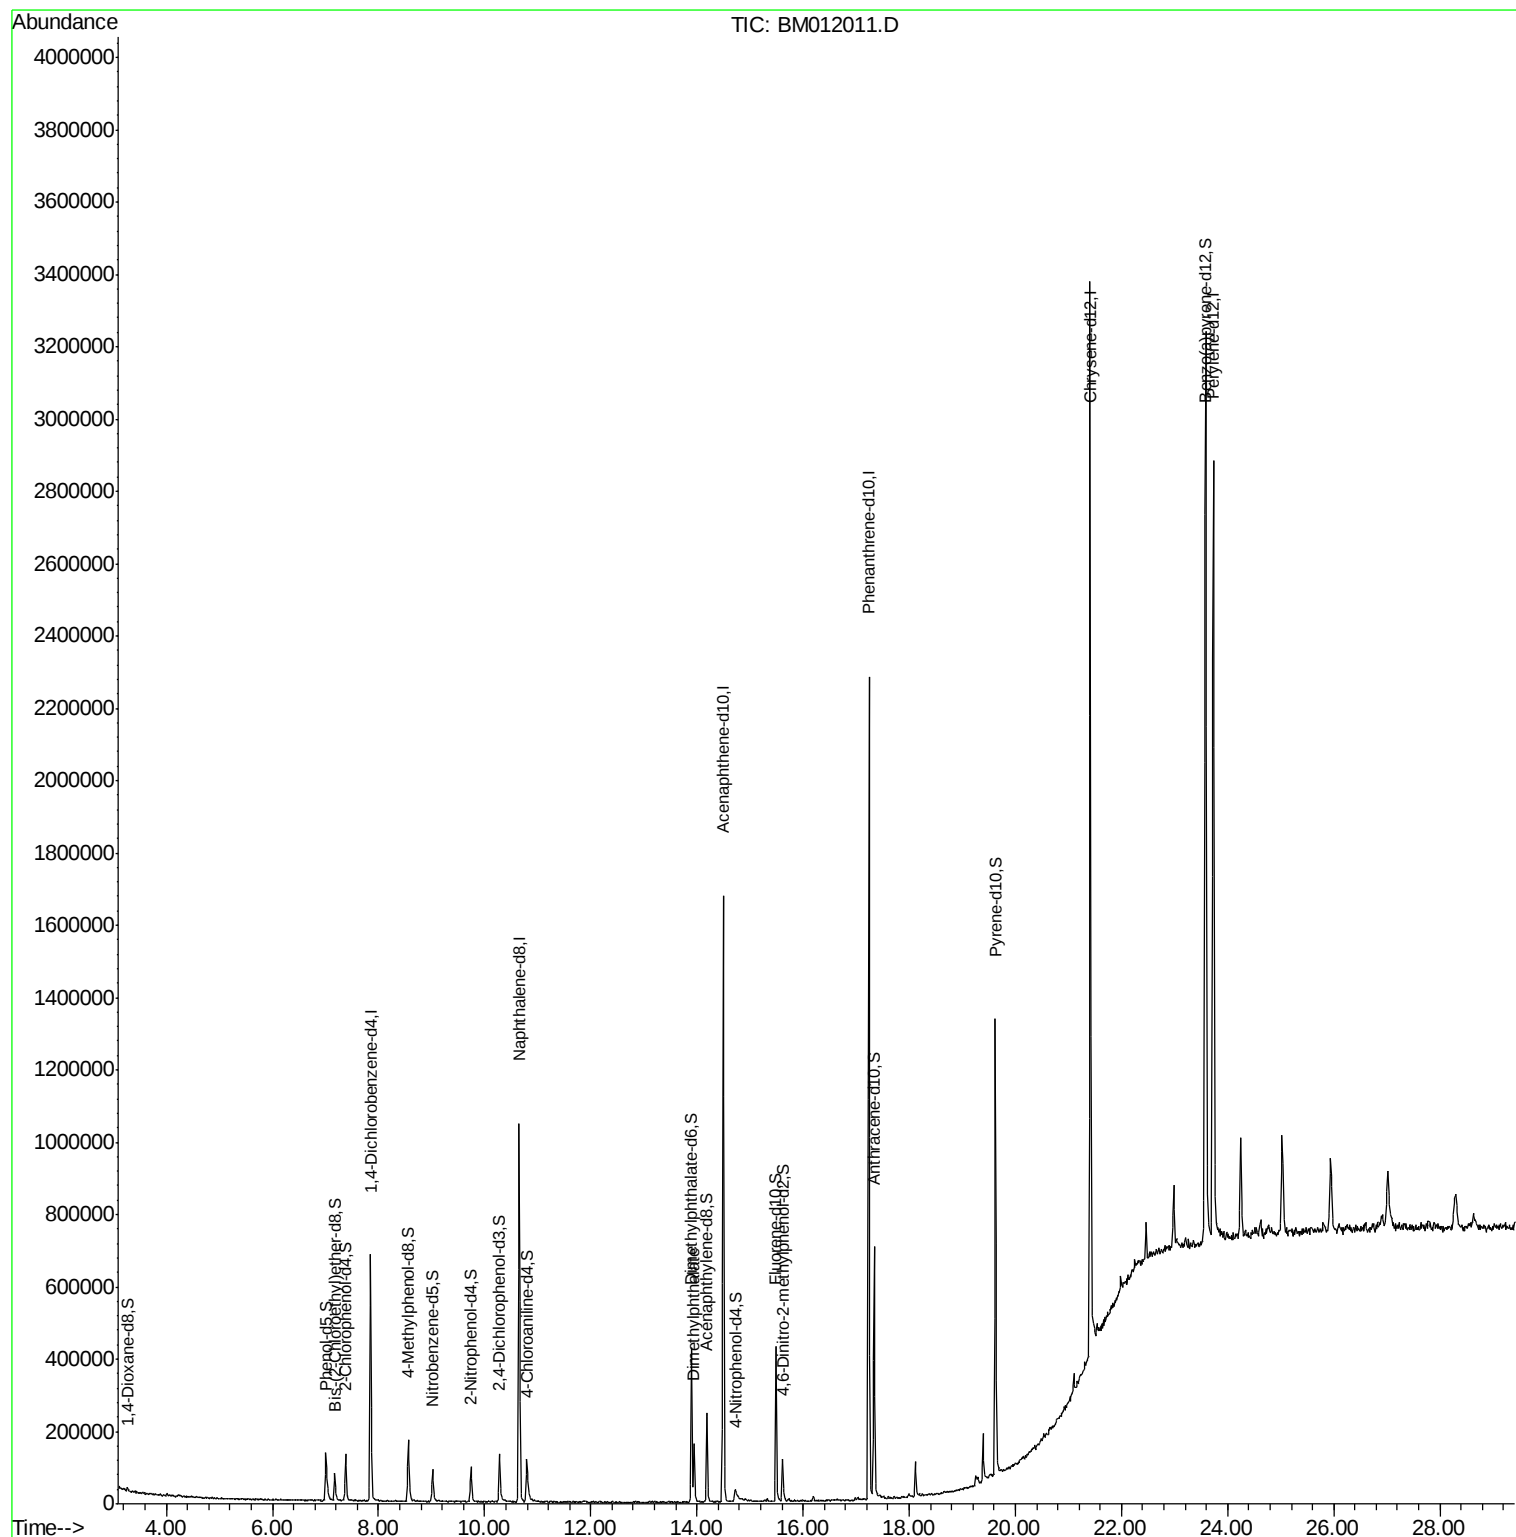

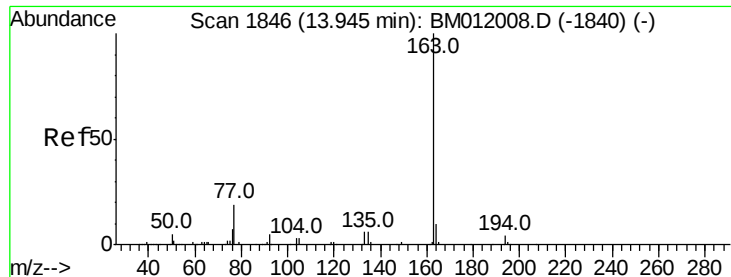

#44
 Dimethylphthalate
 Concen: 2.408 ng/ul
 RT: 13.95 min Scan# 1846
 Delta R.T. -0.00 min
 Lab File: BM012011.D
 Acq: 09 Oct 2017 14:11

Instrument :
 BNA_M
 ClientSampleId :
 C0AE2

Tot Ion:	163	Resp:	110030
Ion Ratio	Lower	Upper	
163	100		
194	4.8	3.5	5.3
164	10.4	8.2	12.4

Manual Integrations
 APPROVED

Sohil
 10/10/2017 5:05:12 PM

