

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
 Data File : BM012018.D
 Acq On : 09 Oct 2017 18:24
 Operator : SJ/JU
 Sample : I5666-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB7

Quant Time: Oct 10 01:18:09 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 01:14:20 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	215177	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	959932	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	615307	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	1461235	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	1801875	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	1898998	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	32805	7.21	ng/uL	0.00
5) Phenol-d5	7.01	99	86541	4.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	232580	21.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	271026	18.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	177729	11.11	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	155206	22.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	180423	23.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	325299	20.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.81	131	9623	0.57	ng/ul	0.02
43) Dimethylphthalate-d6	13.90	166	1439456	26.99	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	1583514	25.27	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	26007	2.79	ng/ul	0.00
57) Fluorene-d10	15.49	176	1205736	25.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	223602	22.74	ng/ul	0.00
70) Anthracene-d10	17.34	188	2122683	29.48	ng/ul	0.00
76) Pyrene-d10	19.63	212	2605114	32.05	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.59	264	2710006	29.67	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.95	163	182156	3.551	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
Data File : BM012018.D
Acq On : 09 Oct 2017 18:24
Operator : SJ/JU
Sample : I5666-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB7

Quant Time: Oct 10 01:18:09 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 01:14:20 2017
Response via : Initial Calibration

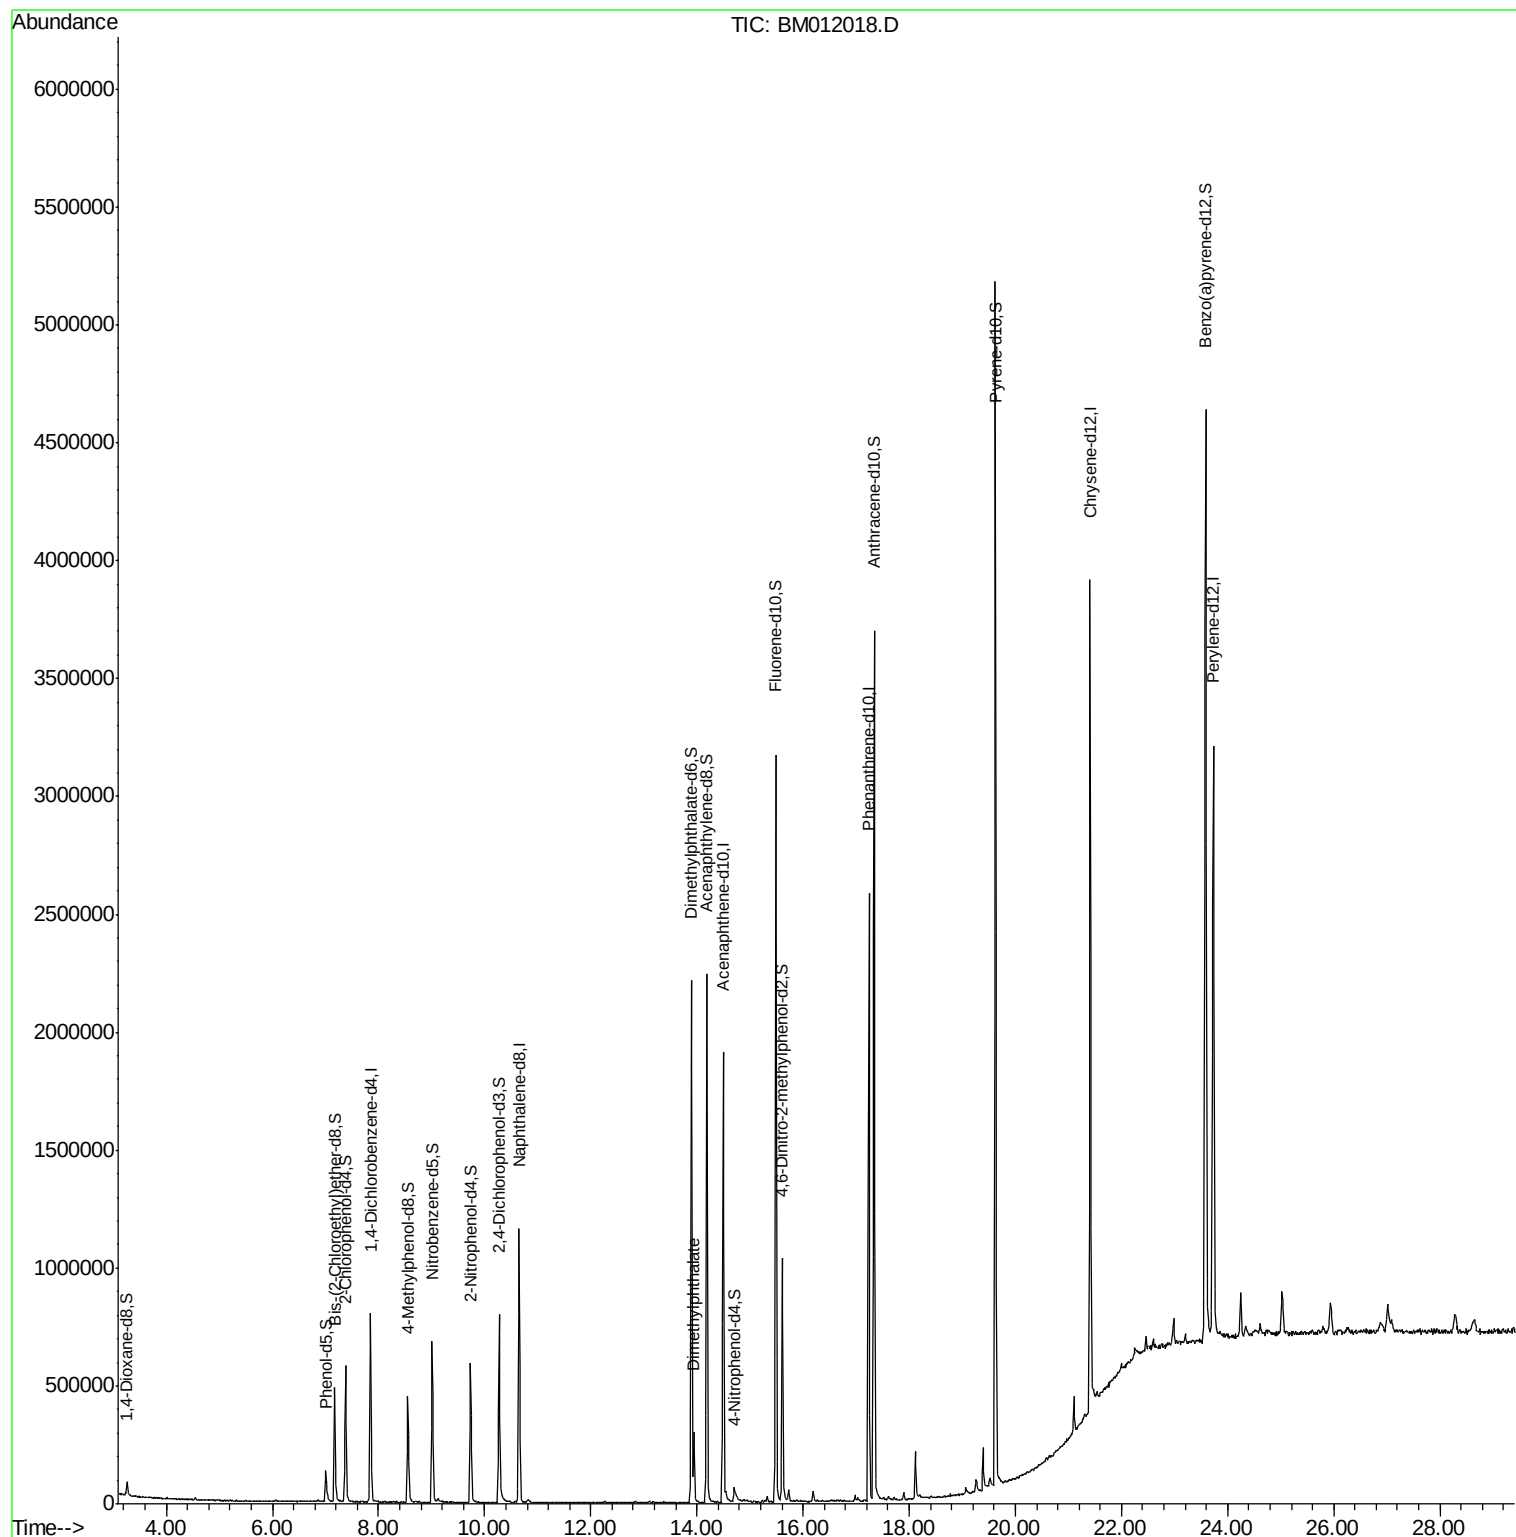

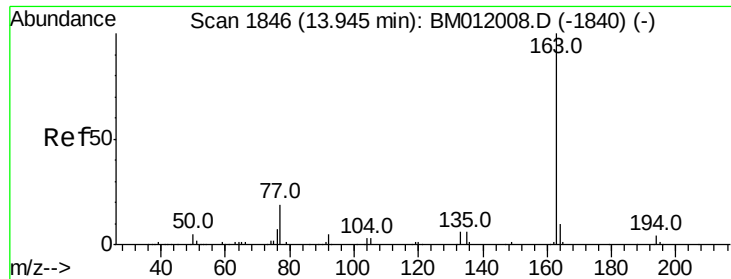

#44

Dimethylphthalate

Concen: 3.551 ng/ul

RT: 13.95 min Scan# 1846

Delta R.T. -0.00 min

Lab File: BM012018.D

Acq: 09 Oct 2017 18:24

Instrument :

BNA_M

ClientSampleId :

H0AB7


Tot Ion:163 Resp: 182156

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 9.8 8.2 12.4

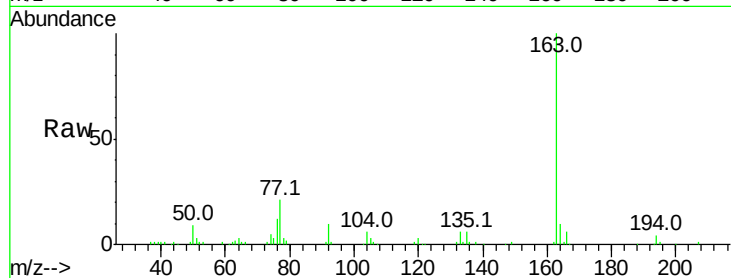

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

