

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
 Data File : BM012022.D
 Acq On : 09 Oct 2017 20:49
 Operator : SJ/JU
 Sample : I5666-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AC2

Manual Integrations
 APPROVED

Sohil
 10/10/2017 5:05:24 PM

Quant Time: Oct 10 02:19:01 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 01:14:20 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	276955	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1225905	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	785011	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	1897329	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	2214592	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	2129540	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	33351	5.70	ng/uL	0.00
5) Phenol-d5	7.00	99	156648	6.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	385391	27.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	450728	23.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	319884	15.53	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	268127	30.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	311262	31.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	570919	28.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.80	131	56285m	2.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	2258714	33.20	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	2612266	32.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	67851	5.71	ng/ul	0.00
57) Fluorene-d10	15.49	176	1926297	32.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	398057	31.18	ng/ul	0.00
70) Anthracene-d10	17.34	188	3314855	35.46	ng/ul	0.00
76) Pyrene-d10	19.63	212	4184719	41.89	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.59	264	3788050	36.98	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	13.95	163	133053	2.033	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
Data File : BM012022.D
Acq On : 09 Oct 2017 20:49
Operator : SJ/JU
Sample : I5666-05
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
H0AC2

Manual Integrations
APPROVED

Sohil
10/10/2017 5:05:24 PM

Quant Time: Oct 10 02:19:01 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 01:14:20 2017
Response via : Initial Calibration

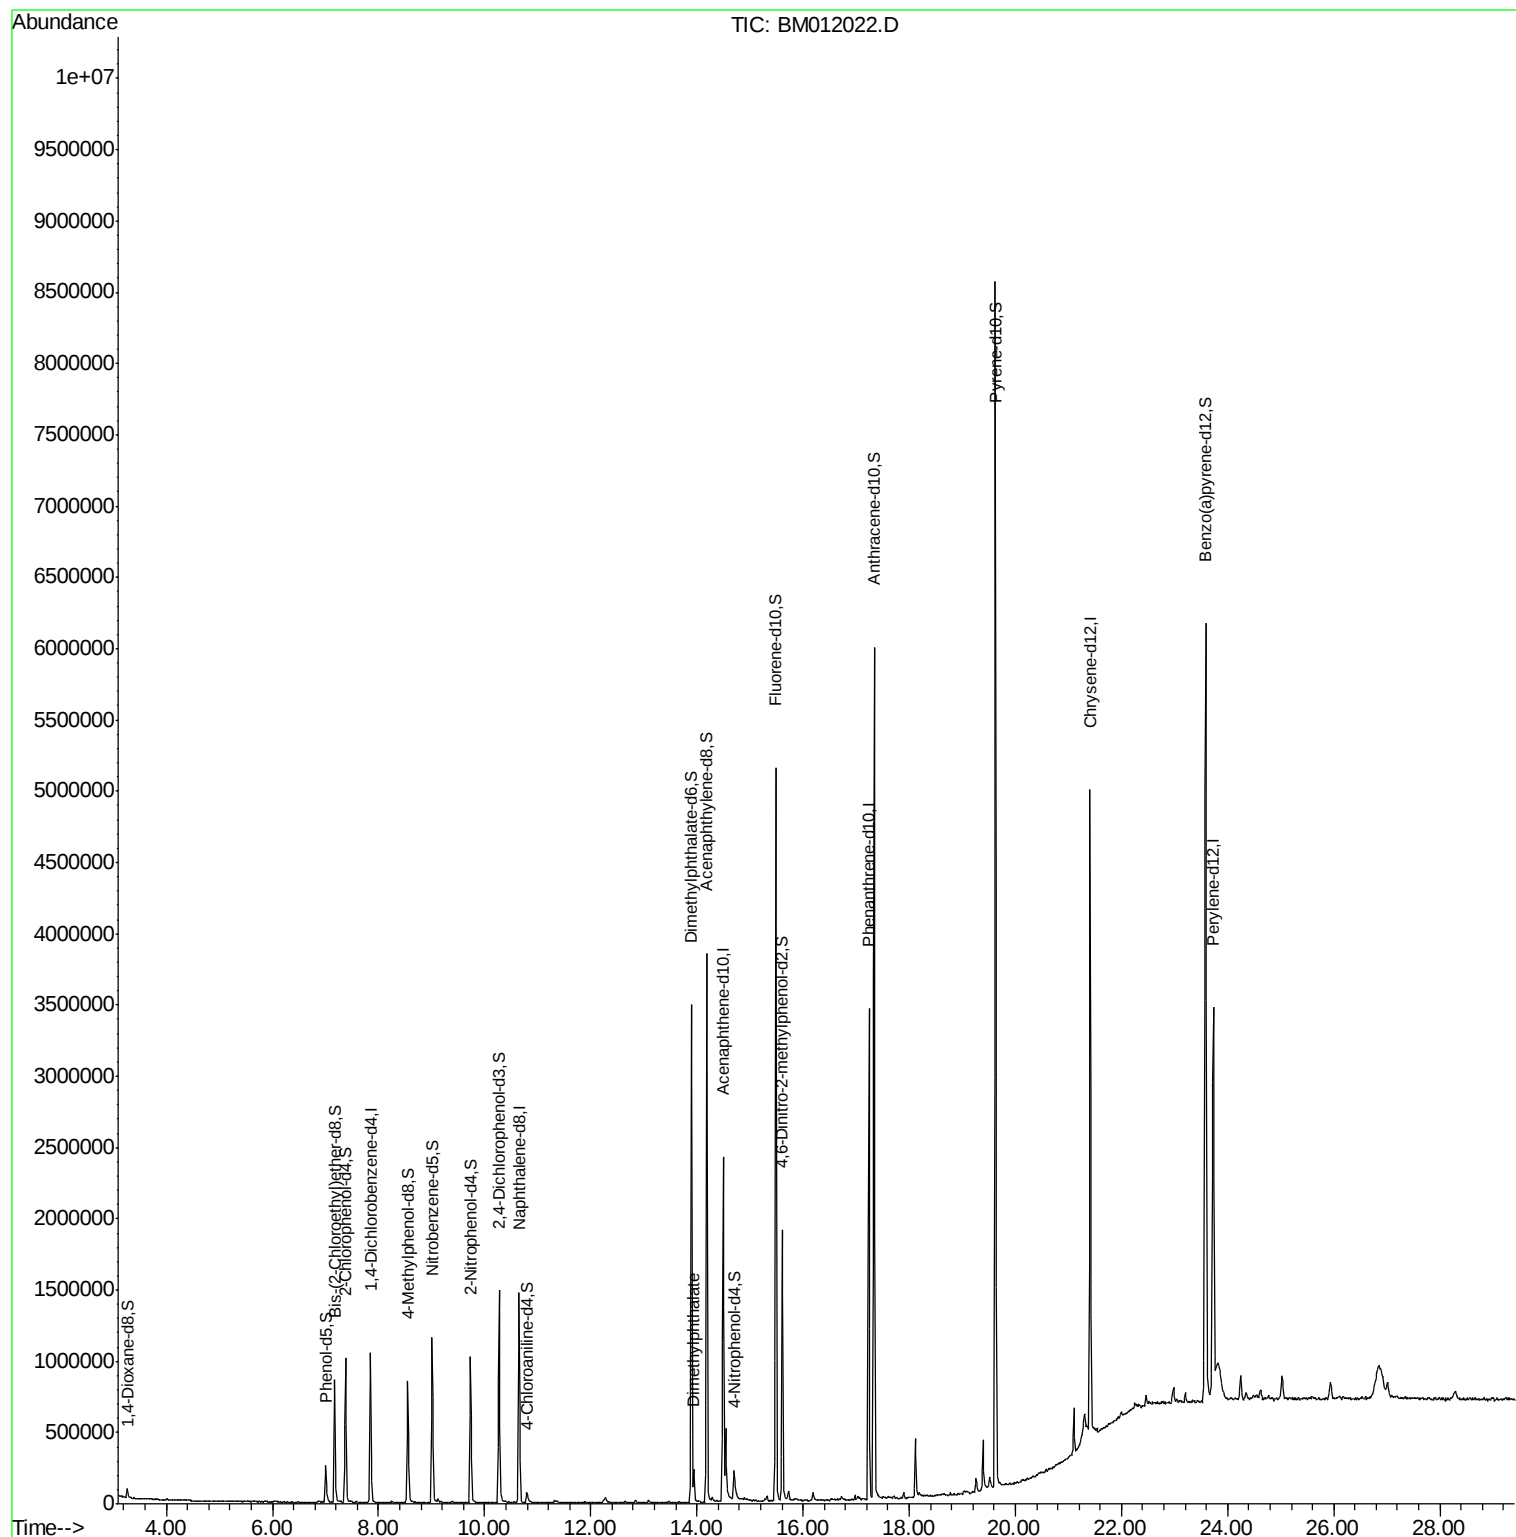

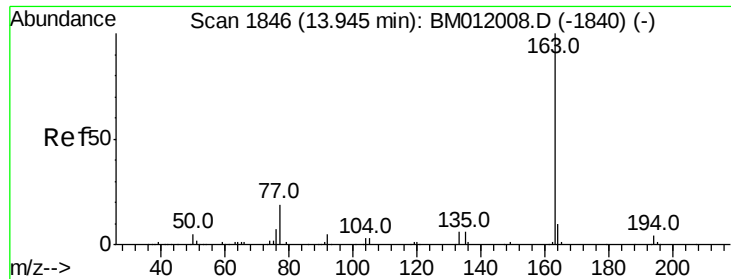

#44
 Dimethylphthalate
 Concen: 2.033 ng/ul
 RT: 13.95 min Scan# 1846
 Delta R.T. 0.00 min
 Lab File: BM012022.D
 Acq: 09 Oct 2017 20:49

Instrument :
 BNA_M
 ClientSampleId :
 H0AC2

Tot Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.2	3.5	5.3
164	9.5	8.2	12.4

Manual Integrations
 APPROVED

Sohil
 10/10/2017 5:05:24 PM

