

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
 Data File : BM012024.D
 Acq On : 09 Oct 2017 22:02
 Operator : SJ/JU
 Sample : I5666-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AC4

Manual Integrations
 APPROVED

Sohil
 10/10/2017 5:05:30 PM

Quant Time: Oct 10 02:42:17 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 02:27:01 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	99380	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	446981	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	288272	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	716679	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	1044125	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	1342295	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	15361m	7.31	ng/uL	0.00
5) Phenol-d5	7.01	99	48482	5.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	136258	26.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	153327	22.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	105136	14.22	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	90259	28.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	100538	28.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	188947	26.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.82	131	16265m	2.06	ng/ul	0.03
43) Dimethylphthalate-d6	13.90	166	848346	33.96	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	954705	32.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.71	143	16517m	3.78	ng/ul	0.02
57) Fluorene-d10	15.49	176	744799	33.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	148252	30.74	ng/ul	0.00
70) Anthracene-d10	17.33	188	1349109	38.20	ng/ul	0.00
76) Pyrene-d10	19.63	212	1816222	38.56	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.58	264	2488133	38.53	ng/ul	0.00

Target Compounds					Ovalue	
44) Dimethylphthalate	13.95	163	81331	3.384	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM100917\
Data File : BM012024.D
Acq On : 09 Oct 2017 22:02
Operator : SJ/JU
Sample : I5666-06
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
H0AC4

Manual Integrations
APPROVED

Sohil
10/10/2017 5:05:30 PM

Quant Time: Oct 10 02:42:17 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 02:27:01 2017
Response via : Initial Calibration

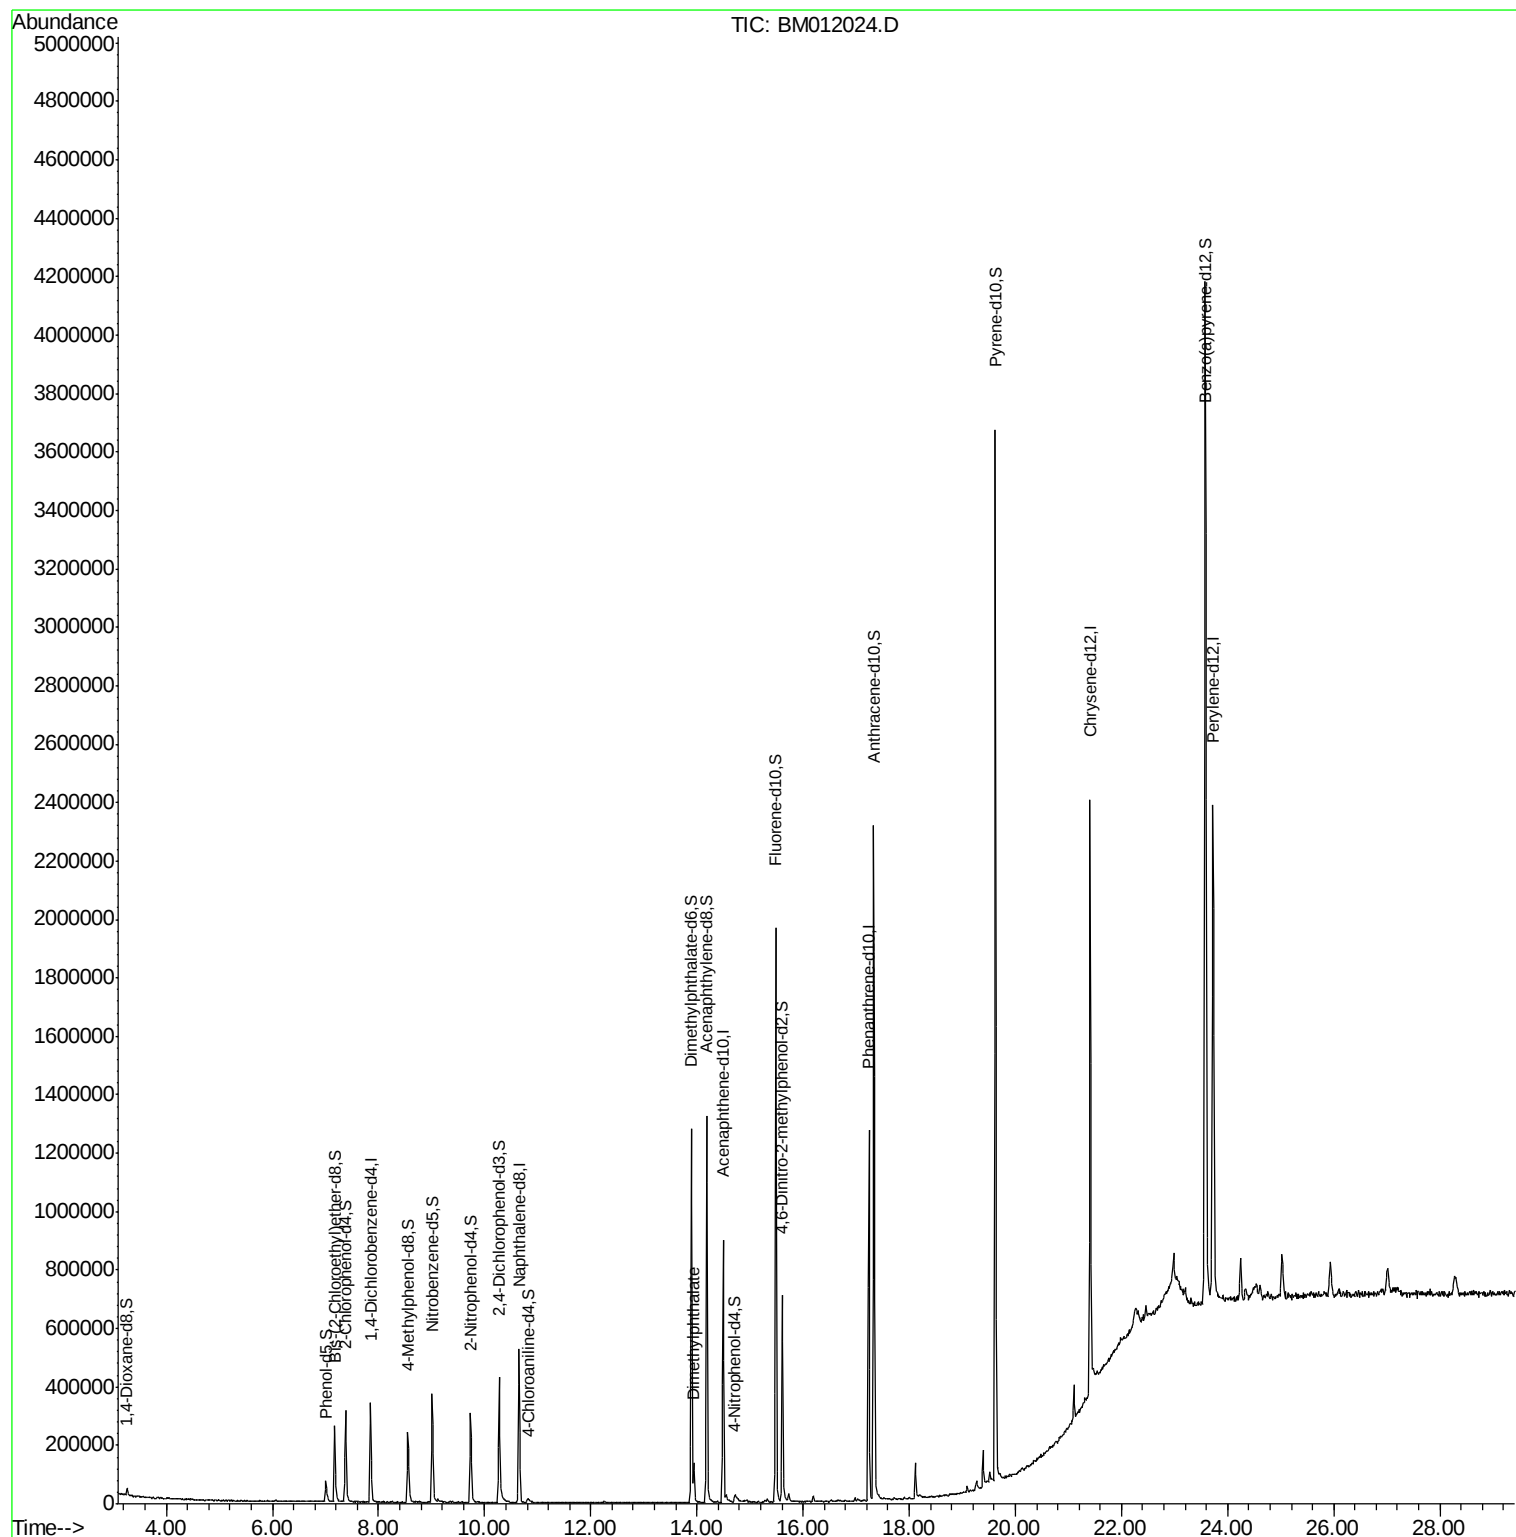

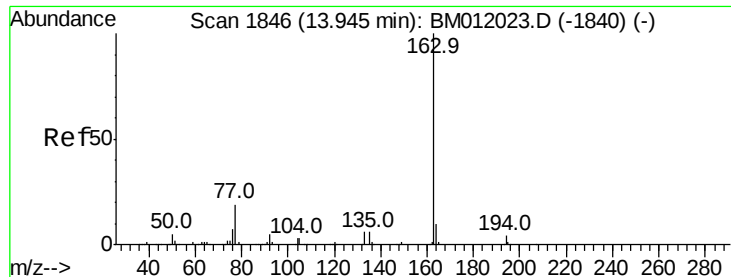


#44
 Dimethylphthalate
 Concen: 3.384 ng/ul
 RT: 13.95 min Scan# 1846
 Delta R.T. -0.00 min
 Lab File: BM012024.D
 Acq: 09 Oct 2017 22:02

Instrument :
 BNA_M
 ClientSampleId :
 H0AC4

Tot Ion:	163	Resp:	81331
Ion Ratio	Lower	Upper	
163	100		
194	3.8	3.5	5.3
164	10.8	8.2	12.4

Manual Integrations
 APPROVED

Sohil
 10/10/2017 5:05:30 PM

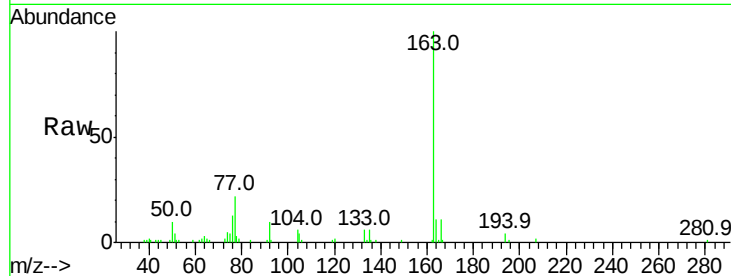

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

