

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
 Data File : BM032398.D
 Acq On : 08 Oct 2021 18:05
 Operator : CG/JU
 Sample : M4104-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 55TH-ST-33

Manual Integrations
 APPROVED

mohammad
 10/11/2021 2:13:24 PM

Quant Time: Oct 08 19:17:20 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 17:11:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.613	152	361464	20.00	ng	0.00
21) Naphthalene-d8	10.401	136	1479389	20.00	ng	# 0.00
39) Acenaphthene-d10	14.260	164	937888	20.00	ng	0.00
64) Phenanthrene-d10	16.989	188	1922913	20.00	ng	# 0.00
76) Chrysene-d12	21.153	240	1835531	20.00	ng	0.00
86) Perylene-d12	23.294	264	1587169	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.190	112	731506	34.10	ng	0.00
7) Phenol-d6	6.801	99	587771	20.03	ng	-0.01
23) Nitrobenzene-d5	8.766	82	1882174	70.76	ng	0.00
42) 2,4,6-Tribromophenol	15.748	330	727757	69.31	ng	0.00
45) 2-Fluorobiphenyl	12.883	172	4119163	65.30	ng	0.00
79) Terphenyl-d14	19.606	244	5507972	63.20	ng	0.00
Target Compounds						
32) Benzoic acid	9.666	122	3175m	5.01	ng	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
Data File : BM032398.D
Acq On : 08 Oct 2021 18:05
Operator : CG/JU
Sample : M4104-01
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
55TH-ST-33

Manual Integrations
APPROVED

mohammad
10/11/2021 2:13:24 PM

Quant Time: Oct 08 19:17:20 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 08 17:11:04 2021
Response via : Initial Calibration

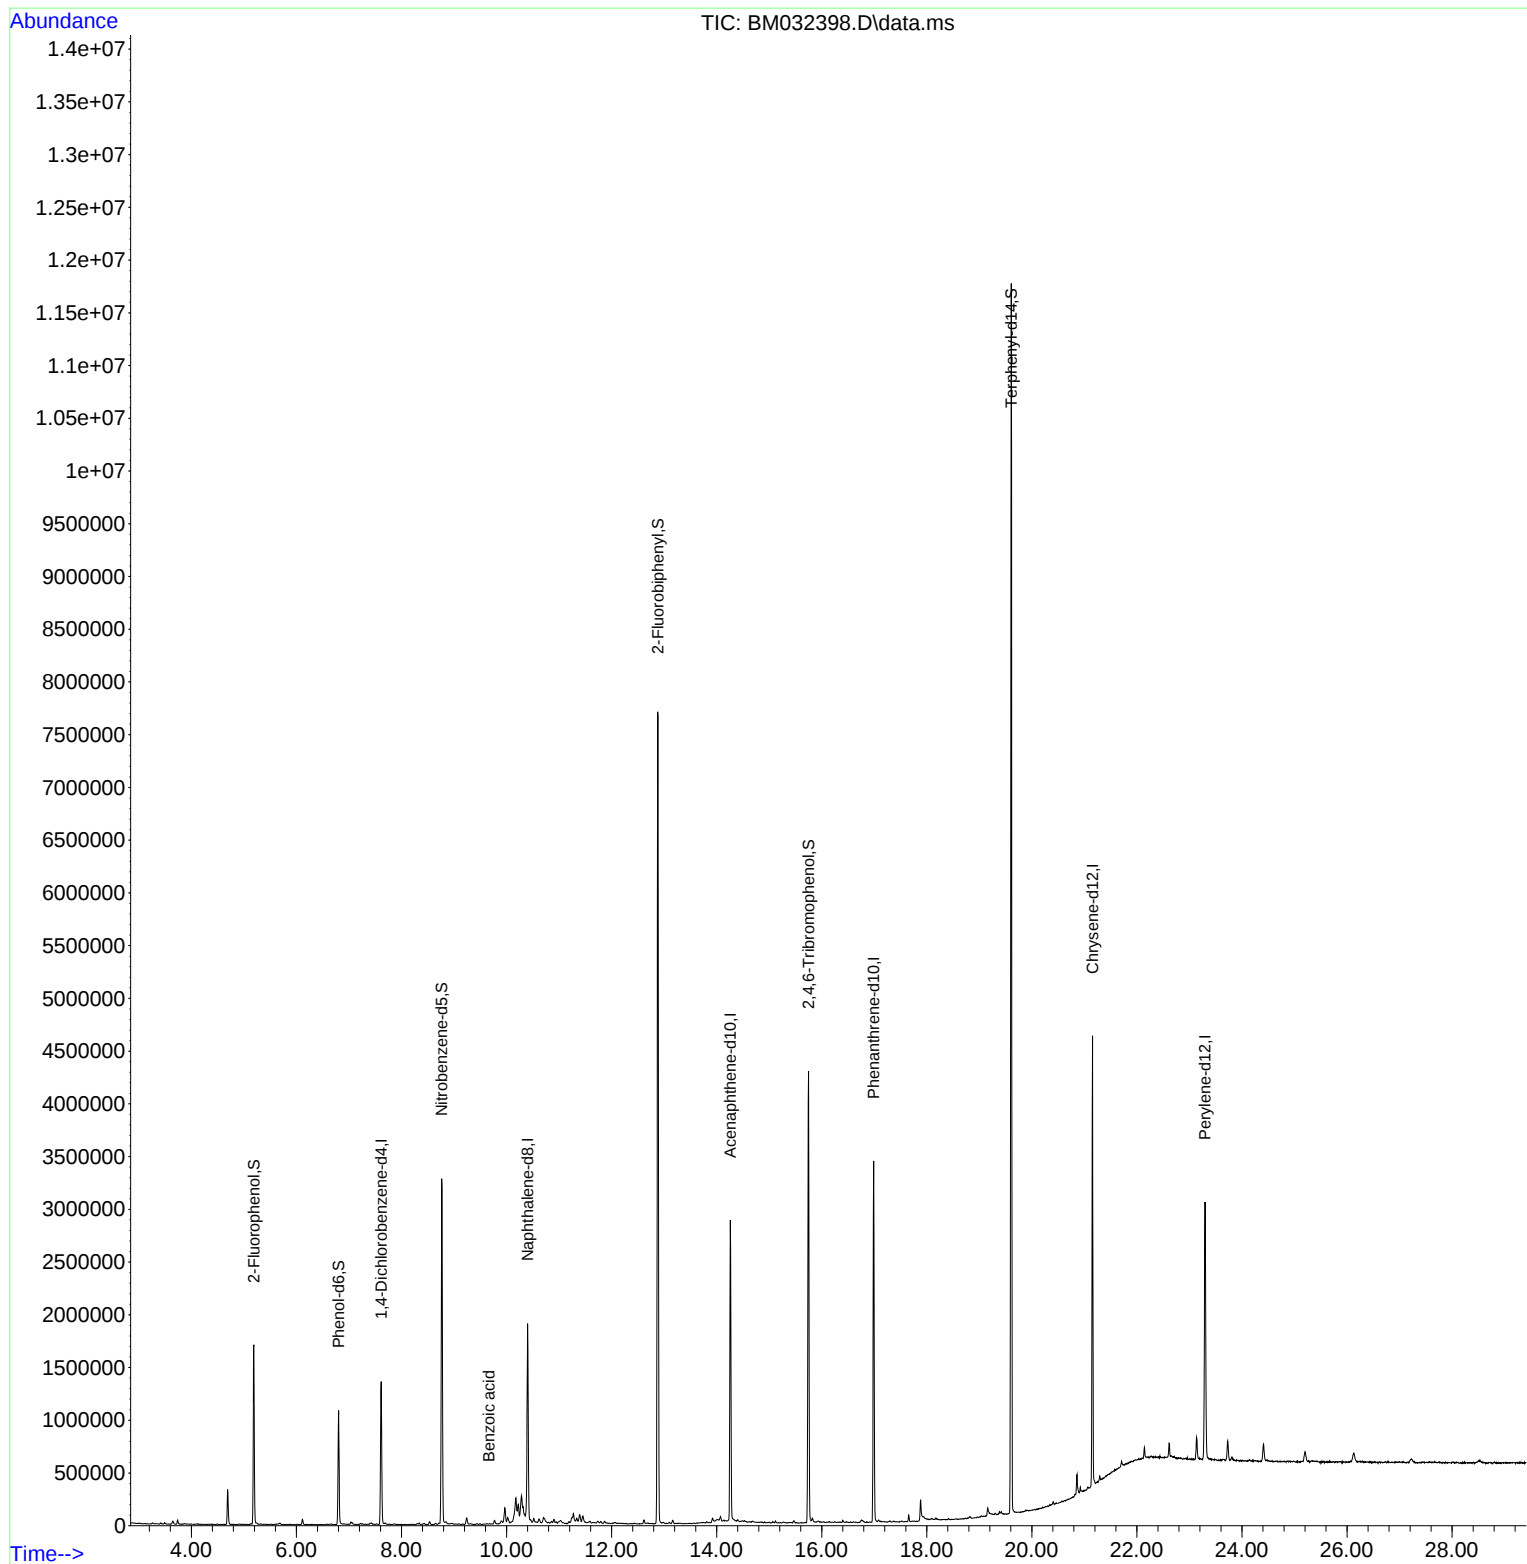







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.613 min Scan# 812
Delta R.T. -0.006 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

Tgt Ion:152 Resp: 361464
Ion Ratio Lower Upper
152 100
150 154.7 122.4 183.6
115 59.6 53.8 80.8

Instrument :
BNA_M
ClientSampleId :
55TH-ST-33




Manual Integrations
APPROVED


mohammad
10/11/2021 2:13:24 PM

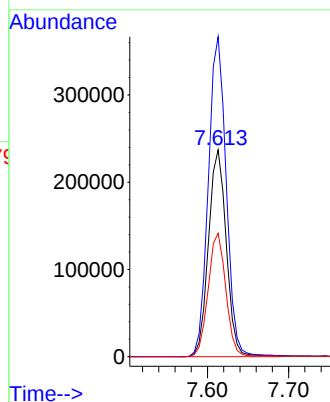

#5
2-Fluorophenol
Concen: 34.10 ng
RT: 5.190 min Scan# 400
Delta R.T. 0.000 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

Tgt Ion:112 Resp: 731506
Ion Ratio Lower Upper
112 100
64 54.9 53.7 80.5
63 28.8 33.9 50.9#

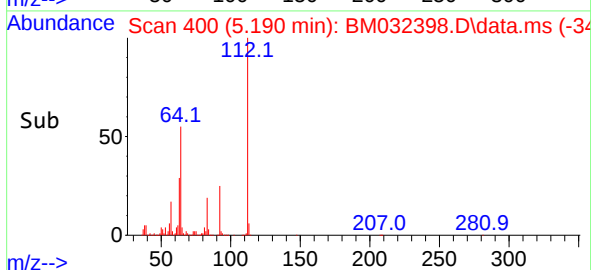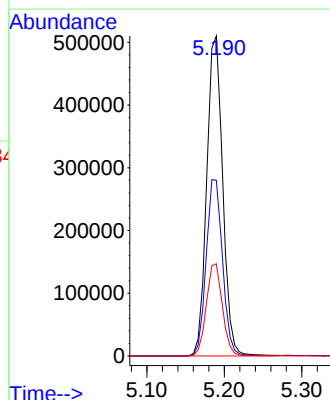







#7
Phenol-d6
Concen: 20.03 ng
RT: 6.801 min Scan# 674
Delta R.T. -0.012 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

Tgt Ion: 99 Resp: 587771
Ion Ratio Lower Upper
99 100
42 15.8 23.0 34.6#
71 32.3 37.8 56.8#

Instrument :
BNA_M
ClientSampleId :
55TH-ST-33




Manual Integrations
APPROVED


mohammad
10/11/2021 2:13:24 PM

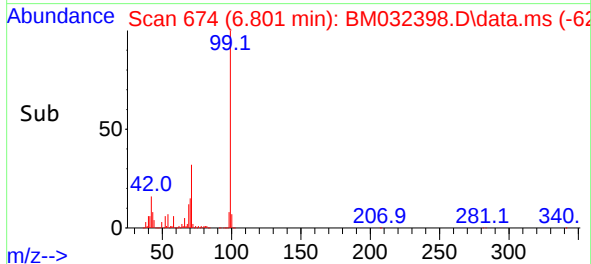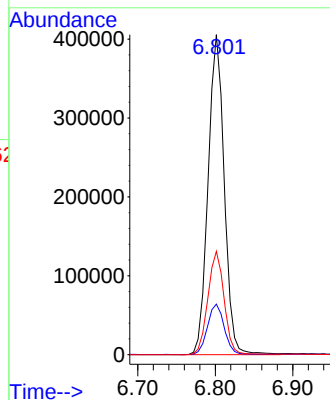

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.401 min Scan# 1286
Delta R.T. -0.006 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

Tgt Ion: 136 Resp: 1479389
Ion Ratio Lower Upper
136 100
137 10.9 8.7 13.1
54 7.9 7.4 11.0
68 6.0 3.8 5.8#

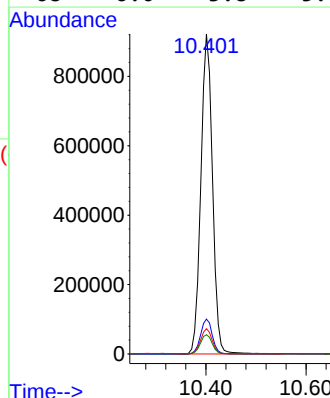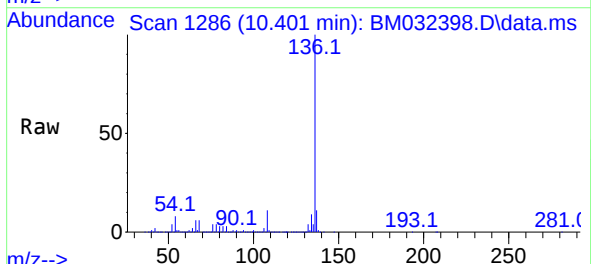







#23
Nitrobenzene-d5
Concen: 70.76 ng
RT: 8.766 min Scan# 1008
Delta R.T. -0.006 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

Instrument :
BNA_M
ClientSampleId :
55TH-ST-33

Tgt Ion: 82 Resp: 1882174
Ion Ratio Lower Upper
82 100
128 44.1 29.0 43.6#
54 48.5 45.8 68.8




Manual Integrations
APPROVED


mohammad
10/11/2021 2:13:24 PM

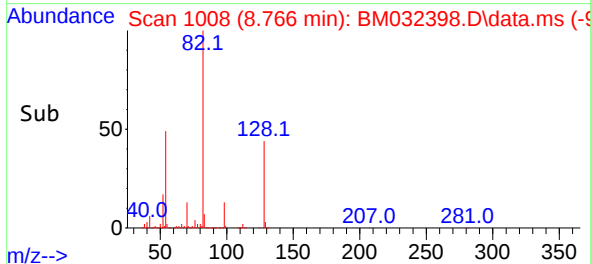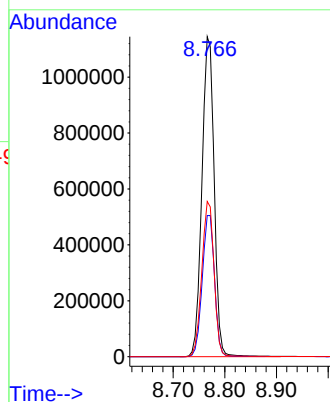

#32
Benzoic acid
Concen: 5.01 ng m
RT: 9.666 min Scan# 1161
Delta R.T. -0.106 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05


Tgt Ion: 122 Resp: 3175
Ion Ratio Lower Upper
122 100
105 91.1 120.3 160.3#
77 81.7 100.0 140.0#

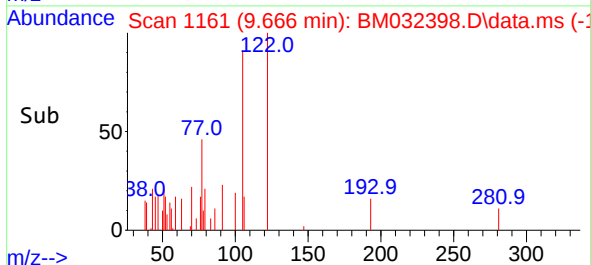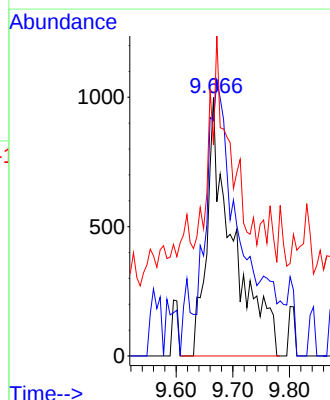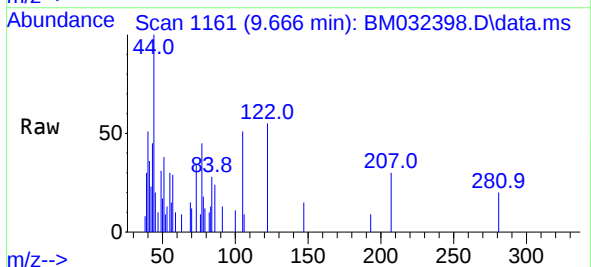



#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.260 min Scan# 1942
Delta R.T. -0.006 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05




Instrument :
BNA_M
ClientSampleId :
55TH-ST-33




Tgt Ion:164 Resp: 937888
Ion Ratio Lower Upper
164 100
162 99.8 80.6 121.0
160 43.5 35.1 52.7

Manual Integrations
APPROVED



mohammad
10/11/2021 2:13:24 PM

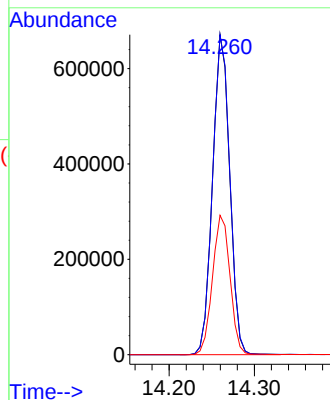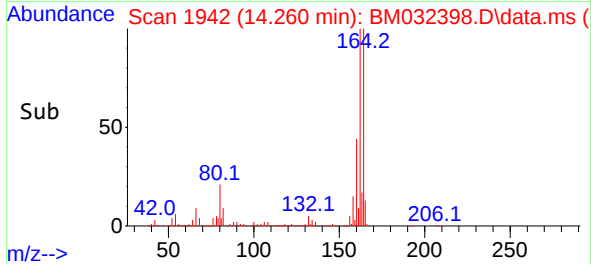


#42
2,4,6-Tribromophenol
Concen: 69.31 ng
RT: 15.748 min Scan# 2195
Delta R.T. -0.006 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

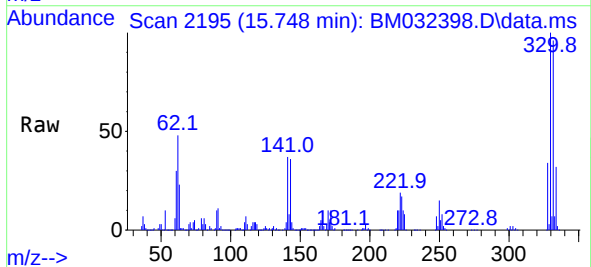


Tgt Ion:330 Resp: 727757
Ion Ratio Lower Upper
330 100
332 96.5 75.7 113.5
141 38.4 50.7 76.1#

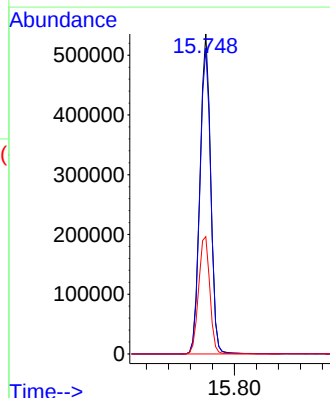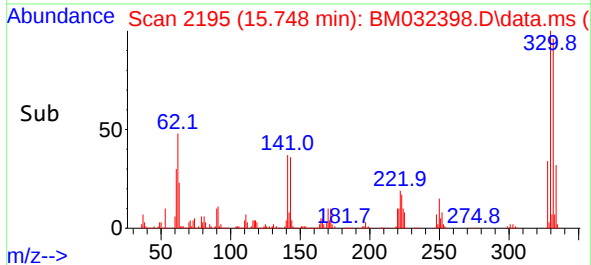



#45
2-Fluorobiphenyl
Concen: 65.30 ng
RT: 12.883 min Scan# 1708
Delta R.T. 0.000 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05




Instrument :
BNA_M
ClientSampleId :
55TH-ST-33




Tgt Ion:172 Resp: 4119163
Ion Ratio Lower Upper
172 100
171 35.6 28.1 42.1
170 23.7 18.6 27.8

Manual Integrations
APPROVED



mohammad
10/11/2021 2:13:24 PM

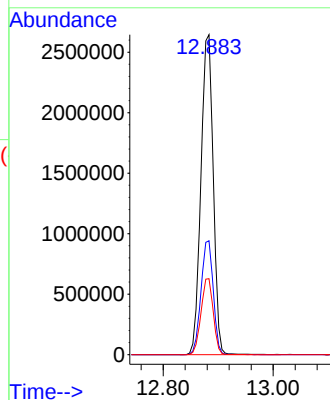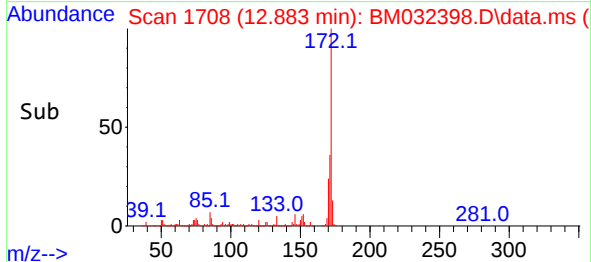


#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.989 min Scan# 2406
Delta R.T. -0.006 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

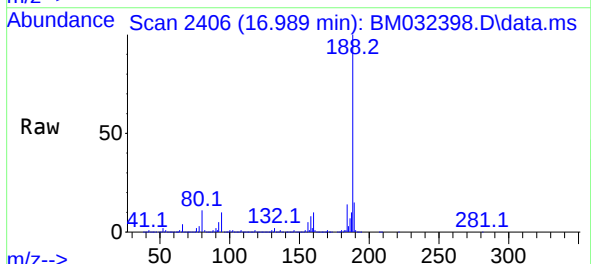


Tgt Ion:188 Resp: 1922913
Ion Ratio Lower Upper
188 100
94 9.7 6.3 9.5#
80 10.6 7.3 10.9

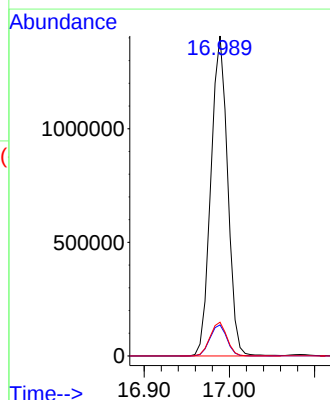






#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.153 min Scan# 3114
Delta R.T. -0.006 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

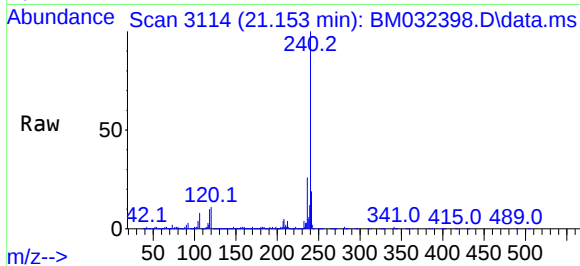


Tgt Ion:240 Resp: 1835531

Ion	Ratio	Lower	Upper
240	100		
120	11.2	7.8	11.6
236	25.9	20.9	31.3

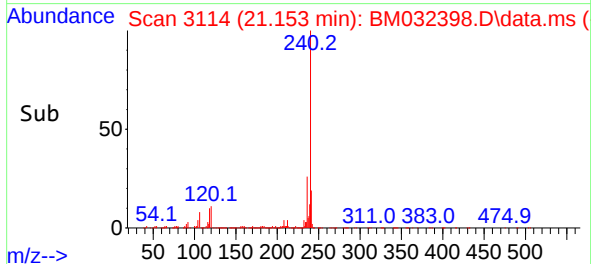
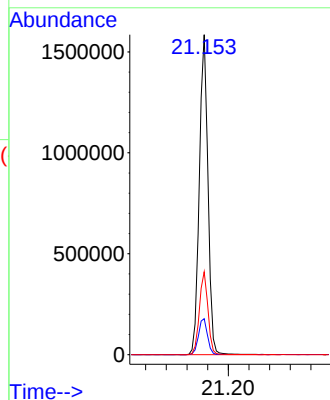


#79
Terphenyl-d14
Concen: 63.20 ng
RT: 19.606 min Scan# 2851
Delta R.T. 0.000 min
Lab File: BM032398.D
Acq: 08 Oct 2021 18:05

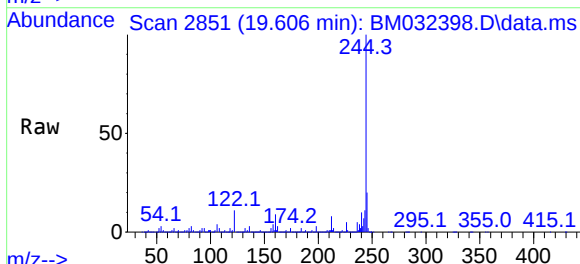

Tgt Ion:244 Resp: 5507972


Ion	Ratio	Lower	Upper
244	100		
212	7.9	6.5	9.7
122	11.4	8.7	13.1

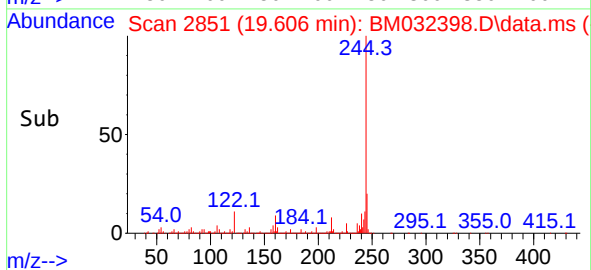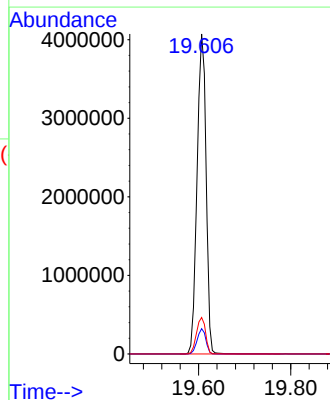

Instrument :
BNA_M
ClientSampleId :
55TH-ST-33


Manual Integrations
APPROVED

mohammad
10/11/2021 2:13:24 PM



#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 23.294 min Scan# 3478
 Delta R.T. -0.006 min
 Lab File: BM032398.D
 Acq: 08 Oct 2021 18:05

Instrument :
 BNA_M
 ClientSampleId :
 55TH-ST-33



Tgt Ion:264 Resp: 1587169

Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.3	28.9
265	21.9	18.3	27.5

Manual Integrations
 APPROVED

mohammad
 10/11/2021 2:13:24 PM

