

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
 Data File : BM032395.D
 Acq On : 08 Oct 2021 16:10
 Operator : CG/JU
 Sample : PB139742BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB139742BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.690	310	315	327	rBV	804837	1134518	7.35%	1.577%
2	5.190	394	400	416	rBV	3959011	5631579	36.51%	7.826%
3	6.808	668	675	690	rBV	3783197	5859159	37.98%	8.142%
4	7.613	806	812	829	rBV	1157989	1845815	11.97%	2.565%
5	8.772	1001	1009	1021	rBV	3448703	5475061	35.49%	7.608%
6	10.407	1279	1287	1298	rBV	1615058	2637533	17.10%	3.665%
7	12.884	1701	1708	1721	rBV	8095396	12043192	78.07%	16.735%
8	14.266	1936	1943	1951	rBV	2480335	3512704	22.77%	4.881%
9	15.748	2188	2195	2211	rBV	4233375	5846190	37.90%	8.124%
10	16.989	2400	2406	2419	rBV	3052794	4143157	26.86%	5.757%
11	19.607	2845	2851	2856	rBV	11166172	15426687	100.00%	21.437%
12	21.154	3109	3114	3127	rBV	3594029	4381081	28.40%	6.088%
13	23.301	3473	3479	3489	rVB2	2356619	4027026	26.10%	5.596%




Sum of corrected areas: 71963702

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
Data File : BM032395.D
Acq On : 08 Oct 2021 16:10
Operator : CG/JU
Sample : PB139742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139742BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

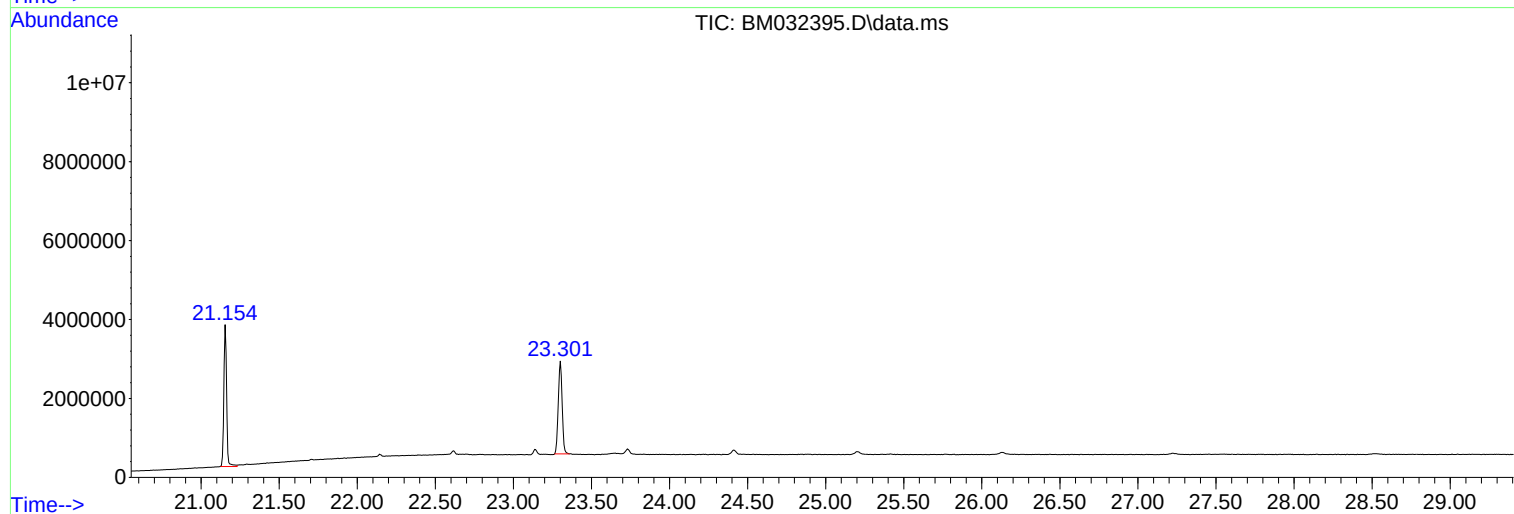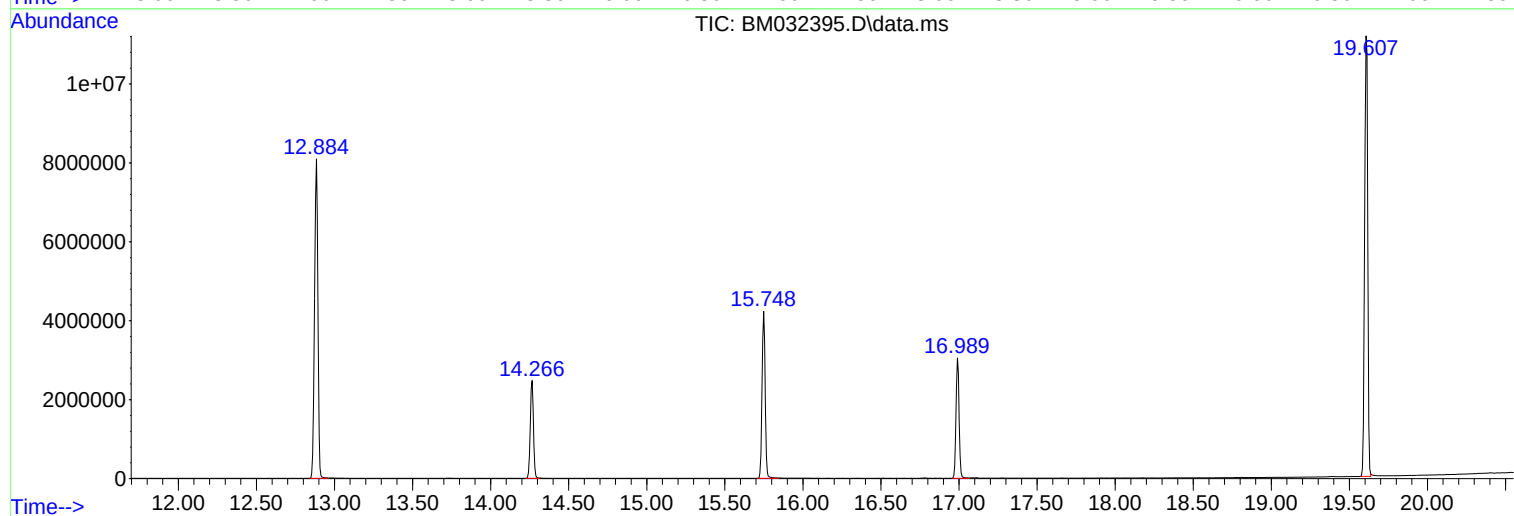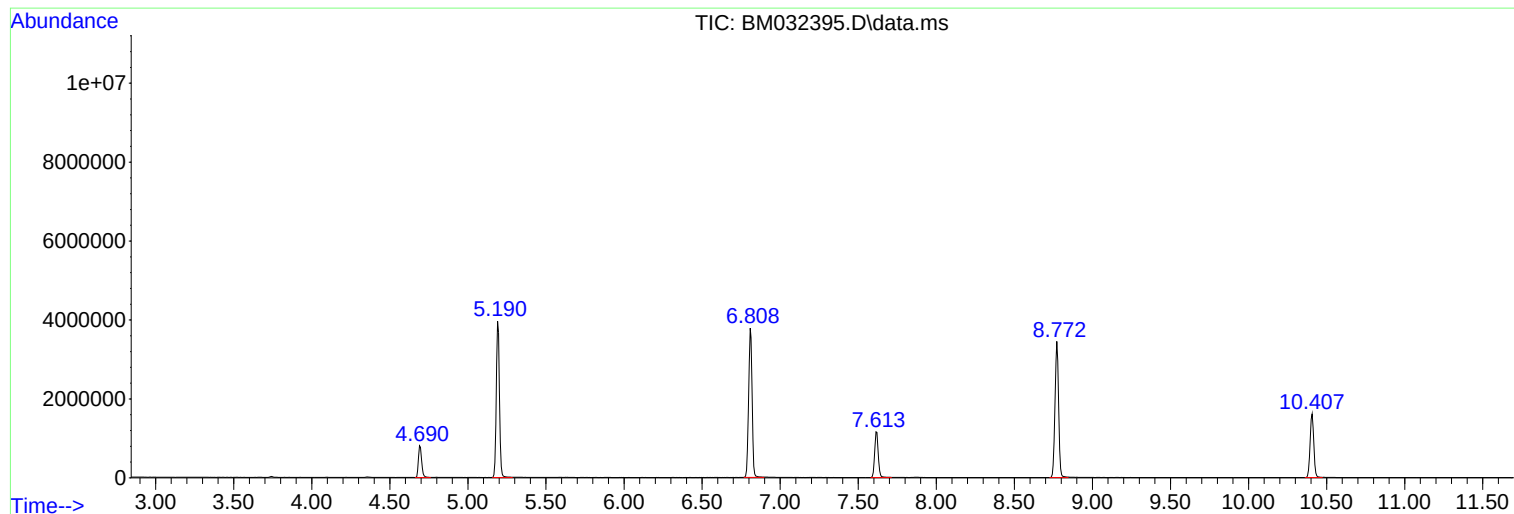

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
Data File : BM032395.D
Acq On : 08 Oct 2021 16:10
Operator : CG/JU
Sample : PB139742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139742BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.690	12.29 ng	1134520	1,4-Dichlorobenzene-d4	7.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9		

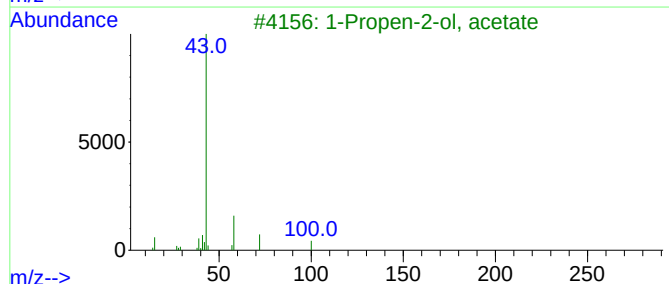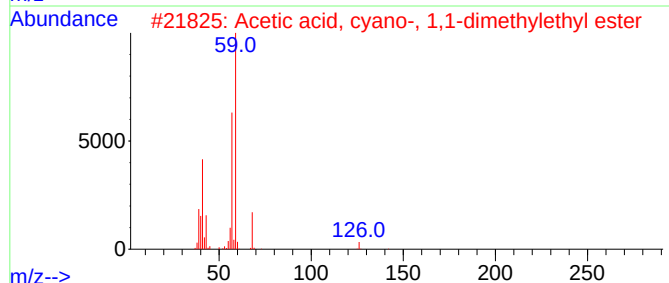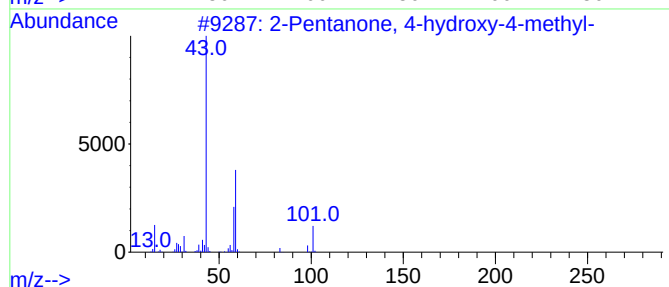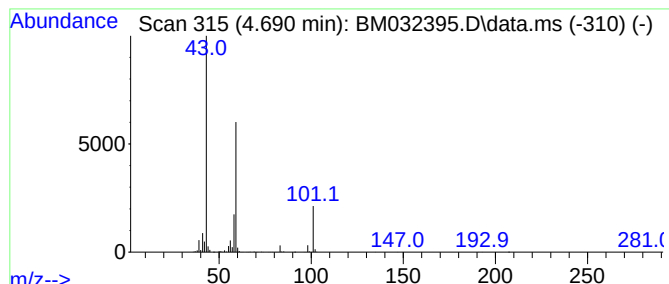

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
Data File : BM032395.D
Acq On : 08 Oct 2021 16:10
Operator : CG/JU
Sample : PB139742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139742BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.690	12.3	ng	1134520	1	7.619	1845820	20.0