
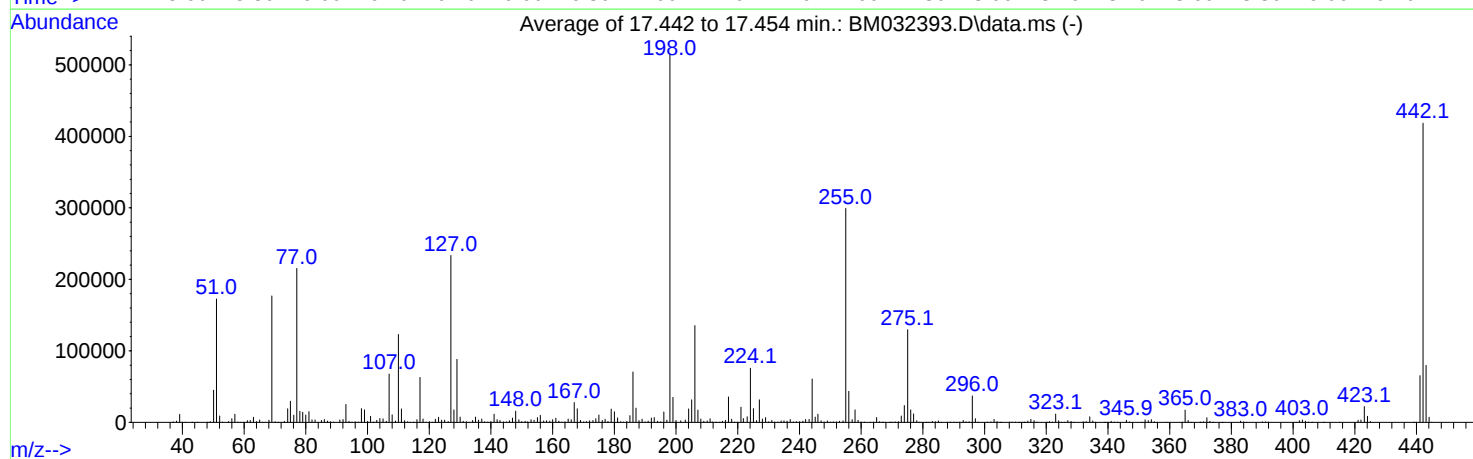


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
 Data File : BM032393.D
 Acq On : 08 Oct 2021 14:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 08 17:11:04 2021

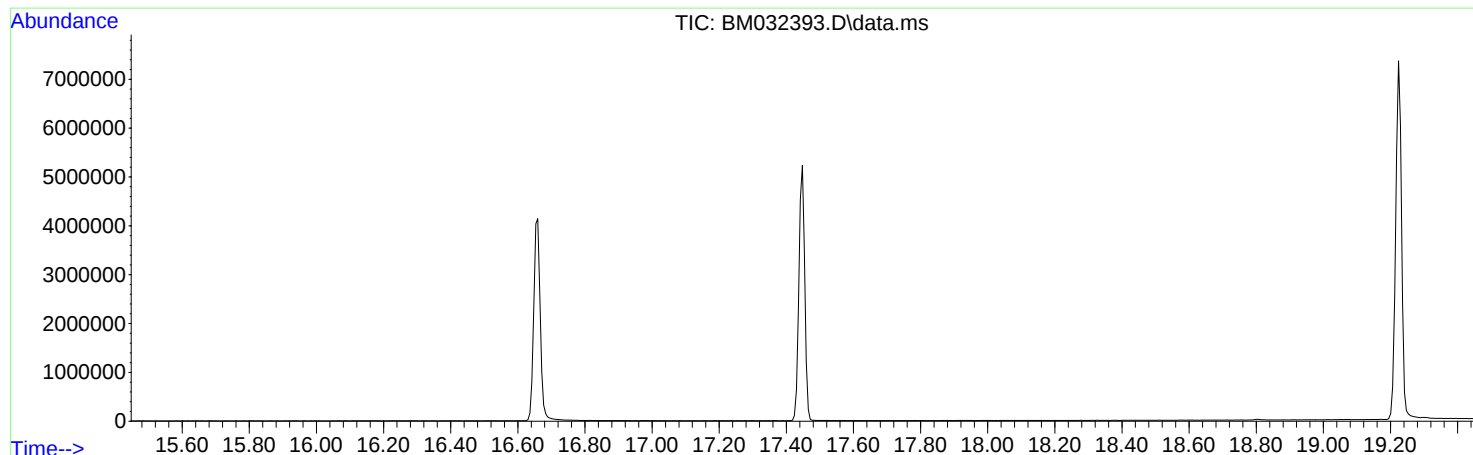




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	172479	PASS
68	69	0.00	2	1.8	3198	PASS
69	198	0.00	100	34.4	176736	PASS
70	69	0.00	2	0.5	958	PASS
127	198	10	80	45.4	233365	PASS
197	198	0.00	2	0.6	3044	PASS
198	198	100	100	100.0	514475	PASS
199	198	5	9	6.8	35035	PASS
275	198	10	60	25.2	129605	PASS
365	198	1	100	3.3	17186	PASS
441	198	0.01	100	12.7	65267	PASS
442	442	50	100	100.0	418389	PASS
443	442	15	24	19.0	79603	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
 Data File : BM032393.D
 Acq On : 08 Oct 2021 14:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Oct 08 17:06:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 18:34:58 2021
 Response via : Initial Calibration

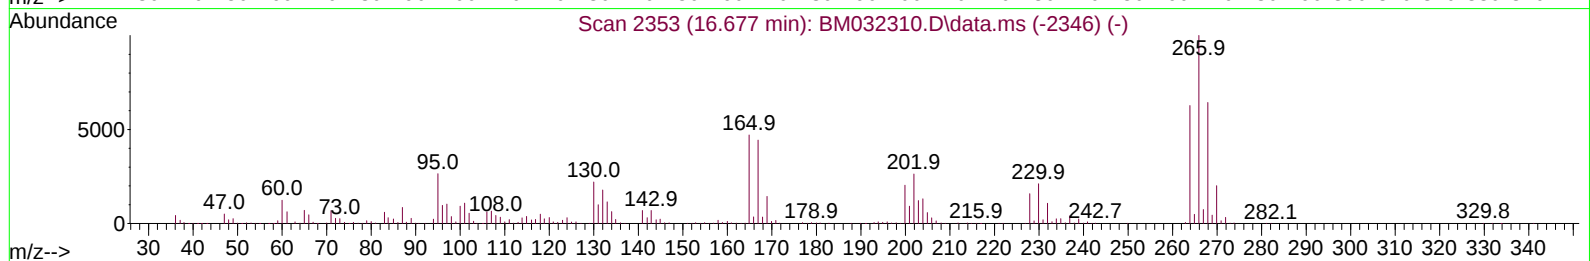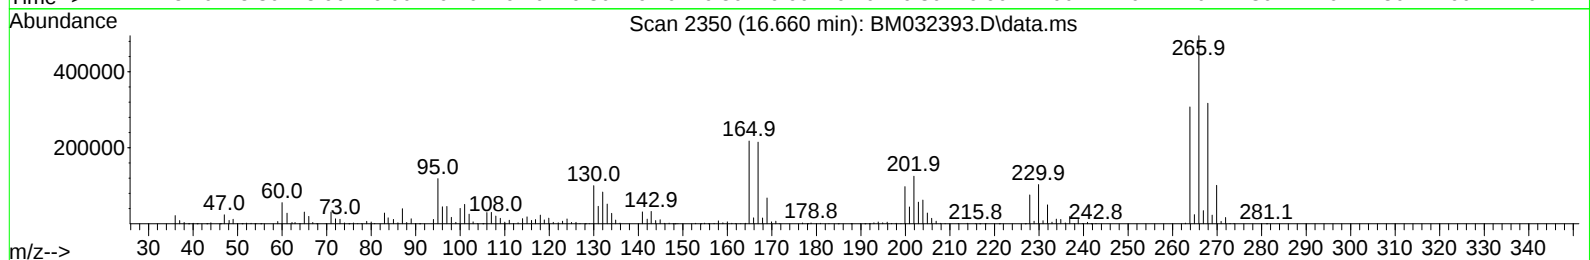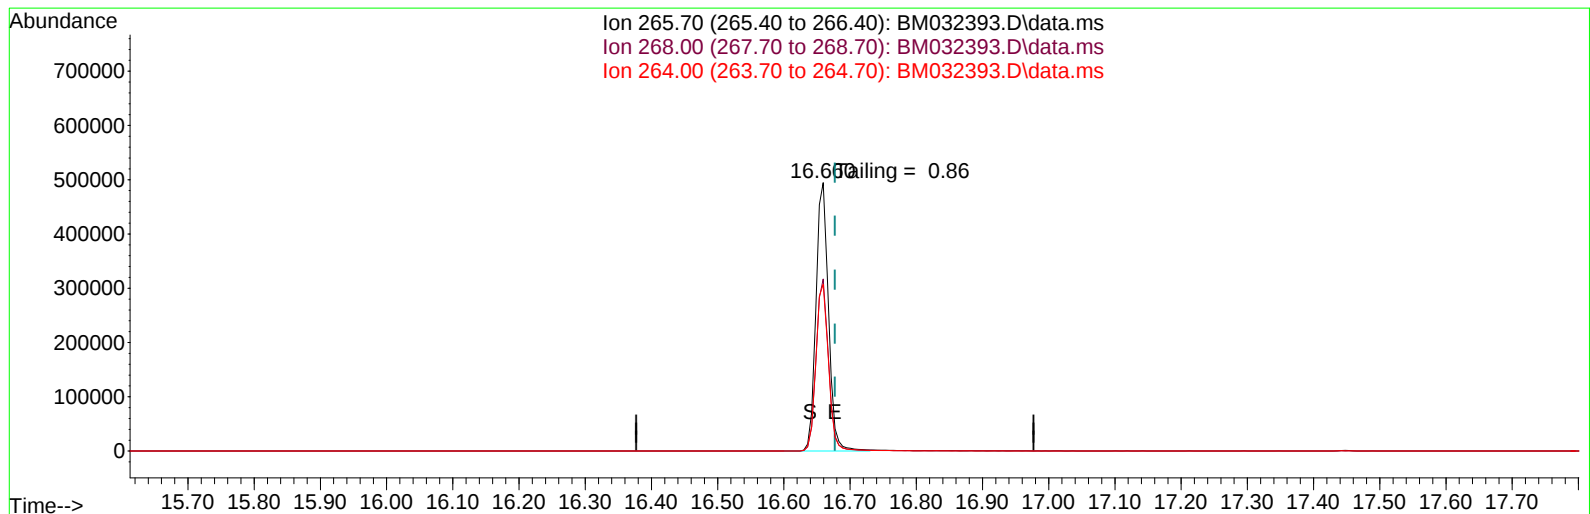

TIC: BM032393.D\data.ms

(70) Pentachlorophenol (C)

16.660min (-0.018) 1263797.82 ng




response 652390

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.12
264.00	65.10	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100921\
Data File : BM032393.D
Acq On : 08 Oct 2021 14:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 08 17:06:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 18:34:58 2021
Response via : Initial Calibration

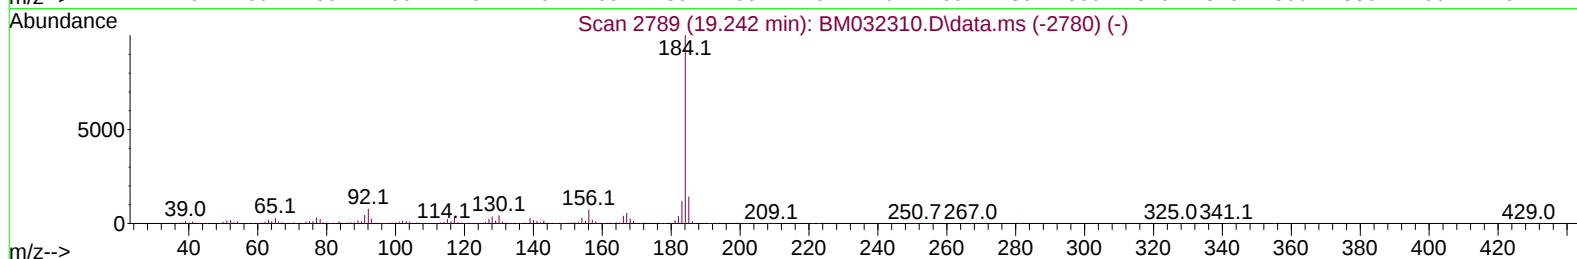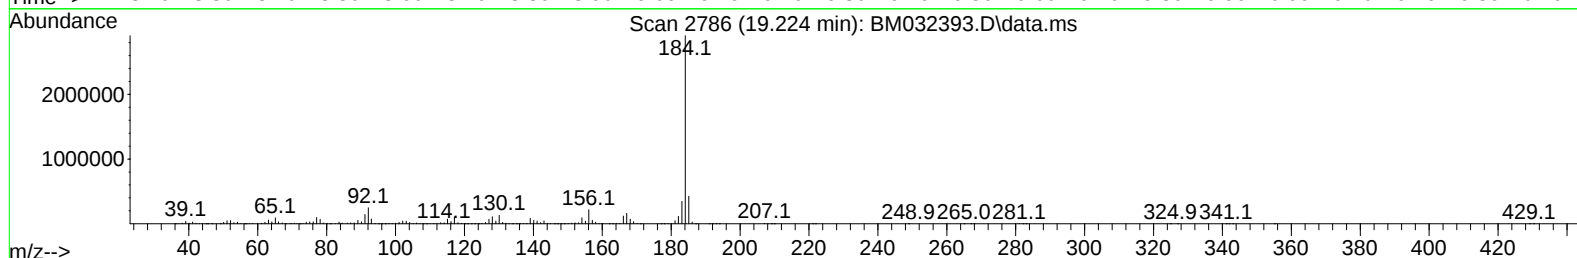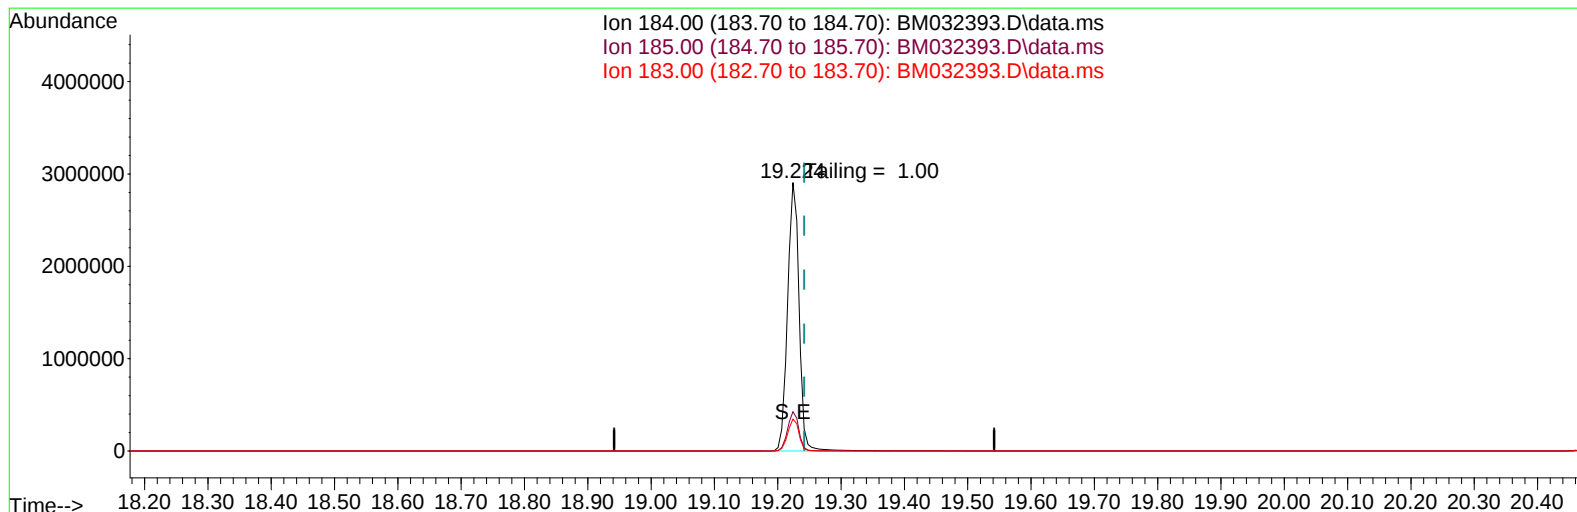

TIC: BM032393.D\data.ms

(77) Benzidine

19.224min (-0.018) 593999.81 ng

response 3674138

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.66
183.00	11.20	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/9/2021	BNA_M	<u>BM032393.D</u>
Compound Name	Response	Retention Time
DDT	1723881	20.45
DDD	21626	20.02
DDE	1322	19.52
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22948	1746829	1.31