

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047943.D
 Acq On : 09 Oct 2024 12:48
 Operator : RC/JU
 Sample : PB163684BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK684

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	54	rVB	73579	107515	1.91%	0.185%
2	3.657	110	114	129	rBV	897822	1365945	24.33%	2.344%
3	3.987	167	170	174	rVB	14131	17877	0.32%	0.031%
4	6.681	625	628	634	rBV8	3104	5909	0.11%	0.010%
5	6.963	667	676	685	rBV	943747	1563995	27.85%	2.684%
6	7.122	696	703	714	rVB	778266	1215985	21.66%	2.087%
7	7.322	731	737	747	rBV	991973	1607126	28.62%	2.758%
8	7.792	809	817	826	rBV	942040	1521816	27.10%	2.612%
9	8.281	896	900	904	rBV7	4034	8518	0.15%	0.015%
10	8.498	927	937	952	rBV	1183535	1887235	33.61%	3.239%
11	8.945	1005	1013	1021	rBV	863536	1442951	25.70%	2.477%
12	9.375	1082	1086	1092	rVB6	9970	18965	0.34%	0.033%
13	9.663	1127	1135	1144	rBV	692052	1180859	21.03%	2.027%
14	9.880	1170	1172	1177	rVB5	4167	6236	0.11%	0.011%
15	9.975	1184	1188	1193	rBV6	3992	8541	0.15%	0.015%
16	10.204	1219	1227	1241	rBV	1069240	1842171	32.81%	3.162%
17	10.580	1283	1291	1300	rBV	1225182	2075576	36.96%	3.562%
18	10.716	1305	1314	1331	rBV	1064038	1879405	33.47%	3.226%
19	11.874	1506	1511	1513	rBV6	4891	6742	0.12%	0.012%
20	12.174	1558	1562	1568	rBV4	16621	28873	0.51%	0.050%
21	12.386	1593	1598	1603	rBV7	3621	8009	0.14%	0.014%
22	13.833	1837	1844	1856	rBV	1675384	2330736	41.51%	4.000%
23	14.115	1884	1892	1905	rBV	2046265	3065617	54.59%	5.261%
24	14.427	1938	1945	1953	rBV	1779045	2619984	46.66%	4.497%
25	14.627	1971	1979	2000	rBV	749016	1289691	22.97%	2.213%
26	14.845	2011	2016	2022	rVB9	11214	21399	0.38%	0.037%
27	15.227	2075	2081	2084	rBV8	4314	7881	0.14%	0.014%
28	15.415	2106	2113	2126	rBV	2536614	3646467	64.94%	6.258%
29	15.533	2127	2133	2142	rBV	762100	1075600	19.15%	1.846%
30	15.657	2150	2154	2158	rVB4	14032	18089	0.32%	0.031%
31	15.986	2204	2210	2213	rVB6	4404	7445	0.13%	0.013%
32	16.198	2243	2246	2251	rBV6	4377	7421	0.13%	0.013%
33	16.951	2372	2374	2382	rVB5	5461	7320	0.13%	0.013%
34	17.162	2403	2410	2419	rBV	2149678	3067154	54.62%	5.264%
35	17.262	2421	2427	2436	rVV	2851985	4019462	71.58%	6.899%
36	17.356	2439	2443	2446	rVB5	4818	7519	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047943.D
Acq On : 09 Oct 2024 12:48
Operator : RC/JU
Sample : PB163684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK684

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	18.056	2557	2562	2572	rBV	145484	282059	5.02%	0.484%
38	19.115	2738	2742	2749	rVB	38051	53294	0.95%	0.091%
39	19.186	2750	2754	2757	rBV2	46976	64774	1.15%	0.111%
40	19.333	2775	2779	2787	rBV2	86885	146468	2.61%	0.251%
41	19.550	2810	2816	2822	rBV	3724203	4958401	88.30%	8.510%
42	21.391	3123	3129	3140	rBV	2564562	3838766	68.36%	6.588%
43	24.174	3594	3602	3613	rVB	2292268	5615253	100.00%	9.637%
44	24.385	3629	3638	3648	rVB	1665440	4314323	76.83%	7.405%




Sum of corrected areas: 58265372

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047943.D
Acq On : 09 Oct 2024 12:48
Operator : RC/JU
Sample : PB163684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

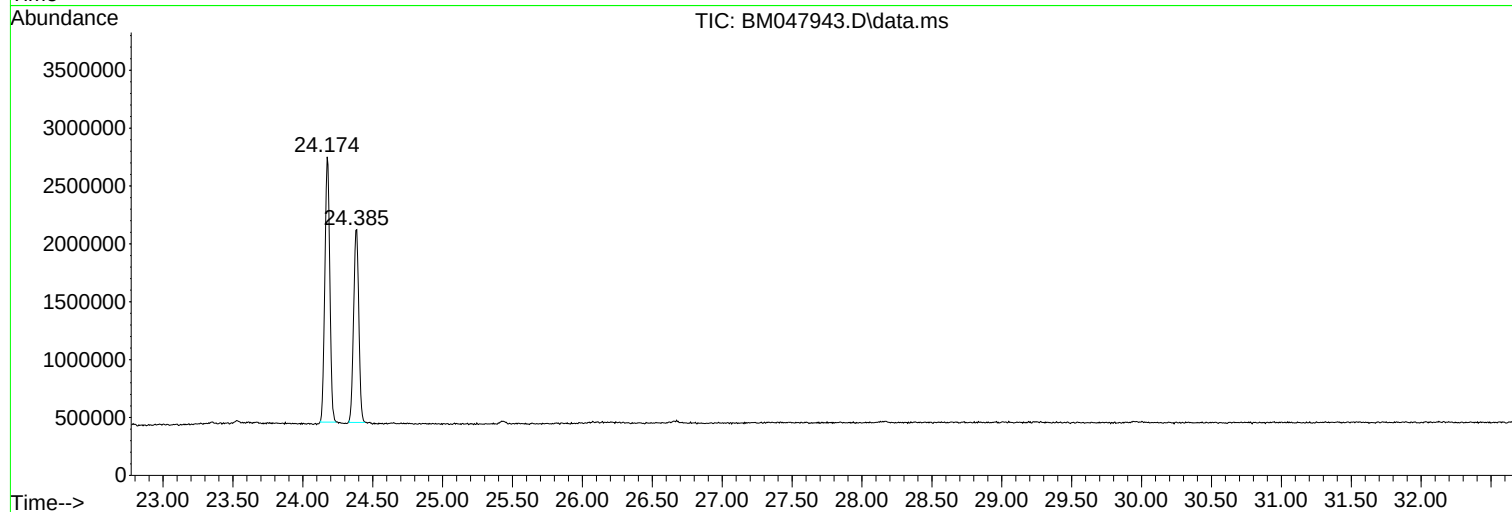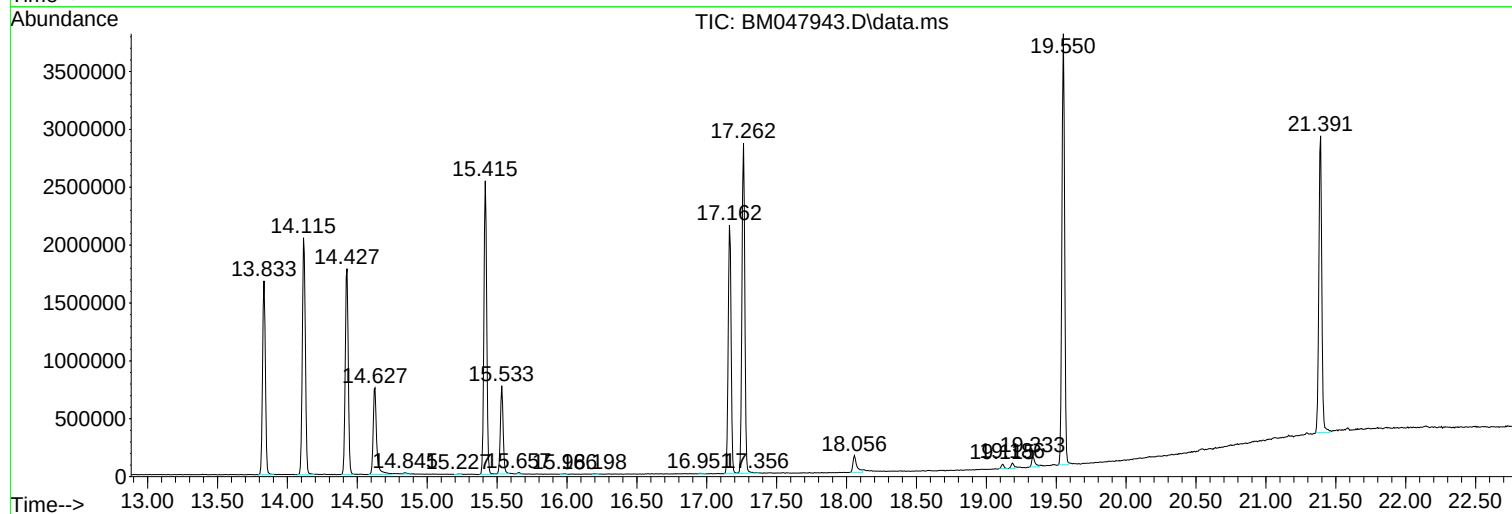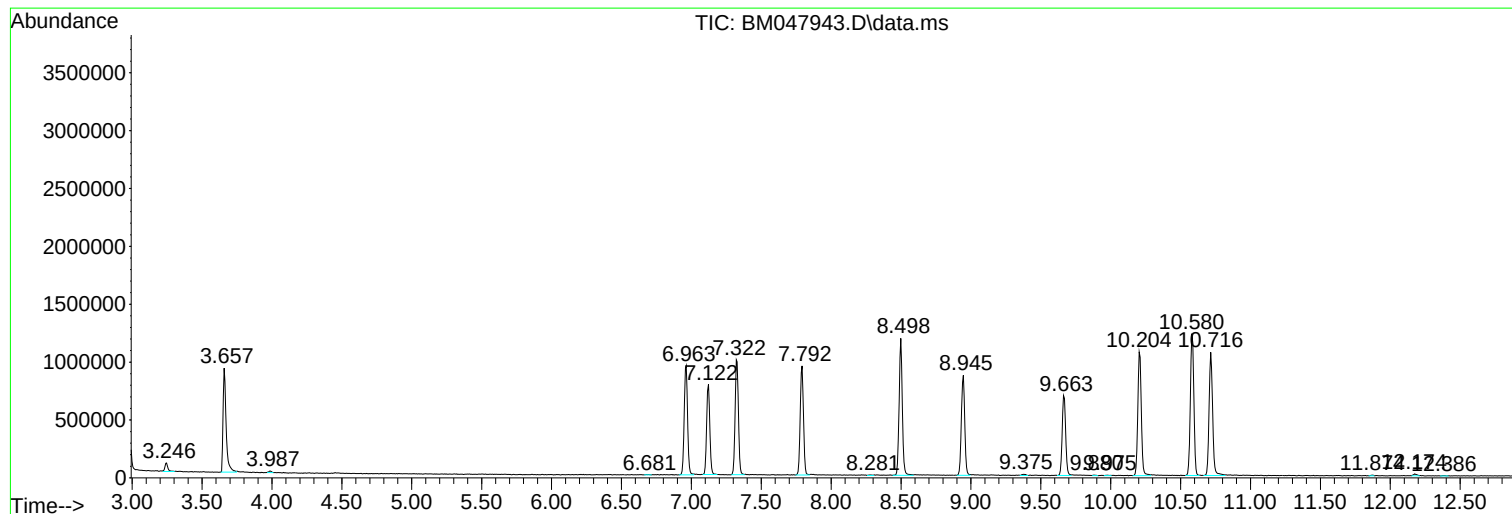

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047943.D
Acq On : 09 Oct 2024 12:48
Operator : RC/JU
Sample : PB163684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047943.D
Acq On : 09 Oct 2024 12:48
Operator : RC/JU
Sample : PB163684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc