

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047944.D
 Acq On : 09 Oct 2024 14:06
 Operator : RC/JU
 Sample : P4187-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY072

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	40	43	51	rVB	49069	67651	1.25%	0.150%
2	3.664	111	115	128	rBV	181802	296069	5.45%	0.654%
3	3.987	166	170	175	rVB	42563	56713	1.04%	0.125%
4	4.511	257	259	267	rVB7	8865	17051	0.31%	0.038%
5	4.781	302	305	311	rVB4	13554	21568	0.40%	0.048%
6	4.905	322	326	334	rVB2	12325	22715	0.42%	0.050%
7	6.052	516	521	529	rVB5	21088	39695	0.73%	0.088%
8	6.958	666	675	689	rBV	222228	387549	7.14%	0.857%
9	7.122	696	703	713	rBV	660727	1068203	19.67%	2.361%
10	7.322	731	737	747	rBV	773353	1243135	22.89%	2.748%
11	7.416	751	753	760	rVB7	7583	10652	0.20%	0.024%
12	7.787	809	816	825	rBV	637030	1055505	19.44%	2.333%
13	7.857	827	828	832	rVB3	7102	6518	0.12%	0.014%
14	8.152	875	878	883	rBV5	7781	11746	0.22%	0.026%
15	8.287	896	901	906	rVB9	6634	12614	0.23%	0.028%
16	8.428	922	925	928	rVB4	4028	5657	0.10%	0.013%
17	8.499	928	937	946	rBV	602328	1033095	19.02%	2.284%
18	8.946	1005	1013	1025	rBV	743571	1267428	23.34%	2.802%
19	9.063	1028	1033	1037	rVV4	3741	6307	0.12%	0.014%
20	9.381	1081	1087	1090	rBV3	18086	28757	0.53%	0.064%
21	9.663	1124	1135	1148	rBV	621021	1046058	19.26%	2.312%
22	10.204	1219	1227	1238	rBV	937260	1582930	29.15%	3.499%
23	10.581	1283	1291	1300	rBV	873647	1433410	26.40%	3.168%
24	10.716	1304	1314	1331	rBV	771587	1416796	26.09%	3.132%
25	11.875	1507	1511	1515	rVB3	7675	10909	0.20%	0.024%
26	12.181	1557	1563	1571	rVB3	14734	26440	0.49%	0.058%
27	12.798	1660	1668	1671	rBV8	3979	9111	0.17%	0.020%
28	13.834	1837	1844	1853	rBV	1489831	2075313	38.22%	4.587%
29	14.116	1883	1892	1901	rBV	1865329	2678711	49.33%	5.921%
30	14.422	1938	1944	1954	rBV	1171049	1786014	32.89%	3.948%
31	14.628	1971	1979	1994	rBV	126548	265380	4.89%	0.587%
32	14.781	2002	2005	2009	rVB5	4353	6518	0.12%	0.014%
33	14.839	2012	2015	2021	rVV8	10666	18578	0.34%	0.041%
34	15.228	2079	2081	2085	rVB4	4922	7161	0.13%	0.016%
35	15.416	2106	2113	2123	rBV	2294987	3257442	59.99%	7.200%
36	15.533	2127	2133	2143	rBV	714391	986737	18.17%	2.181%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047944.D
Acq On : 09 Oct 2024 14:06
Operator : RC/JU
Sample : P4187-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY072

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	15.657	2150	2154	2157	rVB4	11325	15959	0.29%	0.035%
38	16.839	2349	2355	2360	rBV8	5037	10491	0.19%	0.023%
39	17.163	2404	2410	2419	rBV	1465916	2062930	37.99%	4.560%
40	17.263	2419	2427	2437	rBV	2569779	3716837	68.45%	8.216%
41	18.057	2557	2562	2569	rBV2	94914	163783	3.02%	0.362%
42	19.116	2738	2742	2747	rBV2	33331	48302	0.89%	0.107%
43	19.186	2750	2754	2761	rBV	40727	69268	1.28%	0.153%
44	19.333	2775	2779	2786	rBV3	70449	122177	2.25%	0.270%
45	19.551	2810	2816	2828	rBV	3392846	4645666	85.55%	10.269%
46	21.386	3123	3128	3141	rBV2	1692448	2599381	47.87%	5.746%
47	24.174	3594	3602	3619	rVB	2153944	5430314	100.00%	12.003%
48	24.380	3629	3637	3652	rVB	1194499	3088972	56.88%	6.828%




Sum of corrected areas: 45240216

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047944.D
Acq On : 09 Oct 2024 14:06
Operator : RC/JU
Sample : P4187-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

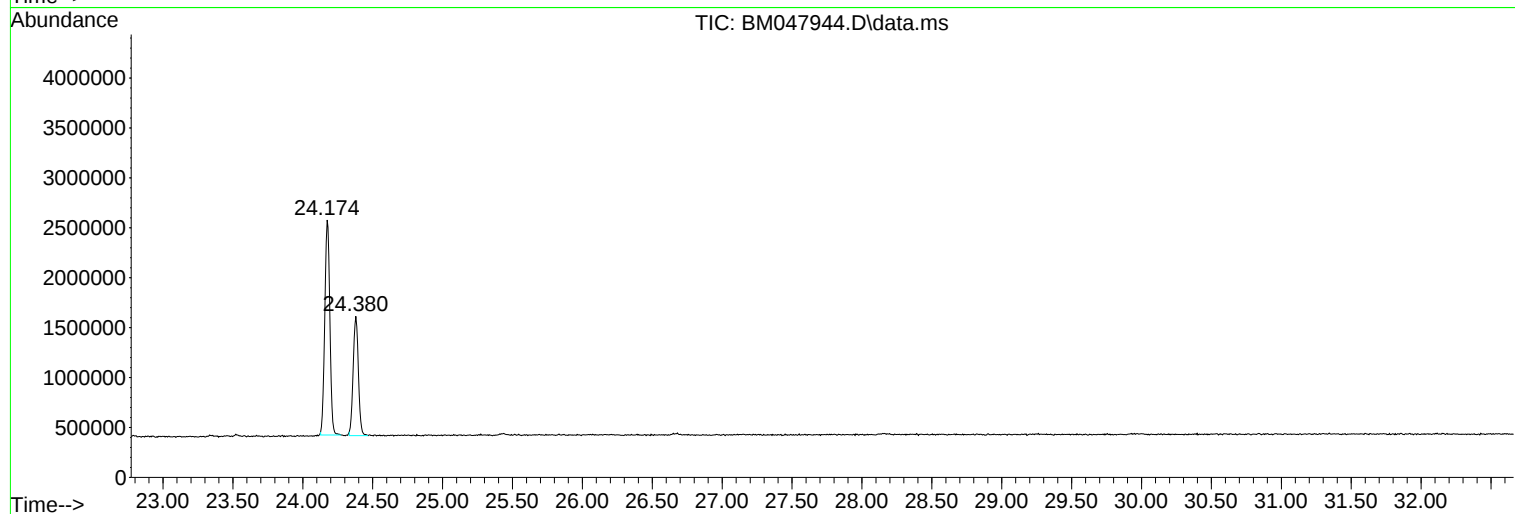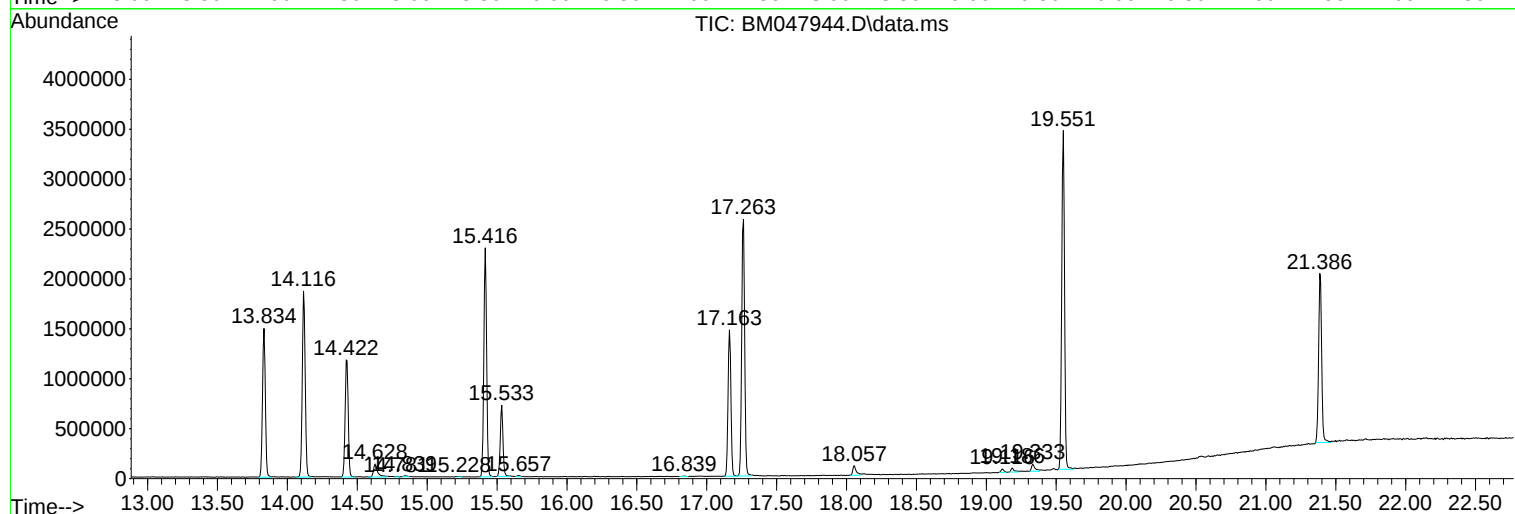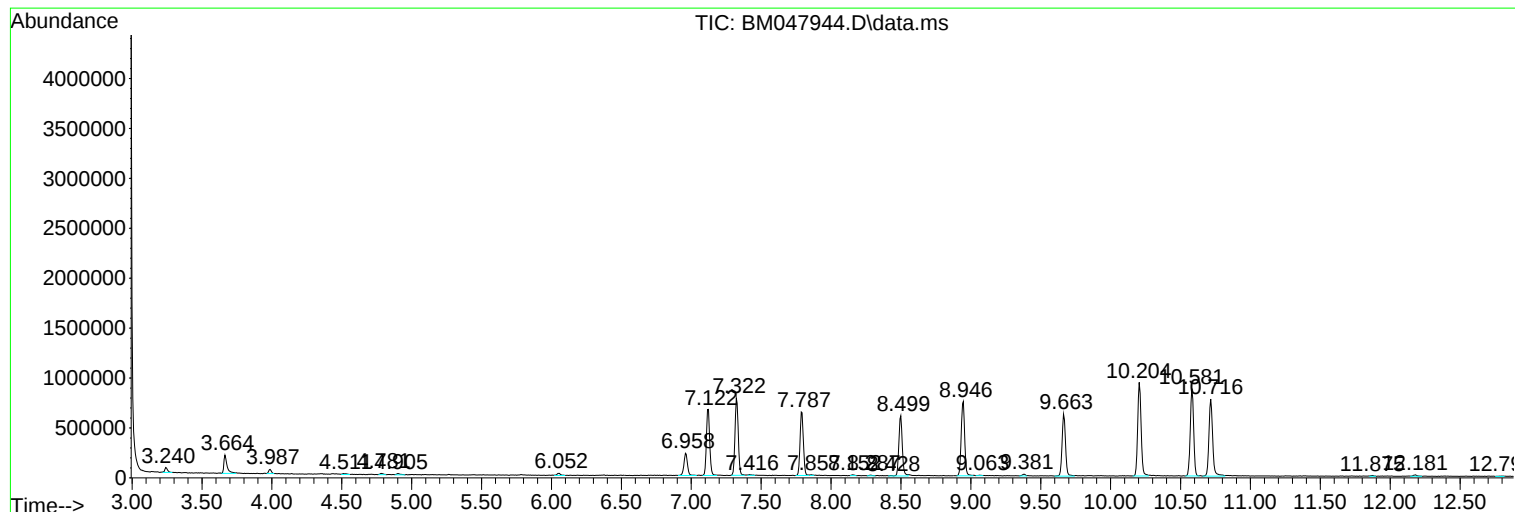

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047944.D
Acq On : 09 Oct 2024 14:06
Operator : RC/JU
Sample : P4187-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047944.D
Acq On : 09 Oct 2024 14:06
Operator : RC/JU
Sample : P4187-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc