

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047949.D
 Acq On : 09 Oct 2024 18:03
 Operator : RC/JU
 Sample : PB163686BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	52	rVB	76114	105036	1.96%	0.186%
2	3.657	110	114	133	rBV	919682	1388274	25.87%	2.459%
3	3.987	167	170	177	rVB	14843	20611	0.38%	0.037%
4	6.957	668	675	684	rBV	966551	1566480	29.19%	2.775%
5	7.122	696	703	716	rBV	769159	1240667	23.12%	2.198%
6	7.322	729	737	748	rBV	1020628	1623403	30.25%	2.876%
7	7.786	809	816	826	rBV	901272	1465783	27.32%	2.596%
8	7.857	826	828	832	rVB5	4785	6092	0.11%	0.011%
9	8.498	929	937	947	rBV	1132605	1878245	35.00%	3.327%
10	8.939	1004	1012	1021	rBV	856481	1466344	27.33%	2.597%
11	9.663	1127	1135	1145	rBV	728025	1201354	22.39%	2.128%
12	10.204	1219	1227	1240	rBV	1068641	1859925	34.66%	3.294%
13	10.580	1283	1291	1299	rBV	1214099	2020167	37.65%	3.578%
14	10.716	1305	1314	1332	rBV	1026363	1900321	35.41%	3.366%
15	11.657	1470	1474	1479	rVB8	2831	5506	0.10%	0.010%
16	12.186	1558	1564	1573	rVB5	11757	27531	0.51%	0.049%
17	13.833	1838	1844	1853	rBV	1664739	2354891	43.88%	4.171%
18	14.115	1884	1892	1907	rBV	2075835	3113197	58.01%	5.514%
19	14.227	1907	1911	1914	rVB5	3456	5863	0.11%	0.010%
20	14.421	1938	1944	1955	rBV	1700249	2531579	47.18%	4.484%
21	14.621	1971	1978	2005	rBV	736174	1282115	23.89%	2.271%
22	15.415	2102	2113	2123	rBV	2579524	3687725	68.72%	6.532%
23	15.533	2127	2133	2145	rVV	784320	1102989	20.55%	1.954%
24	15.657	2149	2154	2160	rVB5	14989	26274	0.49%	0.047%
25	16.945	2370	2373	2379	rVB5	5748	10328	0.19%	0.018%
26	17.162	2404	2410	2420	rBV	2153349	2947426	54.93%	5.221%
27	17.262	2420	2427	2440	rVV	2787177	3995260	74.45%	7.077%
28	18.056	2556	2562	2571	rBV8	19224	46457	0.87%	0.082%
29	19.115	2738	2742	2747	rVB2	35358	44620	0.83%	0.079%
30	19.186	2750	2754	2761	rVV	33134	50778	0.95%	0.090%
31	19.550	2810	2816	2824	rBV	3495313	4833744	90.08%	8.562%
32	21.386	3123	3128	3142	rBV2	2256250	3377088	62.93%	5.982%
33	24.174	3594	3602	3619	rVB	2243277	5366210	100.00%	9.505%
34	24.379	3629	3637	3648	rVB	1533038	3903770	72.75%	6.915%

Sum of corrected areas: 56456053

Instrument :

BNA_M

ClientSampleId :




SBLK686

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047949.D
Acq On : 09 Oct 2024 18:03
Operator : RC/JU
Sample : PB163686BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

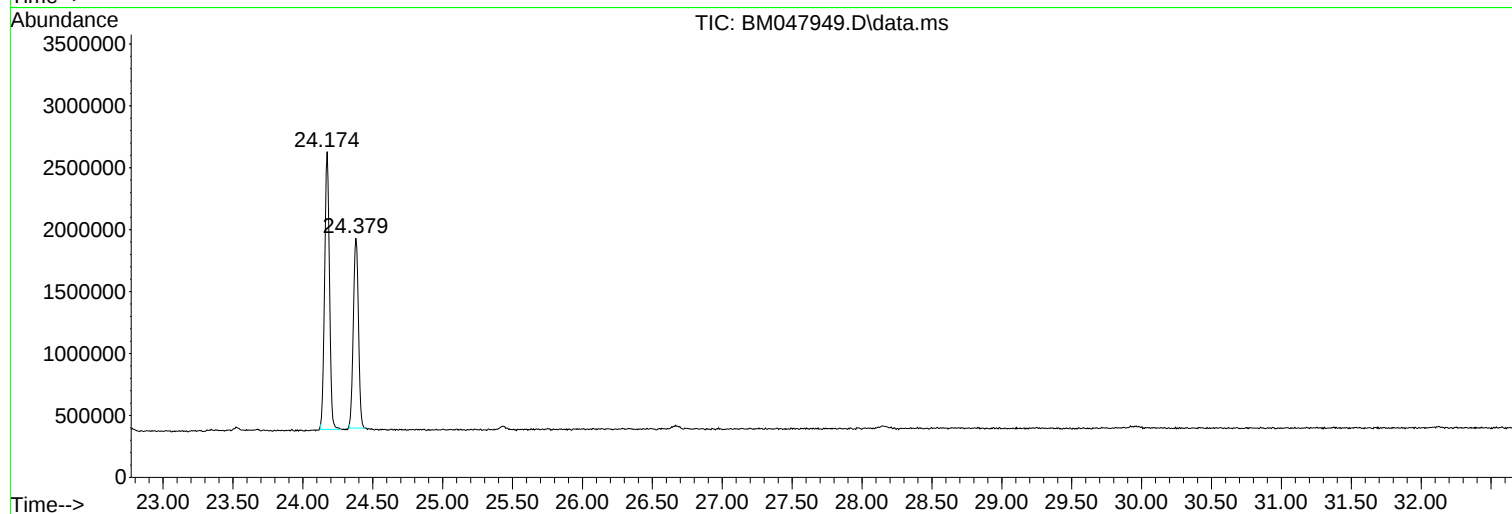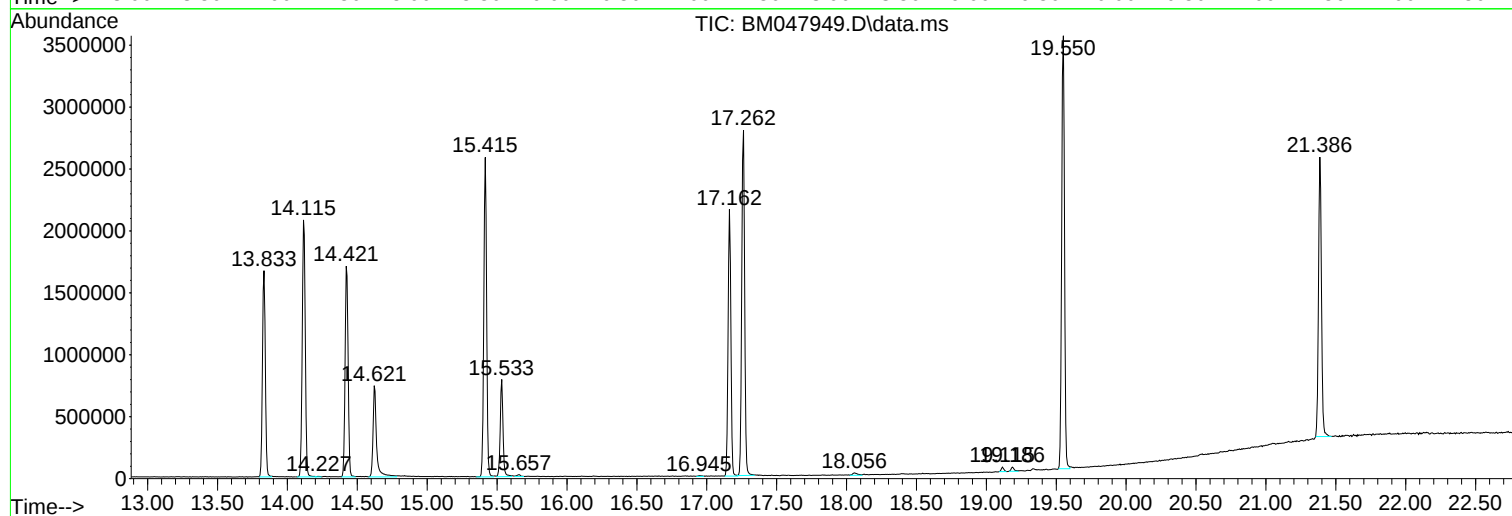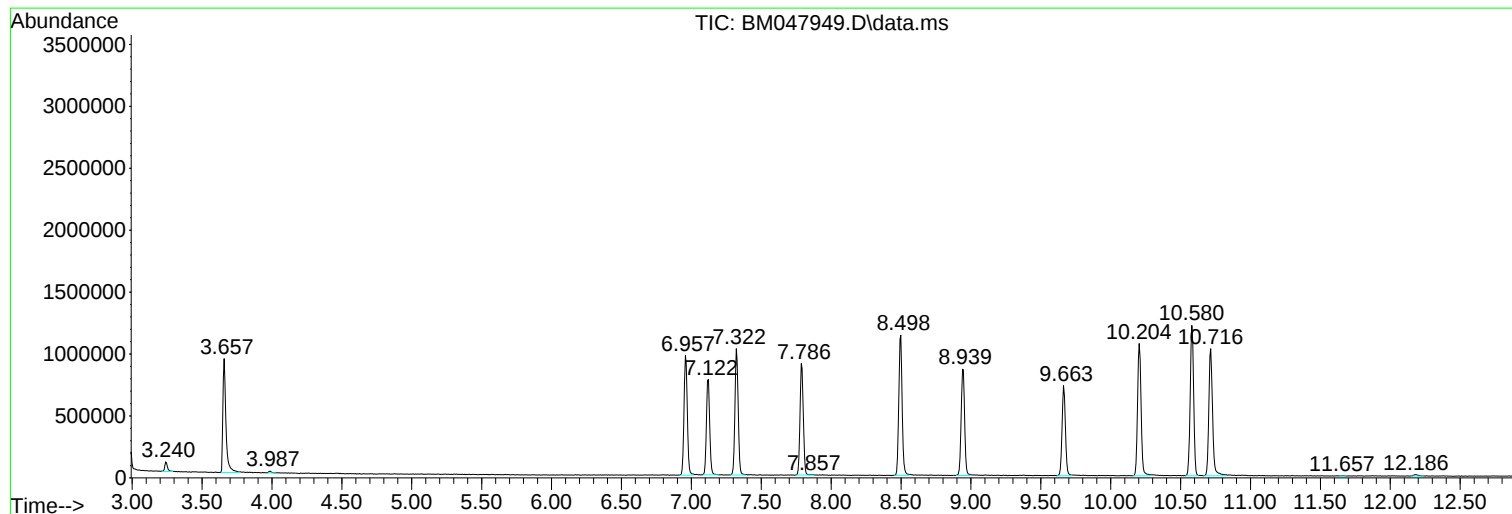

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047949.D
Acq On : 09 Oct 2024 18:03
Operator : RC/JU
Sample : PB163686BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047949.D
Acq On : 09 Oct 2024 18:03
Operator : RC/JU
Sample : PB163686BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc