

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047957.D
 Acq On : 09 Oct 2024 23:19
 Operator : RC/JU
 Sample : P4187-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	47	rBV	54725	68130	1.12%	0.123%
2	3.657	111	114	127	rBV	283899	450269	7.42%	0.814%
3	3.987	167	170	176	rVB	14110	16997	0.28%	0.031%
4	4.434	243	246	249	rVB3	5551	7085	0.12%	0.013%
5	4.781	301	305	310	rVB4	15320	22643	0.37%	0.041%
6	4.910	322	327	335	rVB2	47549	79395	1.31%	0.143%
7	5.804	477	479	484	rVB4	4316	6346	0.10%	0.011%
8	6.051	516	521	527	rVB4	27394	44583	0.74%	0.081%
9	6.957	666	675	688	rBV	332934	566167	9.34%	1.023%
10	7.116	696	702	713	rBV	818964	1307095	21.55%	2.362%
11	7.322	729	737	747	rBV	995918	1594119	26.29%	2.880%
12	7.422	752	754	757	rVB3	7176	6158	0.10%	0.011%
13	7.786	809	816	825	rBV	803967	1285955	21.20%	2.323%
14	8.151	874	878	883	rVB6	8983	14343	0.24%	0.026%
15	8.281	897	900	908	rVB8	7887	13565	0.22%	0.025%
16	8.492	929	936	945	rBV	804902	1339204	22.08%	2.420%
17	8.939	1005	1012	1029	rBV	944622	1569336	25.88%	2.835%
18	9.375	1081	1086	1092	rVB3	13621	20751	0.34%	0.037%
19	9.663	1125	1135	1146	rBV	749396	1284251	21.18%	2.320%
20	10.204	1219	1227	1238	rBV	1134563	1962748	32.36%	3.546%
21	10.298	1242	1243	1248	rVB5	6263	7326	0.12%	0.013%
22	10.580	1284	1291	1300	rBV	1061322	1756916	28.97%	3.174%
23	10.716	1306	1314	1331	rBV	909435	1711029	28.21%	3.091%
24	11.398	1425	1430	1432	rBV6	6427	11473	0.19%	0.021%
25	11.869	1503	1510	1518	rVB4	10390	19978	0.33%	0.036%
26	12.180	1555	1563	1571	rVB4	13169	30797	0.51%	0.056%
27	13.051	1706	1711	1714	rBV3	5120	8154	0.13%	0.015%
28	13.833	1837	1844	1860	rBV	1916137	2743402	45.24%	4.957%
29	14.115	1883	1892	1904	rBV	2285684	3391355	55.92%	6.127%
30	14.421	1937	1944	1954	rBV	1536248	2242356	36.97%	4.051%
31	14.627	1972	1979	1990	rBV	184840	380749	6.28%	0.688%
32	14.839	2011	2015	2023	rVB	11841	20893	0.34%	0.038%
33	15.227	2075	2081	2086	rBV6	7667	14394	0.24%	0.026%
34	15.415	2106	2113	2125	rBV	2919616	4218570	69.56%	7.622%
35	15.527	2126	2132	2145	rVV	890072	1298585	21.41%	2.346%
36	15.651	2149	2153	2159	rVB5	14179	24775	0.41%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047957.D
 Acq On : 09 Oct 2024 23:19
 Operator : RC/JU
 Sample : P4187-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	16.198	2242	2246	2251	rBV5	5274	7768	0.13%	0.014%
38	16.956	2371	2375	2379	rVB5	5445	8186	0.13%	0.015%
39	17.162	2401	2410	2418	rBV	1836506	2610357	43.04%	4.716%
40	17.256	2420	2426	2439	rBV	3147744	4613545	76.07%	8.335%
41	17.833	2521	2524	2526	rBV4	6168	6525	0.11%	0.012%
42	18.051	2557	2561	2569	rVB3	53092	74554	1.23%	0.135%
43	18.392	2616	2619	2622	rBV5	6478	10914	0.18%	0.020%
44	18.545	2641	2645	2649	rBV7	8428	13793	0.23%	0.025%
45	19.115	2737	2742	2748	rBV3	42344	70168	1.16%	0.127%
46	19.186	2750	2754	2758	rBV	43469	59446	0.98%	0.107%
47	19.327	2775	2778	2783	rBV3	42874	56431	0.93%	0.102%
48	19.480	2802	2804	2808	rVB4	16491	14947	0.25%	0.027%
49	19.545	2809	2815	2830	rBV	4018626	5726709	94.43%	10.346%
50	21.386	3122	3128	3139	rBV	1919882	3055410	50.38%	5.520%
51	24.168	3593	3601	3615	rVB	2399669	6064644	100.00%	10.957%
52	24.374	3628	3636	3648	rVB	1329832	3416016	56.33%	6.172%




Sum of corrected areas: 55349305

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047957.D
Acq On : 09 Oct 2024 23:19
Operator : RC/JU
Sample : P4187-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

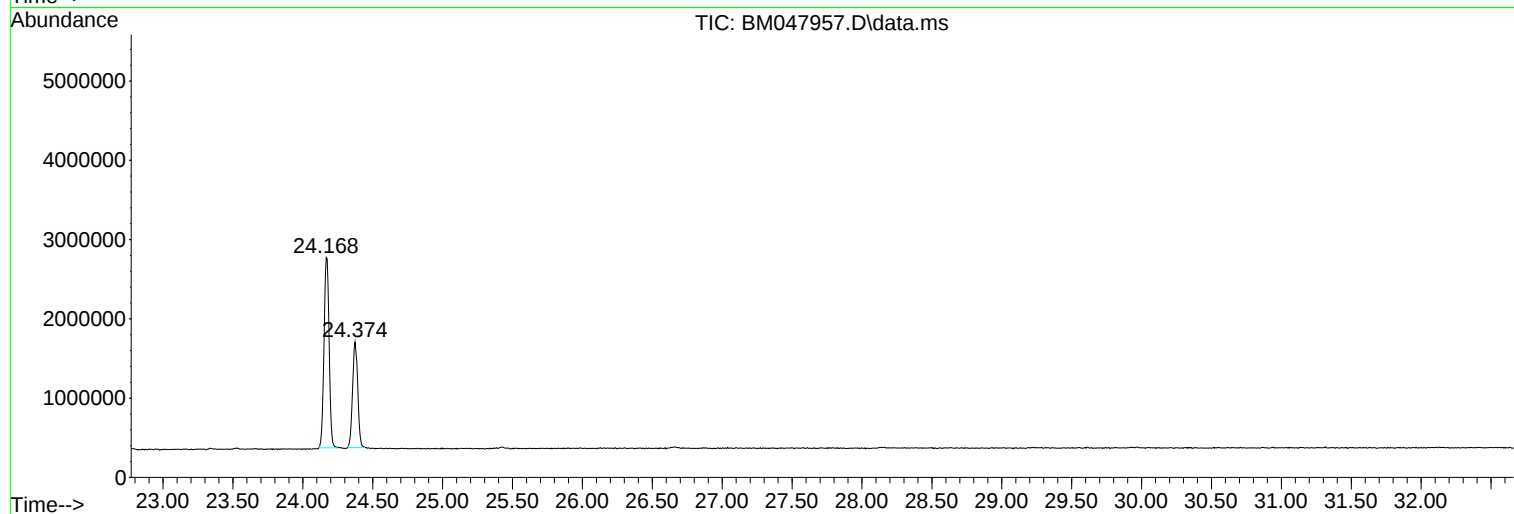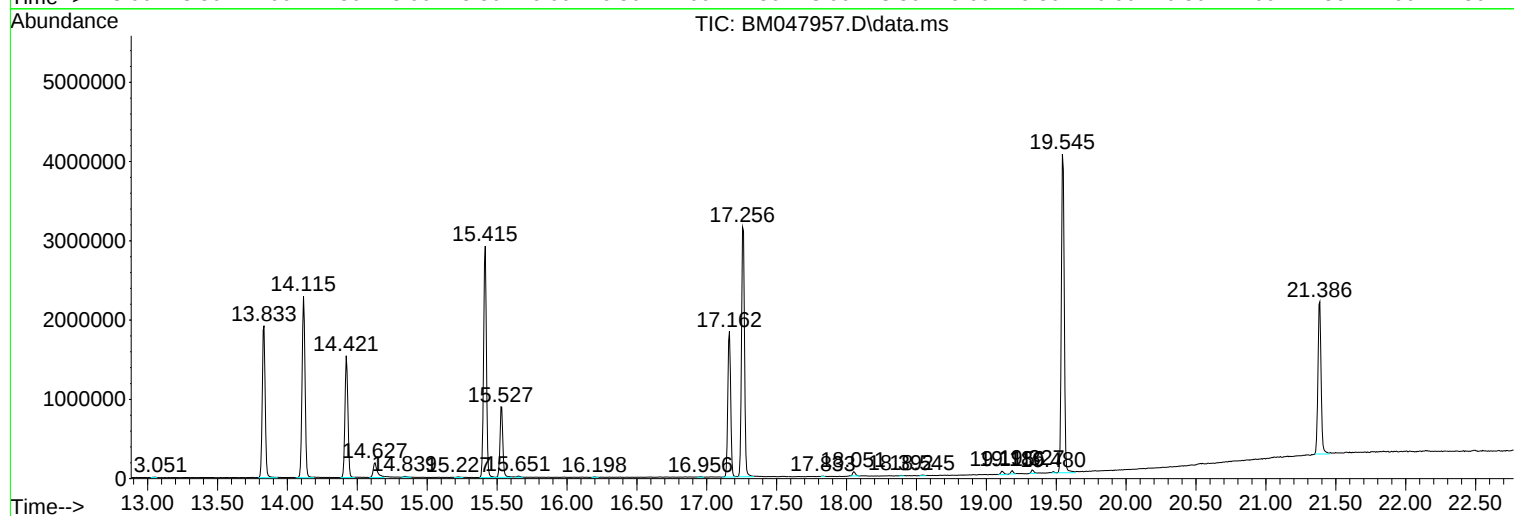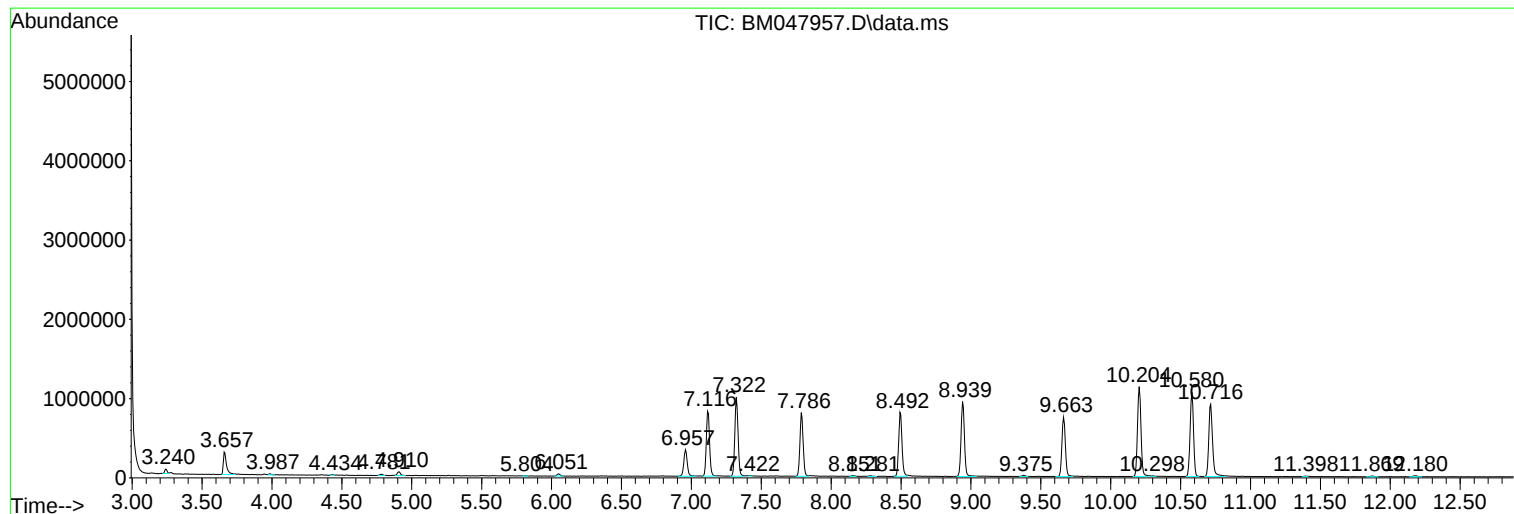

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047957.D
Acq On : 09 Oct 2024 23:19
Operator : RC/JU
Sample : P4187-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047957.D
Acq On : 09 Oct 2024 23:19
Operator : RC/JU
Sample : P4187-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc