

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047965.D
 Acq On : 10 Oct 2024 05:14
 Operator : RC/JU
 Sample : PB163766BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK766

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	54	rVB	71024	101677	2.00%	0.204%
2	3.657	110	114	134	rBV	794715	1226474	24.14%	2.456%
3	3.987	166	170	177	rVB	41279	60128	1.18%	0.120%
4	6.957	667	675	694	rBV	853558	1388232	27.33%	2.780%
5	7.116	696	702	719	rVB	671217	1084312	21.35%	2.172%
6	7.322	729	737	747	rBV	870285	1394570	27.45%	2.793%
7	7.787	809	816	825	rBV	818820	1328009	26.14%	2.660%
8	8.492	929	936	949	rBV	972154	1592448	31.35%	3.189%
9	8.939	1005	1012	1023	rBV	737001	1247843	24.56%	2.499%
10	9.375	1081	1086	1090	rBV5	11057	19797	0.39%	0.040%
11	9.663	1127	1135	1147	rBV	582840	995790	19.60%	1.994%
12	10.204	1219	1227	1238	rBV	893699	1534388	30.21%	3.073%
13	10.581	1283	1291	1300	rBV	1089975	1802730	35.49%	3.610%
14	10.716	1306	1314	1334	rBV	802509	1567014	30.85%	3.138%
15	11.863	1507	1509	1516	rVB4	7045	9677	0.19%	0.019%
16	12.186	1557	1564	1569	rBV6	8084	18253	0.36%	0.037%
17	13.827	1835	1843	1859	rBV	1430184	2083595	41.02%	4.173%
18	14.116	1884	1892	1905	rBV	1748995	2614530	51.47%	5.236%
19	14.204	1905	1907	1914	rVB8	4828	8499	0.17%	0.017%
20	14.421	1937	1944	1955	rBV	1527629	2225756	43.82%	4.458%
21	14.621	1970	1978	2003	rBV	572099	1102029	21.69%	2.207%
22	15.416	2106	2113	2125	rBV	2178926	3166187	62.33%	6.341%
23	15.527	2126	2132	2143	rVV	627083	904901	17.81%	1.812%
24	15.657	2151	2154	2160	rVB5	11872	16008	0.32%	0.032%
25	16.951	2367	2374	2381	rBV8	6375	13623	0.27%	0.027%
26	17.162	2402	2410	2419	rBV	1821766	2591508	51.02%	5.190%
27	17.257	2420	2426	2442	rVB	2541471	3585699	70.59%	7.181%
28	19.115	2738	2742	2745	rBV2	24396	33348	0.66%	0.067%
29	19.186	2750	2754	2758	rBV	27656	36938	0.73%	0.074%
30	19.545	2809	2815	2828	rBV	3280443	4498207	88.55%	9.009%
31	21.380	3122	3127	3137	rBV	1973121	3100268	61.03%	6.209%
32	24.168	3592	3601	3619	rVB	2055785	5079762	100.00%	10.173%
33	24.368	3627	3635	3648	rVB	1329650	3499541	68.89%	7.009%




Sum of corrected areas: 49931741

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047965.D
Acq On : 10 Oct 2024 05:14
Operator : RC/JU
Sample : PB163766BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

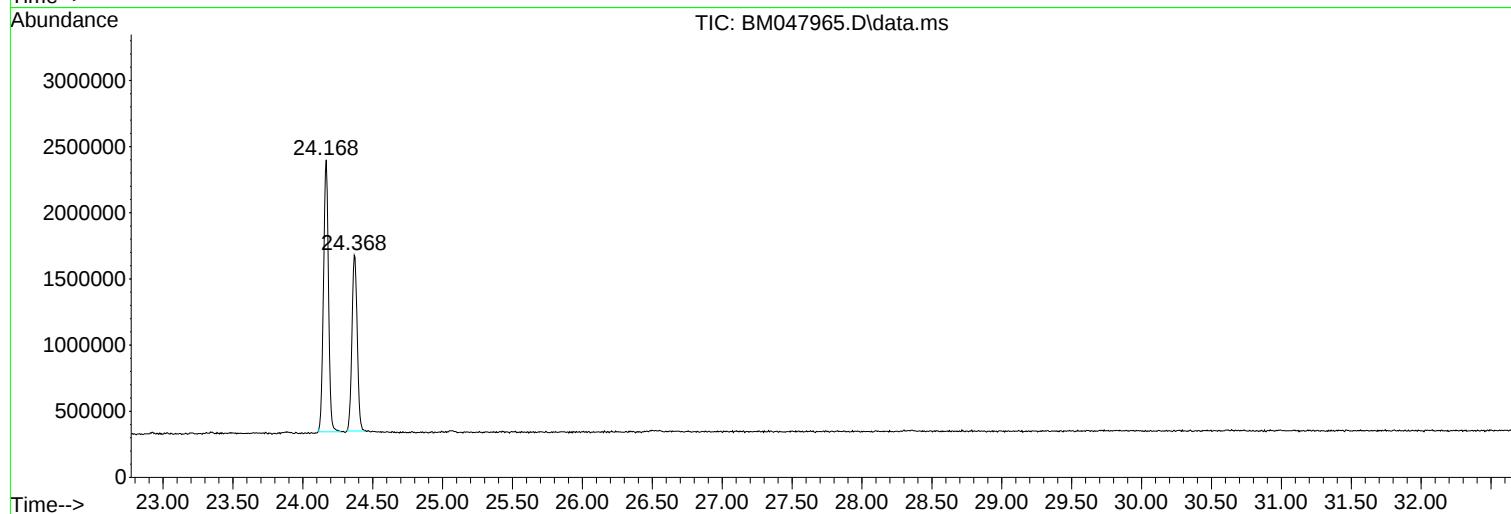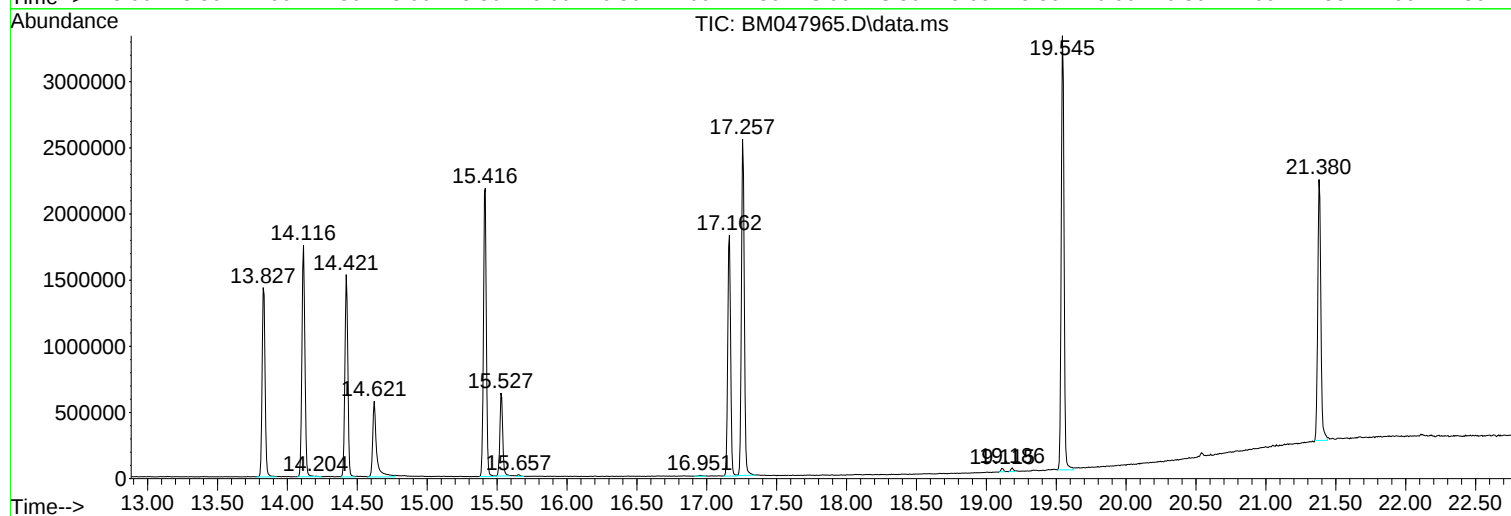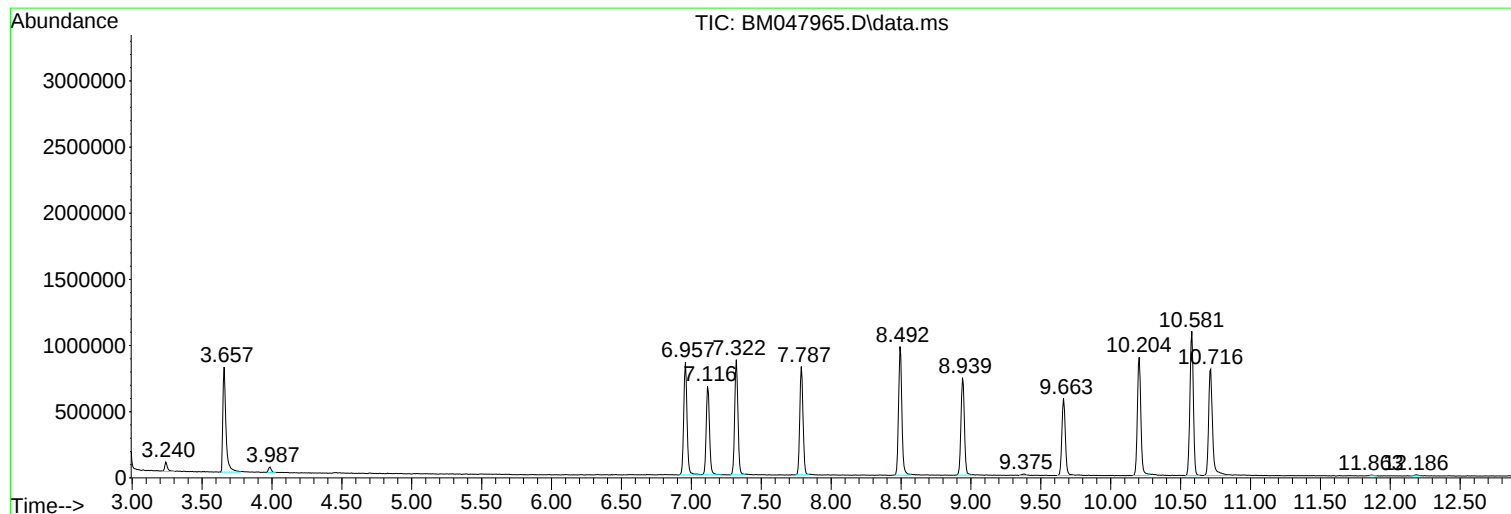

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047965.D
Acq On : 10 Oct 2024 05:14
Operator : RC/JU
Sample : PB163766BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047965.D
Acq On : 10 Oct 2024 05:14
Operator : RC/JU
Sample : PB163766BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc