

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047969.D
 Acq On : 10 Oct 2024 07:52
 Operator : RC/JU
 Sample : P4215-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	46	rBV	61957	77557	1.17%	0.134%
2	3.275	46	49	56	rVB	57800	82124	1.24%	0.142%
3	3.663	111	115	129	rBV2	308675	599365	9.02%	1.038%
4	3.981	167	169	174	rVB	13416	17133	0.26%	0.030%
5	4.781	301	305	312	rVB3	15422	21660	0.33%	0.038%
6	4.899	321	325	329	rVB3	12067	16095	0.24%	0.028%
7	5.587	440	442	449	rVB5	4494	6711	0.10%	0.012%
8	6.051	516	521	528	rVB3	27357	46155	0.69%	0.080%
9	6.363	571	574	579	rVB6	6976	12134	0.18%	0.021%
10	6.957	668	675	686	rBV	283986	485324	7.31%	0.841%
11	7.116	696	702	717	rBV	827272	1330824	20.04%	2.305%
12	7.322	730	737	746	rBV	901869	1470378	22.14%	2.547%
13	7.610	780	786	791	rVB8	3932	8972	0.14%	0.016%
14	7.787	809	816	825	rBV	878734	1404841	21.15%	2.433%
15	8.157	874	879	882	rBV6	8344	14381	0.22%	0.025%
16	8.275	898	899	905	rVB6	7485	9154	0.14%	0.016%
17	8.492	929	936	951	rBV	812429	1359288	20.46%	2.354%
18	8.798	981	988	989	rBV7	5244	7865	0.12%	0.014%
19	8.939	1004	1012	1022	rBV	944201	1584183	23.85%	2.744%
20	9.375	1082	1086	1092	rVB6	7300	12347	0.19%	0.021%
21	9.516	1104	1110	1115	rBV5	13637	25963	0.39%	0.045%
22	9.663	1128	1135	1144	rBV	730213	1248281	18.79%	2.162%
23	10.204	1219	1227	1240	rBV	1091689	1905237	28.68%	3.300%
24	10.581	1282	1291	1298	rBV	1119043	1908771	28.74%	3.306%
25	10.710	1304	1313	1335	rBV	877827	1698737	25.58%	2.942%
26	12.169	1556	1561	1569	rBV3	12042	24585	0.37%	0.043%
27	13.827	1836	1843	1856	rBV	1932389	2676545	40.30%	4.636%
28	13.957	1862	1865	1869	rBV6	3716	6694	0.10%	0.012%
29	14.116	1883	1892	1904	rBV	2243689	3329145	50.12%	5.766%
30	14.421	1937	1944	1952	rBV	1626047	2354058	35.44%	4.077%
31	14.627	1970	1979	1999	rBV	123826	314934	4.74%	0.545%
32	14.845	2011	2016	2020	rVB8	8684	13570	0.20%	0.024%
33	15.063	2047	2053	2054	rBV5	6077	11314	0.17%	0.020%
34	15.227	2076	2081	2086	rBV9	6565	10319	0.16%	0.018%
35	15.415	2104	2113	2126	rBV	2818644	4143137	62.38%	7.176%
36	15.527	2126	2132	2149	rVV	922477	1290106	19.42%	2.235%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047969.D
 Acq On : 10 Oct 2024 07:52
 Operator : RC/JU
 Sample : P4215-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	15.657	2149	2154	2157	rVB5	15388	24123	0.36%	0.042%
38	15.774	2168	2174	2185	rBV	157449	228578	3.44%	0.396%
39	16.133	2232	2235	2239	rBV5	4784	7193	0.11%	0.012%
40	16.339	2268	2270	2276	rVB7	4999	7842	0.12%	0.014%
41	17.162	2403	2410	2419	rBV	1946932	2720054	40.95%	4.711%
42	17.257	2420	2426	2436	rBV	3379595	4767909	71.78%	8.258%
43	17.545	2470	2475	2480	rBV9	7881	17679	0.27%	0.031%
44	17.633	2486	2490	2496	rBV3	13108	21045	0.32%	0.036%
45	17.827	2520	2523	2529	rVB8	12860	20188	0.30%	0.035%
46	18.051	2556	2561	2569	rBV2	162747	248044	3.73%	0.430%
47	18.380	2615	2617	2620	rBV4	6608	7210	0.11%	0.012%
48	18.539	2641	2644	2647	rBV5	7776	11989	0.18%	0.021%
49	19.115	2737	2742	2746	rBV2	45050	70016	1.05%	0.121%
50	19.180	2749	2753	2757	rBV	46174	71438	1.08%	0.124%
51	19.327	2775	2778	2782	rBV4	57812	71878	1.08%	0.124%
52	19.545	2809	2815	2829	rBV	4432689	6015091	90.56%	10.419%
53	21.062	3070	3073	3080	rBV6	70930	105496	1.59%	0.183%
54	21.380	3122	3127	3139	rBV	2148696	3256922	49.03%	5.641%
55	24.168	3592	3601	3620	rVB	2718997	6642103	100.00%	11.505%
56	24.368	3627	3635	3654	rVB	1444111	3891538	58.59%	6.740%




Sum of corrected areas: 57734223

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047969.D
Acq On : 10 Oct 2024 07:52
Operator : RC/JU
Sample : P4215-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY027

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

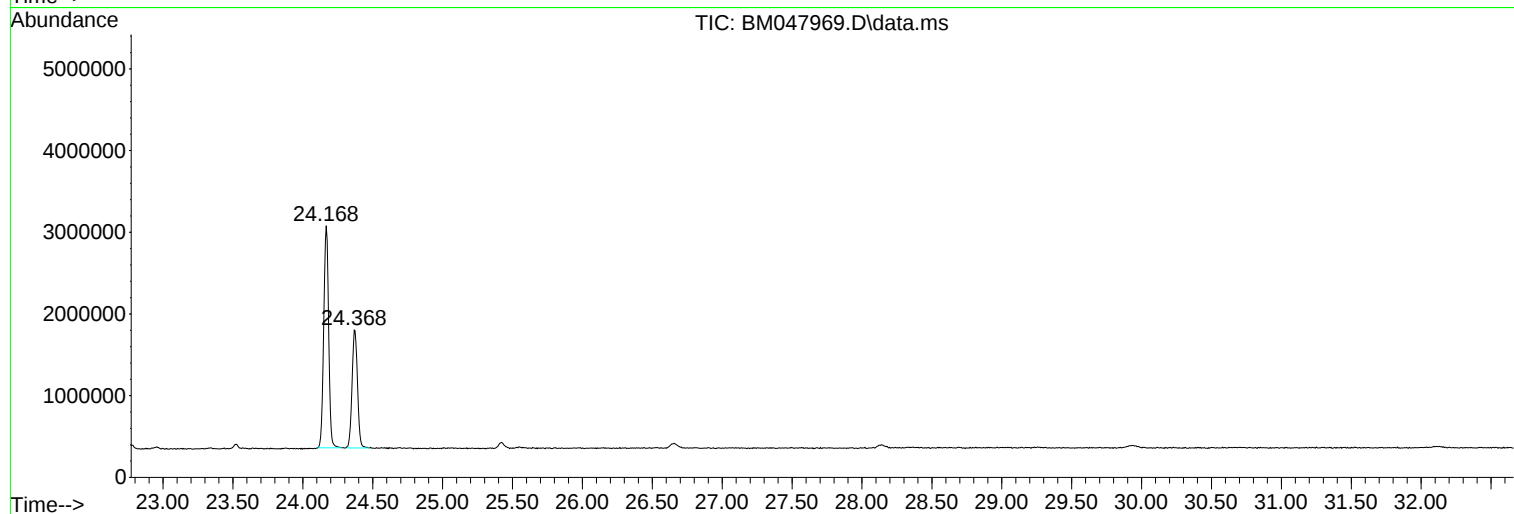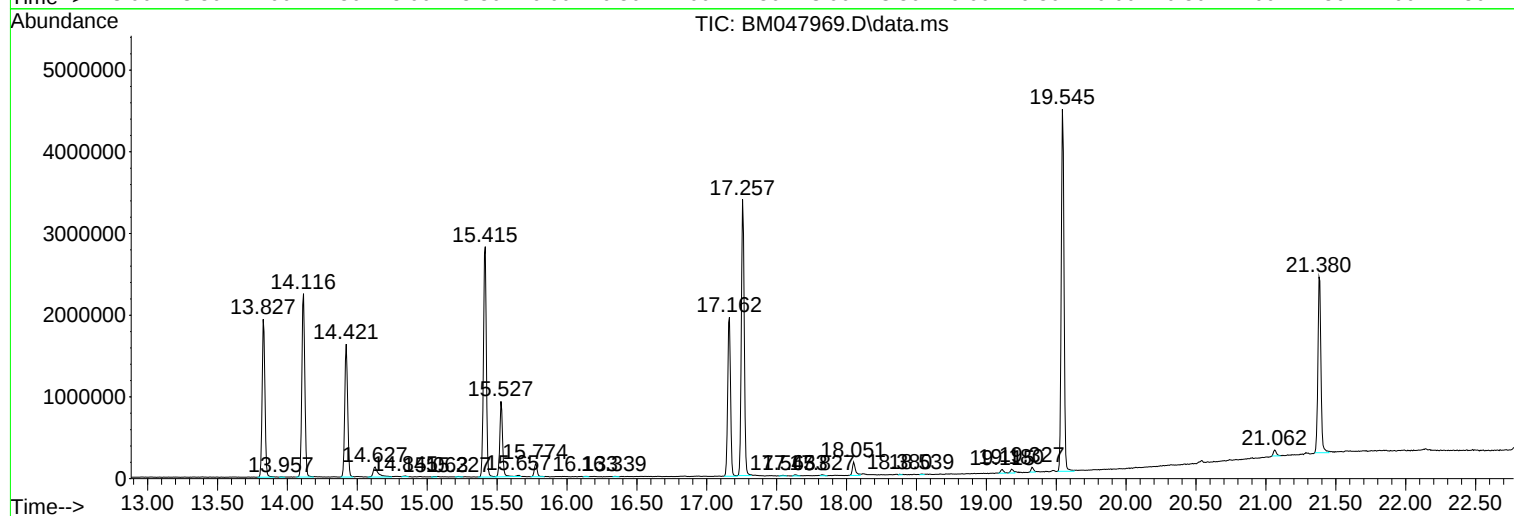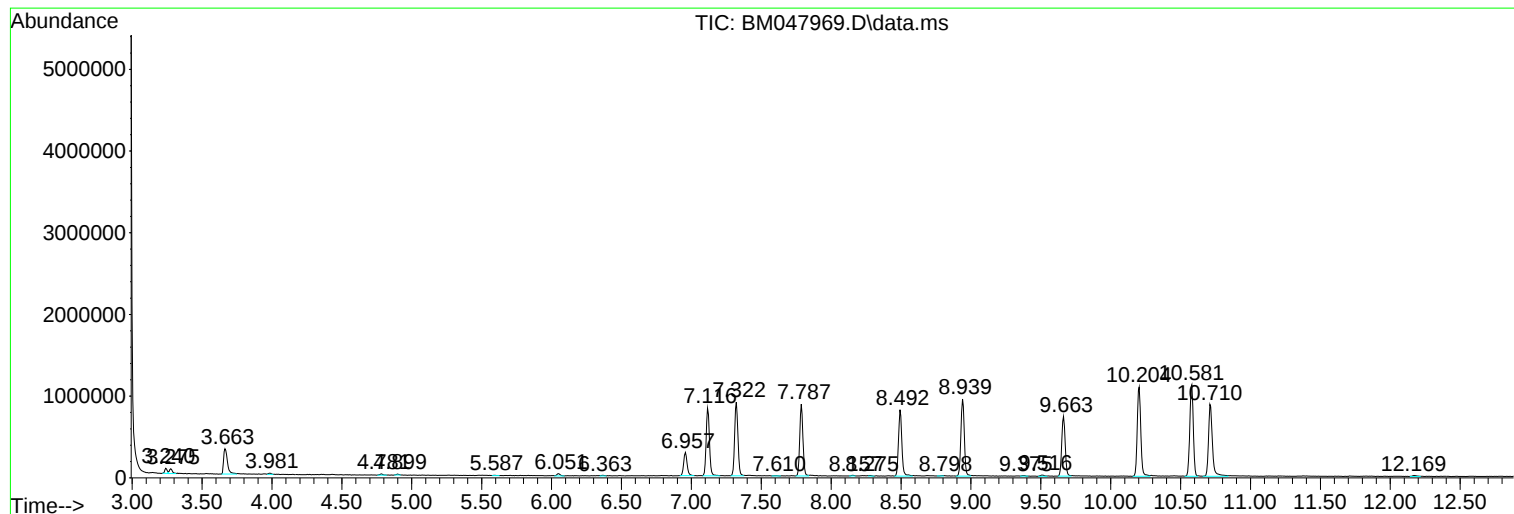

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047969.D
Acq On : 10 Oct 2024 07:52
Operator : RC/JU
Sample : P4215-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY027

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047969.D
Acq On : 10 Oct 2024 07:52
Operator : RC/JU
Sample : P4215-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY027

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc