

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047970.D
 Acq On : 10 Oct 2024 08:31
 Operator : RC/JU
 Sample : P4207-15
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	35	38	40	rBV	21702	24137	0.35%	0.039%
2	3.240	40	43	53	rVB	74467	110161	1.61%	0.178%
3	3.657	110	114	124	rBV	350468	548965	8.04%	0.887%
4	3.981	166	169	176	rVB3	16960	24299	0.36%	0.039%
5	4.428	243	245	251	rVB6	7649	12180	0.18%	0.020%
6	4.510	256	259	263	rBV6	6168	9832	0.14%	0.016%
7	4.781	301	305	313	rVB3	16945	25778	0.38%	0.042%
8	4.899	320	325	332	rVB2	24773	38215	0.56%	0.062%
9	5.381	404	407	412	rBV6	4248	7383	0.11%	0.012%
10	6.046	515	520	525	rBV3	33950	55323	0.81%	0.089%
11	6.363	571	574	578	rVB6	5009	7151	0.10%	0.012%
12	6.875	658	661	665	rBV4	5501	7916	0.12%	0.013%
13	6.957	667	675	689	rVV	454318	772324	11.32%	1.248%
14	7.116	696	702	711	rBV	910515	1416494	20.75%	2.289%
15	7.322	729	737	744	rBV	1091773	1750320	25.64%	2.828%
16	7.428	750	755	760	rVB3	14320	31009	0.45%	0.050%
17	7.787	809	816	824	rBV	924601	1470349	21.54%	2.376%
18	7.898	833	835	840	rVB4	7821	10084	0.15%	0.016%
19	8.157	875	879	883	rVB5	10450	16081	0.24%	0.026%
20	8.275	895	899	904	rVB7	8789	15918	0.23%	0.026%
21	8.334	904	909	911	rBV6	4593	7694	0.11%	0.012%
22	8.434	922	926	928	rBV5	6473	7211	0.11%	0.012%
23	8.492	928	936	945	rBV	1063692	1757897	25.76%	2.841%
24	8.939	1005	1012	1025	rBV	1021890	1700739	24.92%	2.748%
25	9.381	1080	1087	1091	rBV7	6934	14695	0.22%	0.024%
26	9.475	1097	1103	1107	rBV8	4656	7123	0.10%	0.012%
27	9.663	1128	1135	1144	rBV	816327	1383399	20.27%	2.235%
28	9.986	1185	1190	1194	rVB7	4547	7803	0.11%	0.013%
29	10.204	1219	1227	1241	rBV	1236828	2164439	31.71%	3.498%
30	10.581	1283	1291	1301	rBV	1198461	2052220	30.07%	3.316%
31	10.710	1306	1313	1332	rBV	969798	1831040	26.83%	2.959%
32	11.416	1431	1433	1437	rVB5	6341	7366	0.11%	0.012%
33	12.175	1556	1562	1570	rBV4	16608	32268	0.47%	0.052%
34	12.245	1570	1574	1578	rBV6	4678	8791	0.13%	0.014%
35	13.145	1723	1727	1728	rBV4	6603	9697	0.14%	0.016%
36	13.163	1728	1730	1734	rVB4	7130	7292	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
 Data File : BM047970.D
 Acq On : 10 Oct 2024 08:31
 Operator : RC/JU
 Sample : P4207-15
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY054

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	13.392	1761	1769	1770	rBV7	5011	11210	0.16%	0.018%
38	13.492	1783	1786	1792	rVB8	5574	8026	0.12%	0.013%
39	13.710	1819	1823	1828	rBV8	4825	10922	0.16%	0.018%
40	13.827	1834	1843	1854	rBV	2089843	2943230	43.12%	4.756%
41	14.116	1885	1892	1905	rBV	2448507	3656723	53.58%	5.909%
42	14.333	1925	1929	1934	rBV8	7318	13556	0.20%	0.022%
43	14.421	1937	1944	1953	rVV	1725211	2536858	37.17%	4.099%
44	14.516	1957	1960	1963	rVB5	6842	8230	0.12%	0.013%
45	14.621	1972	1978	1993	rBV	258447	524319	7.68%	0.847%
46	14.780	2002	2005	2010	rVV6	6430	9322	0.14%	0.015%
47	14.839	2012	2015	2021	rVB9	11404	20514	0.30%	0.033%
48	14.945	2026	2033	2036	rBV8	9046	17060	0.25%	0.028%
49	14.980	2036	2039	2042	rVB5	7270	8517	0.12%	0.014%
50	15.051	2047	2051	2054	rVB6	6328	8554	0.13%	0.014%
51	15.180	2069	2073	2076	rVB6	6094	7824	0.11%	0.013%
52	15.221	2076	2080	2086	rBV3	10991	18103	0.27%	0.029%
53	15.416	2105	2113	2125	rBV	3108401	4559017	66.80%	7.367%
54	15.527	2125	2132	2143	rBV	1049979	1444232	21.16%	2.334%
55	15.651	2150	2153	2160	rVB5	17421	29709	0.44%	0.048%
56	15.774	2169	2174	2181	rVB2	37870	57205	0.84%	0.092%
57	16.839	2353	2355	2358	rVB3	5736	6984	0.10%	0.011%
58	17.157	2403	2409	2417	rBV	2058382	2909294	42.63%	4.701%
59	17.257	2420	2426	2439	rVV	3543657	5033688	73.75%	8.134%
60	17.539	2469	2474	2479	rBV3	20806	33522	0.49%	0.054%
61	18.051	2556	2561	2569	rBV3	98734	150669	2.21%	0.243%
62	19.109	2737	2741	2748	rVB3	43759	66142	0.97%	0.107%
63	19.180	2749	2753	2758	rBV	46467	78813	1.15%	0.127%
64	19.327	2774	2778	2786	rBV5	54008	92810	1.36%	0.150%
65	19.545	2809	2815	2827	rBV	4515400	6174480	90.47%	9.977%
66	21.380	3122	3127	3140	rBV	2225855	3345824	49.02%	5.406%
67	24.168	3592	3601	3617	rVB	2748808	6825262	100.00%	11.029%
68	24.368	3627	3635	3651	rVB	1530812	3921015	57.45%	6.336%




Sum of corrected areas: 61885227

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047970.D
Acq On : 10 Oct 2024 08:31
Operator : RC/JU
Sample : P4207-15
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

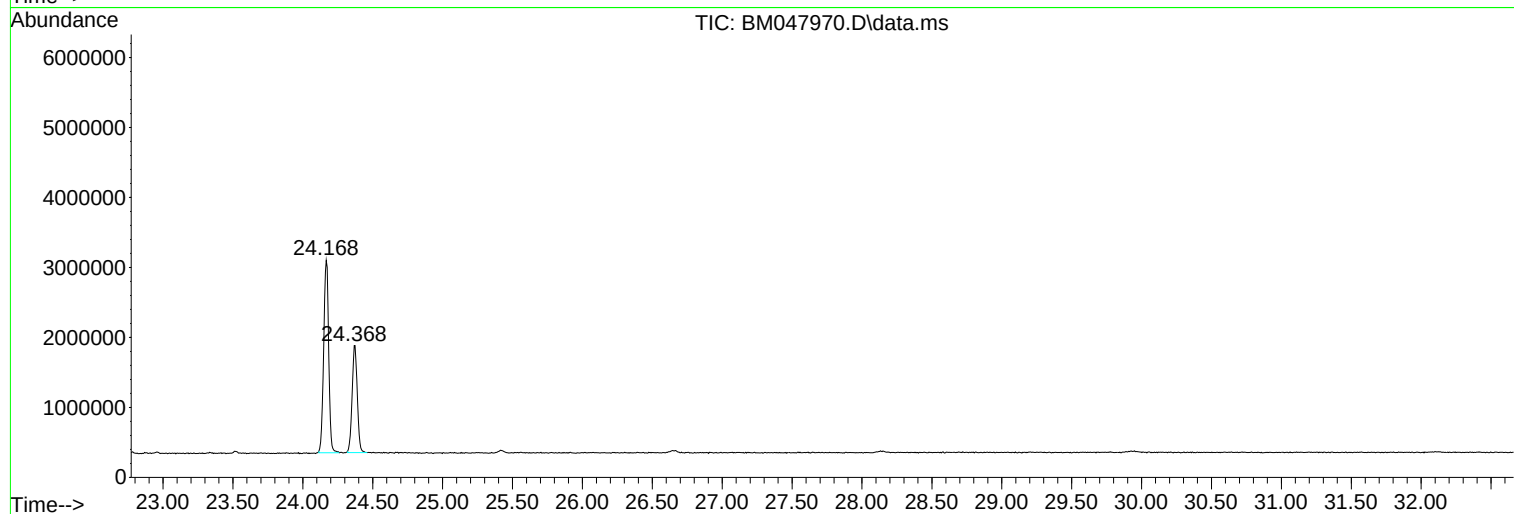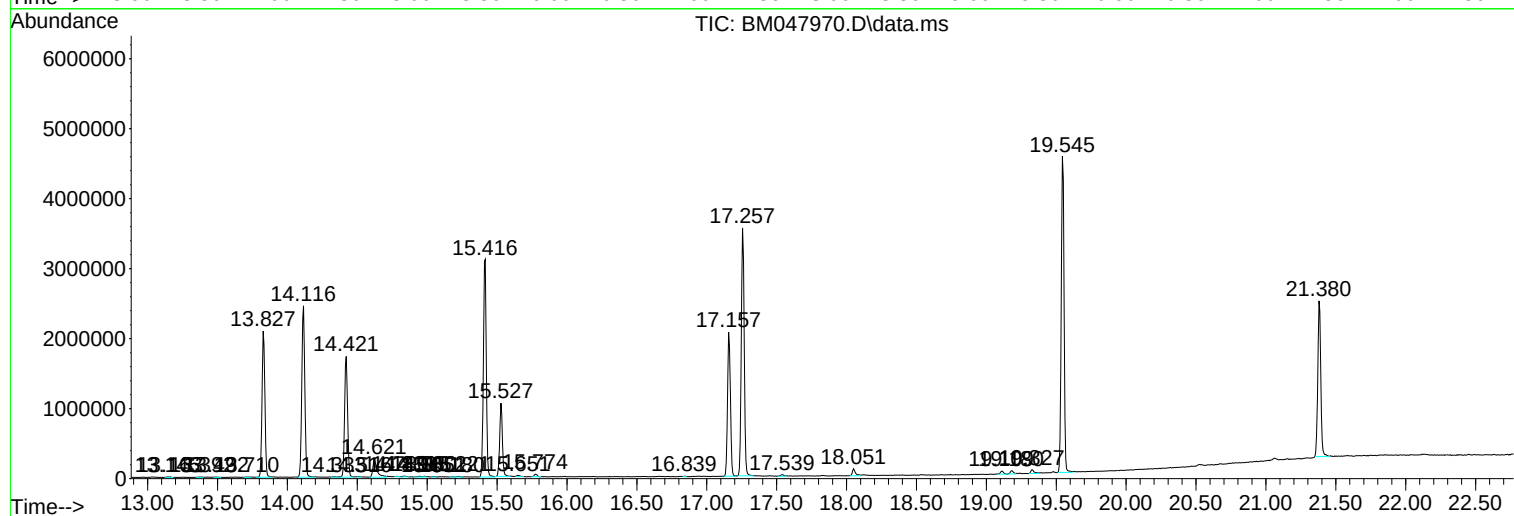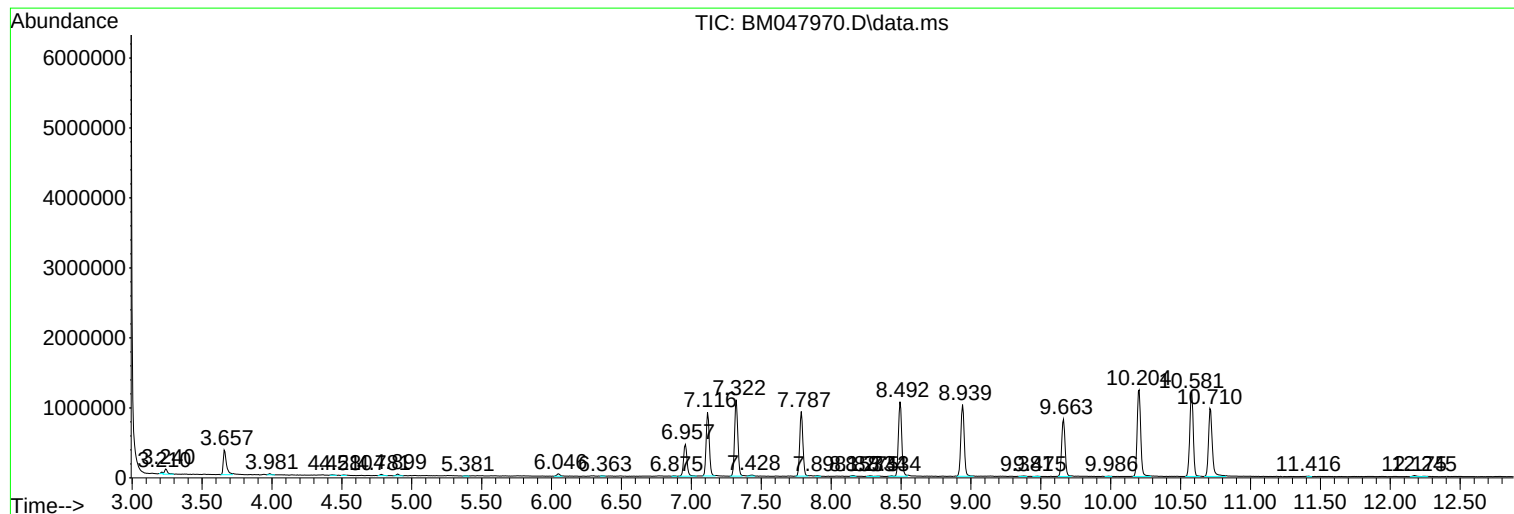

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047970.D
Acq On : 10 Oct 2024 08:31
Operator : RC/JU
Sample : P4207-15
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100924\
Data File : BM047970.D
Acq On : 10 Oct 2024 08:31
Operator : RC/JU
Sample : P4207-15
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EY054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------