

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101017\
 Data File : BM012041.D
 Acq On : 10 Oct 2017 14:07
 Operator : SJ/JU
 Sample : I5522-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 11 01:13:25 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 11 01:12:19 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	182868	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	842965	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	539549	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	1272822	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	1594713	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	1531182	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	35892	9.28	ng/uL	0.00
5) Phenol-d5	7.00	99	648957	41.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	378774	40.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	533893	42.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	583866	42.93	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	253748	42.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	310071	45.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	578425	42.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	774813	51.96	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	1983889	42.43	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	2268855	41.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	255866	31.32	ng/ul	0.00
57) Fluorene-d10	15.49	176	1613054	39.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	278449	32.51	ng/ul	0.00
70) Anthracene-d10	17.34	188	2690616	42.90	ng/ul	0.00
76) Pyrene-d10	19.63	212	3311311	46.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.59	264	3765989	51.13	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.95	163	119272	2.651	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101017\
Data File : BM012041.D
Acq On : 10 Oct 2017 14:07
Operator : SJ/JU
Sample : I5522-13
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 11 01:13:25 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 11 01:12:19 2017
Response via : Initial Calibration

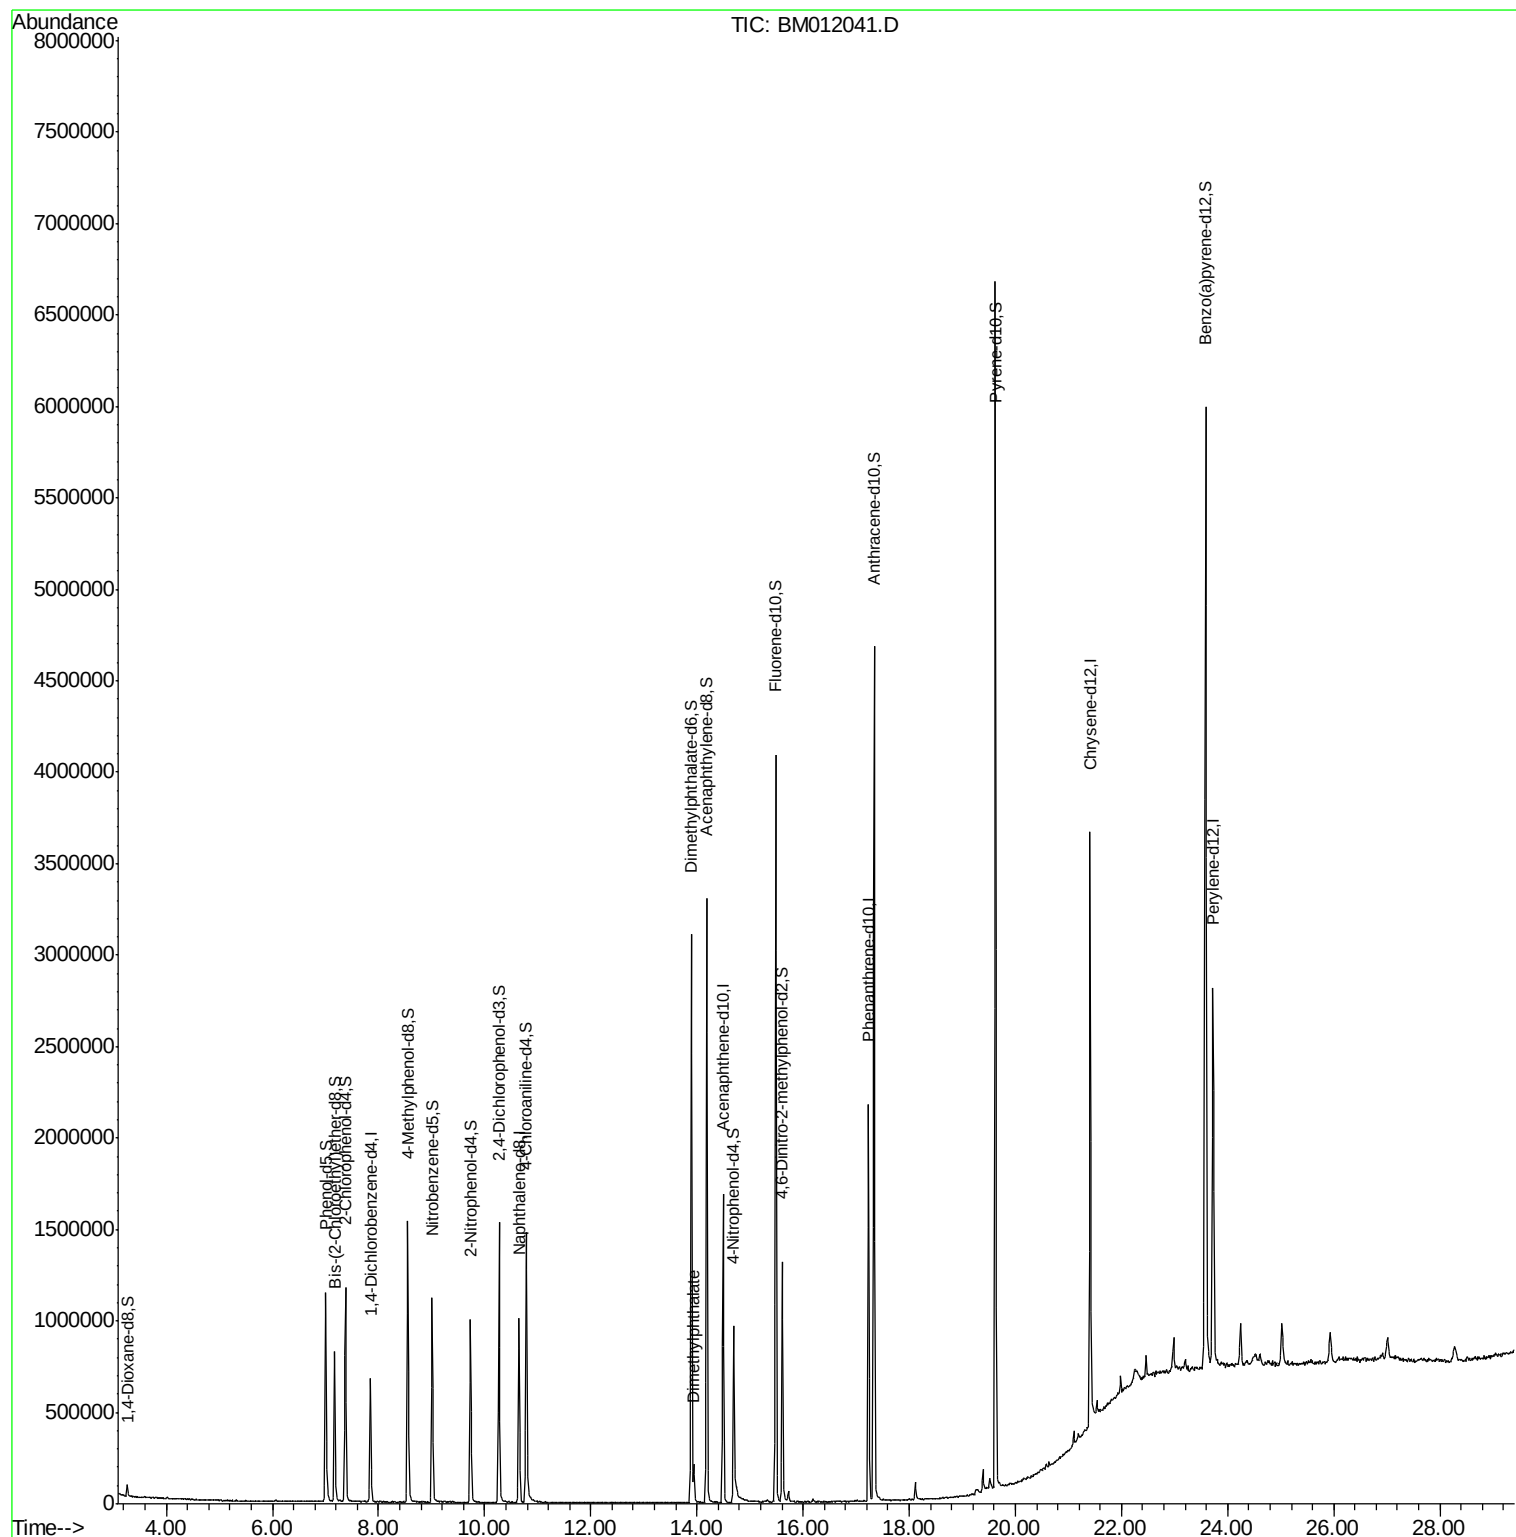

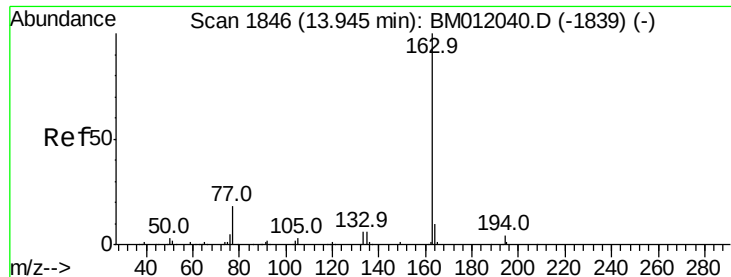

#44

Dimethylphthalate

Concen: 2.651 ng/ul

RT: 13.95 min Scan# 1846

Delta R.T. 0.00 min

Lab File: BM012041.D

Acq: 10 Oct 2017 14:07

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 119272

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 9.5 8.2 12.4

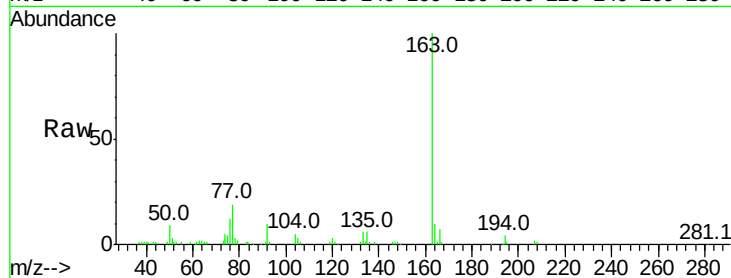

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

