

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101017\
 Data File : BM012045.D
 Acq On : 10 Oct 2017 16:55
 Operator : SJ/JU
 Sample : I5550-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 C0AF1

Manual Integrations
 APPROVED

Sohil
 10/11/2017 7:29:01 PM

Quant Time: Oct 11 01:38:54 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 11 01:12:19 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	154285	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	666100	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	408928	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	1014208	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	1475541	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	1658045	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	17043m	5.22	ng/uL	0.00
5) Phenol-d5	7.00	99	323943	24.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	206240	26.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	289866	27.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	293104	25.54	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	132438	27.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	150880	28.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	297274	27.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	284785	24.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	1105874	31.20	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	1309635	31.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	113687	18.36	ng/ul	0.00
57) Fluorene-d10	15.49	176	980734	31.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	140738	20.62	ng/ul	0.00
70) Anthracene-d10	17.33	188	1657652	33.17	ng/ul	0.00
76) Pyrene-d10	19.63	212	2270652	34.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.58	264	2780710	34.86	ng/ul	0.00

Target Compounds

					Ovalue	
44) Dimethylphthalate	13.95	163	393626	11.545	ng/ul	99
56) Diethylphthalate	15.30	149	61899	1.789	ng/ul	95
58) Fluorene	15.54	166	41144	1.215	ng/ul	96
69) Phenanthrene	17.27	178	767040	13.749	ng/ul	98
71) Anthracene	17.37	178	169823	2.992	ng/ul	99
72) Carbazole	17.64	167	70033	1.424	ng/ul	99
74) Fluoranthene	19.29	202	1011050	14.854	ng/ul#	91
77) Pyrene	19.66	202	870276	10.637	ng/ul#	91
80) Benzo(a)anthracene	21.39	228	509649	6.029	ng/ul	99
81) Bis(2-ethylhexyl)phthalate	21.31	149	82043	1.721	ng/ul	93
82) Chrysene	21.44	228	470739	5.861	ng/ul	98
85) Benzo(b)fluoranthene	23.03	252	536140	5.320	ng/ul#	96
86) Benzo(k)fluoranthene	23.07	252	192897m	1.917	ng/ul	
88) Benzo(a)pyrene	23.63	252	386349	3.990	ng/ul#	97
89) Indeno(1,2,3-cd)pyrene	26.09	276	204274	1.971	ng/ul#	96
91) Benzo(g,h,i)perylene	26.81	276	164158	1.915	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM101017\
Data File : BM012045.D
Acq On : 10 Oct 2017 16:55
Operator : SJ/JU
Sample : I5550-02
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:01 PM

Quant Time: Oct 11 01:38:54 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 11 01:12:19 2017
Response via : Initial Calibration

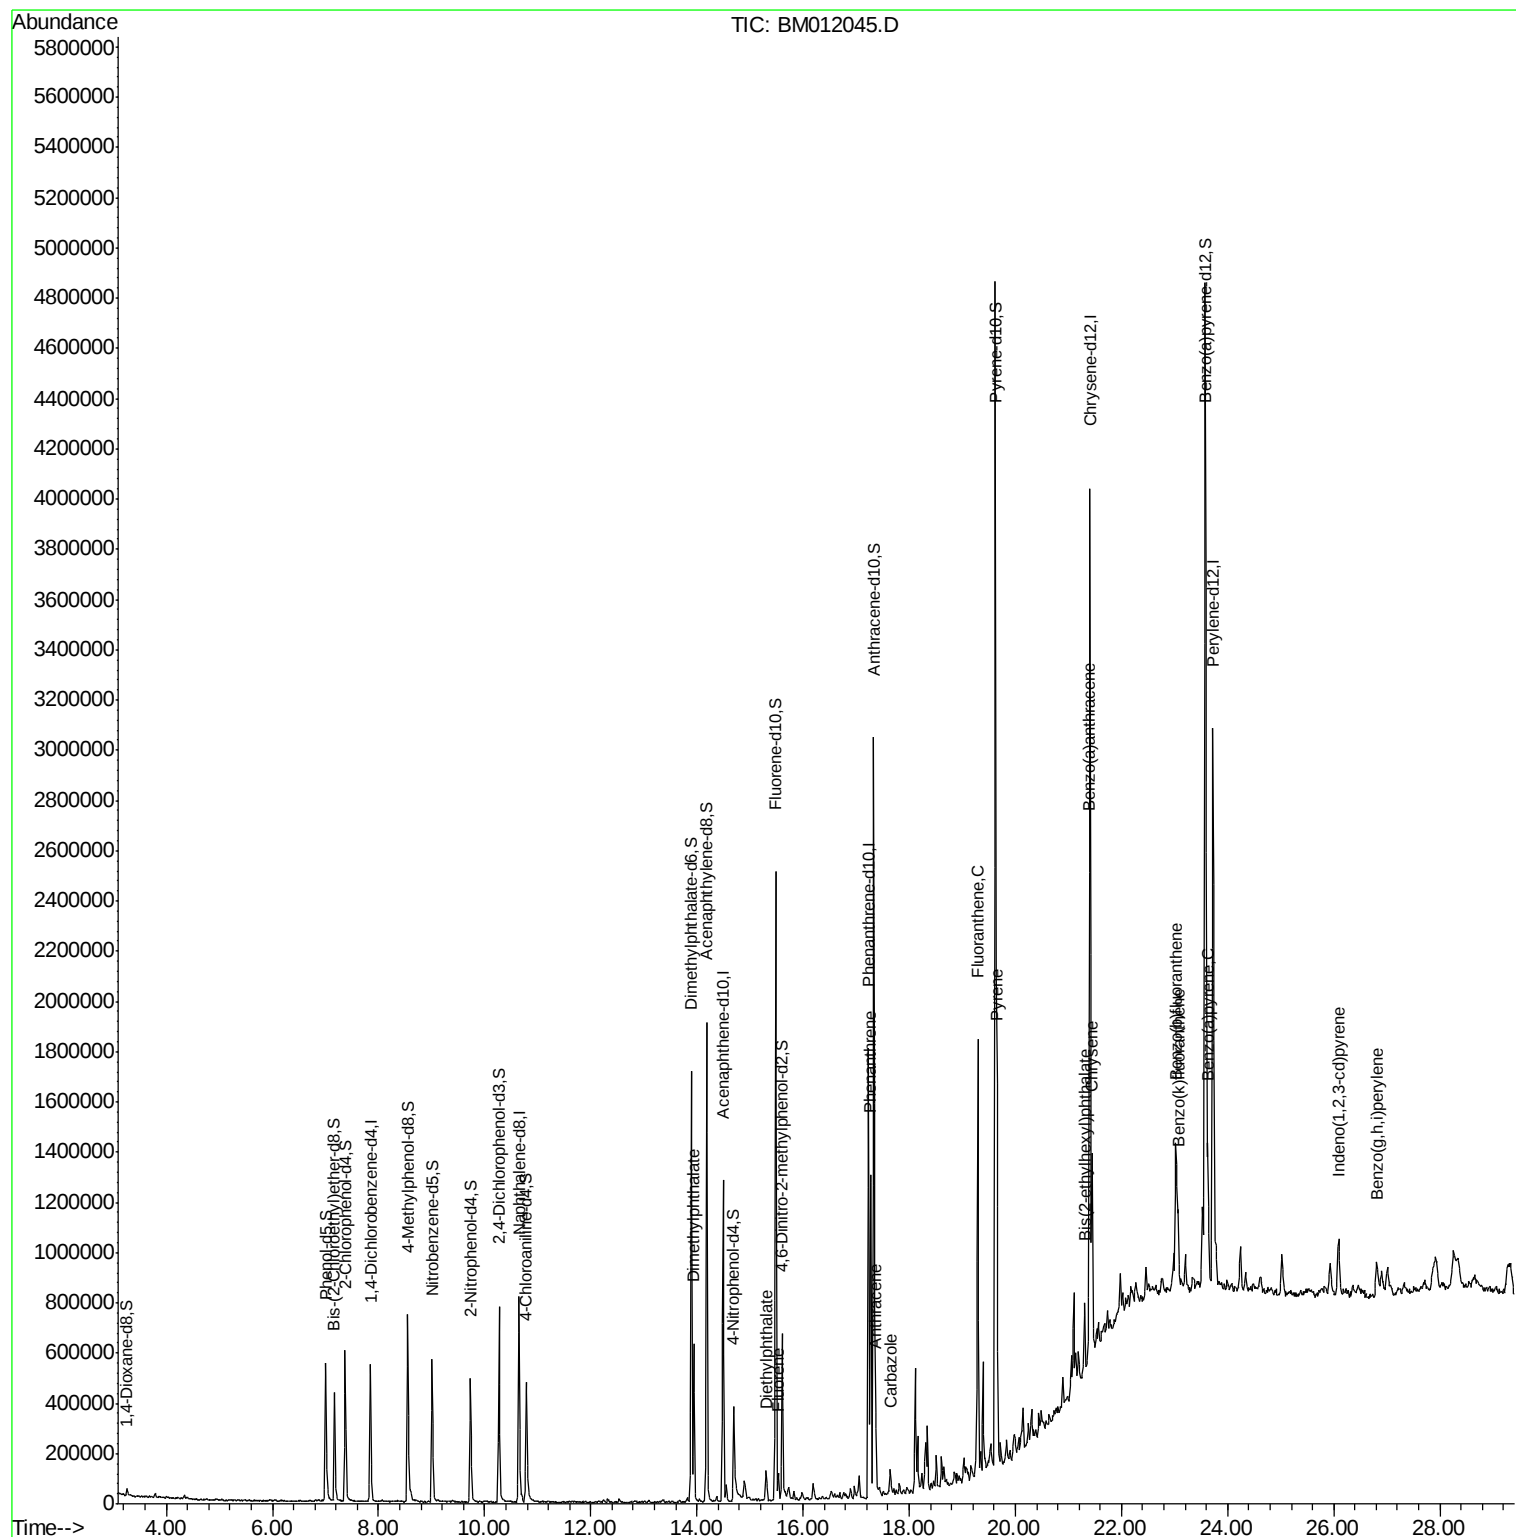

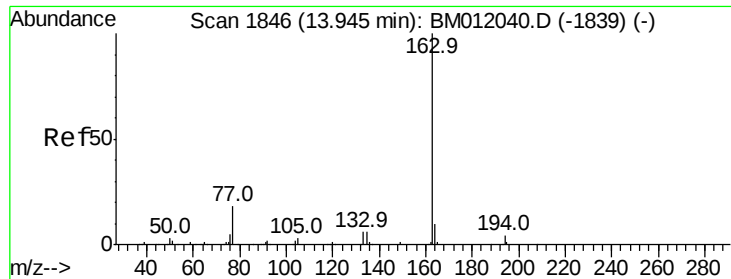





#44
Dimethylphthalate
Concen: 11.545 ng/ul
RT: 13.95 min Scan# 1846
Delta R.T. -0.00 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Instrument :
BNA_M
ClientSampleId :
C0AF1

Tot Ion	Ratio	Resp	Lower	Upper
163	100	393626		
194	4.1		3.5	5.3
164	10.0		8.2	12.4




Manual Integrations
APPROVED


Sohil
10/11/2017 7:29:01 PM

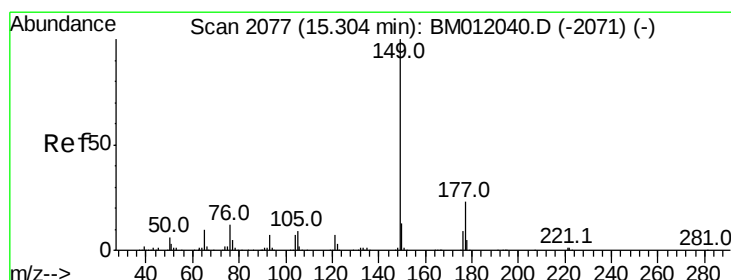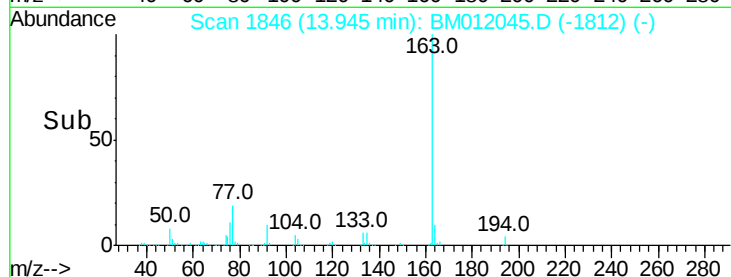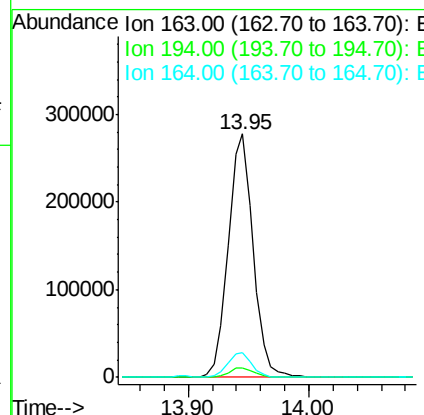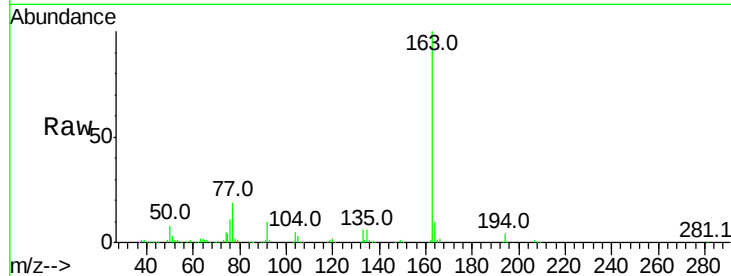

#56
Diethylphthalate
Concen: 1.789 ng/ul
RT: 15.30 min Scan# 2077
Delta R.T. -0.00 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	61899		
177	21.7		20.5	30.7
150	12.8		10.6	15.8

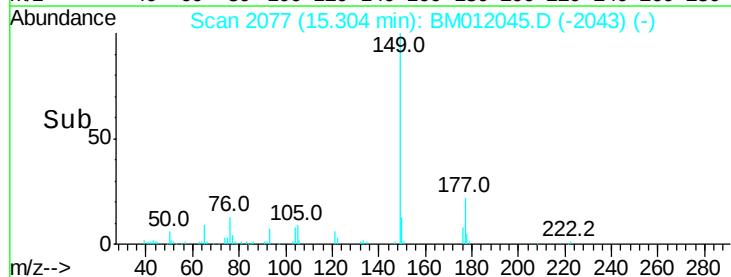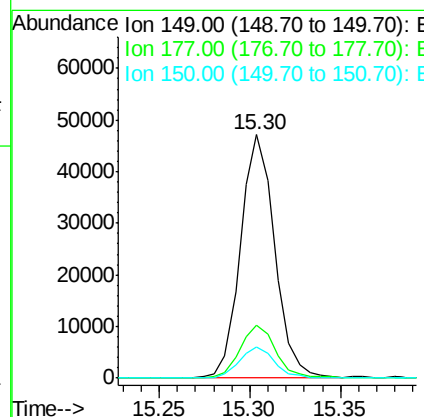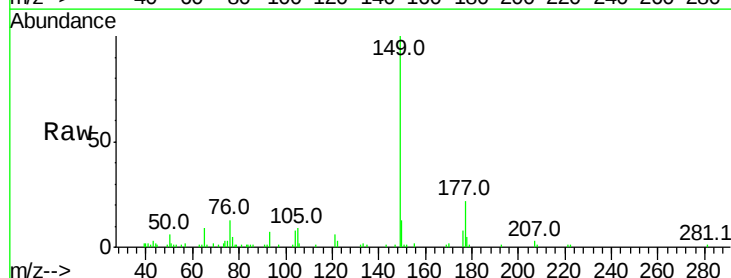







#58
Fluorene
Concen: 1.215 ng/ul
RT: 15.54 min Scan# 2117
Delta R.T. -0.00 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Instrument :
BNA_M
ClientSampleId :
C0AF1

Tot Ion	Ratio	Lower	Upper
166	100		
165	93.4	77.9	116.9
167	13.0	10.6	16.0




Manual Integrations
APPROVED


Sohil
10/11/2017 7:29:01 PM

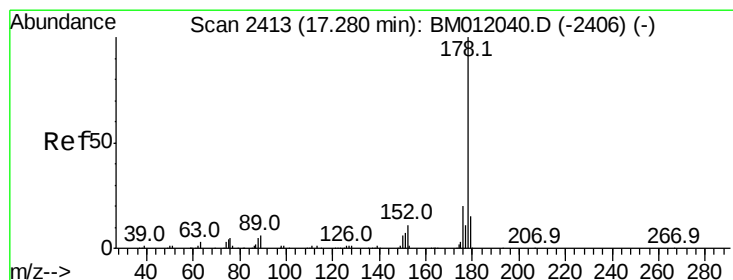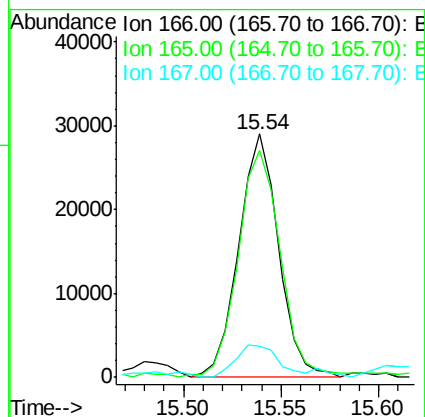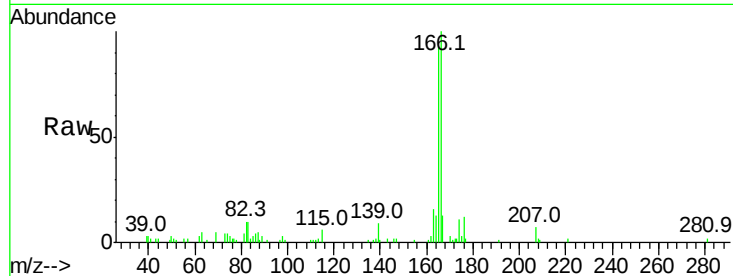

#69
Phenanthrene
Concen: 13.749 ng/ul
RT: 17.27 min Scan# 2412
Delta R.T. -0.01 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.4	12.6	19.0
176	19.5	14.9	22.3

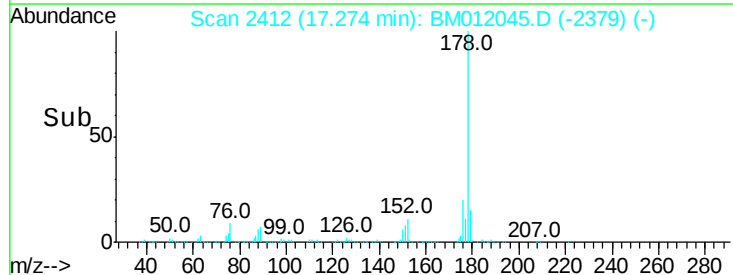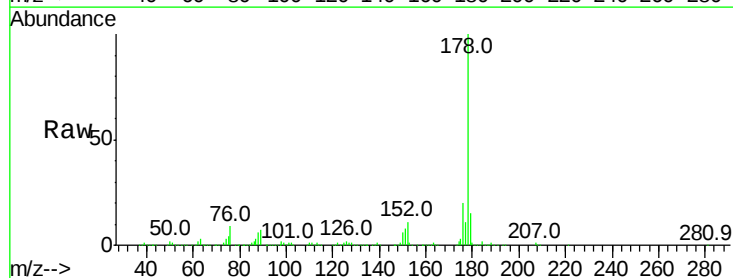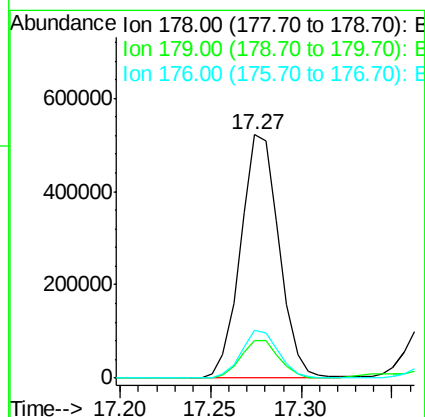







#71
 Anthracene
 Concen: 2.992 ng/ul
 RT: 17.37 min Scan# 2428
 Delta R.T. -0.00 min
 Lab File: BM012045.D
 Acq: 10 Oct 2017 16:55

Instrument :
 BNA_M
 ClientSampleId :
 C0AF1

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.5	11.7	17.5
176	18.5	14.6	21.8




Manual Integrations
 APPROVED


Sohil
 10/11/2017 7:29:01 PM

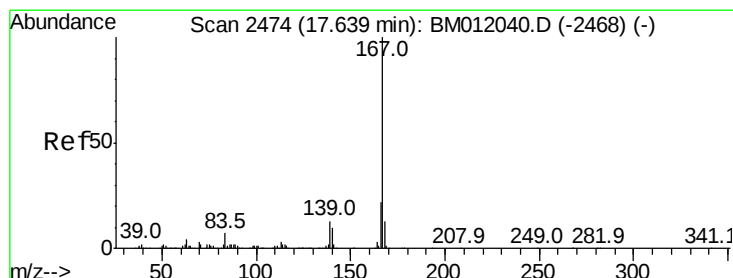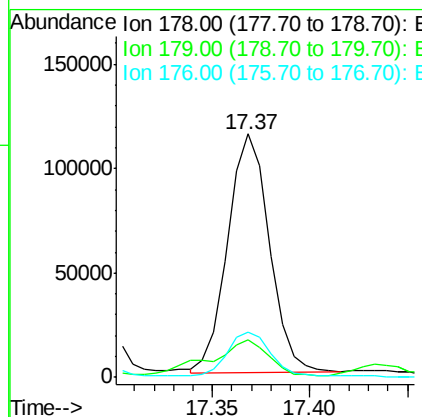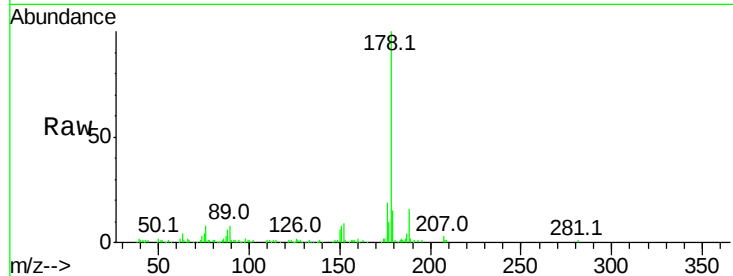

#72
 Carbazole
 Concen: 1.424 ng/ul
 RT: 17.64 min Scan# 2475
 Delta R.T. 0.01 min
 Lab File: BM012045.D
 Acq: 10 Oct 2017 16:55

Tgt Ion	Ratio	Lower	Upper
167	100		
166	22.1	17.1	25.7
139	12.3	10.0	15.0

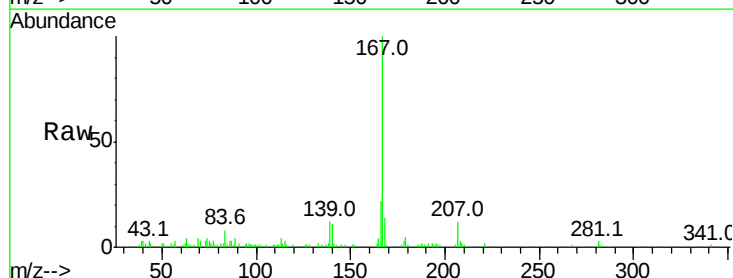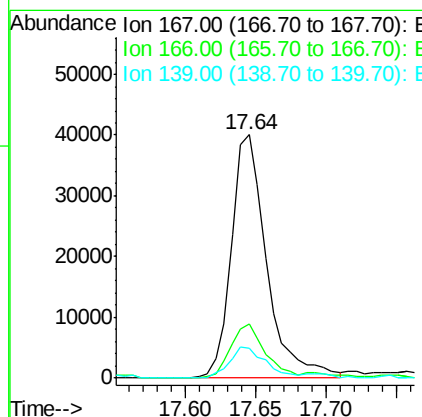

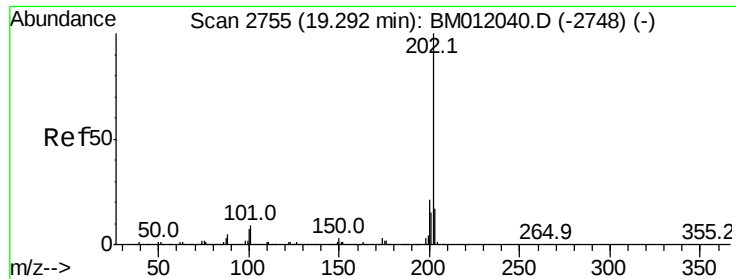

#74

Fluoranthene

Concen: 14.854 ng/ul

RT: 19.29 min Scan# 2755

Delta R.T. -0.00 min

Lab File: BM012045.D

Acq: 10 Oct 2017 16:55

Instrument :

BNA_M


ClientSampled :

C0AF1




Tot Ion	Ratio	Resp	Lower	Upper
202	100	1011050		
101	9.2	4.6	7.0#	
100	6.8	3.4	5.2#	

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:01 PM

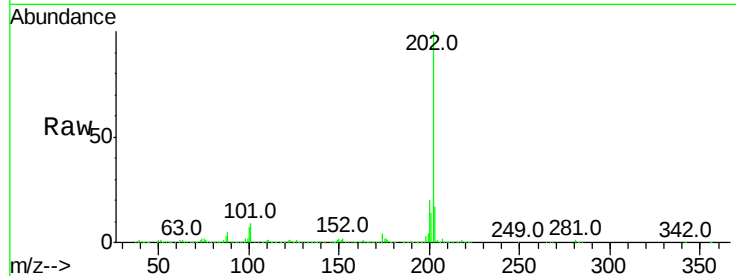

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

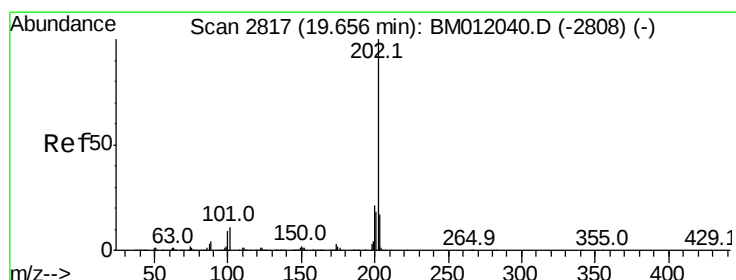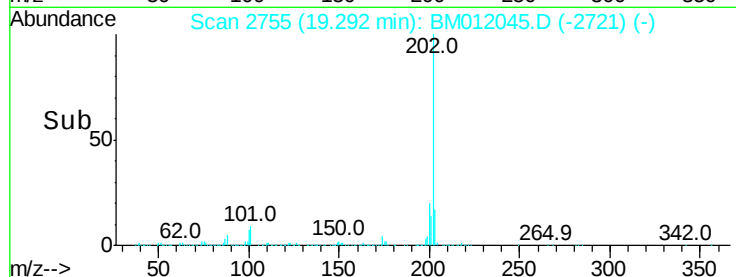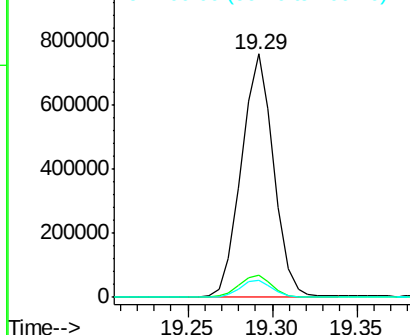

#77

Pyrene

Concen: 10.637 ng/ul


RT: 19.66 min Scan# 2817

Delta R.T. -0.00 min



Lab File: BM012045.D


Acq: 10 Oct 2017 16:55

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	870276		
101	10.3	5.1	7.7#	
100	8.6	4.9	7.3#	

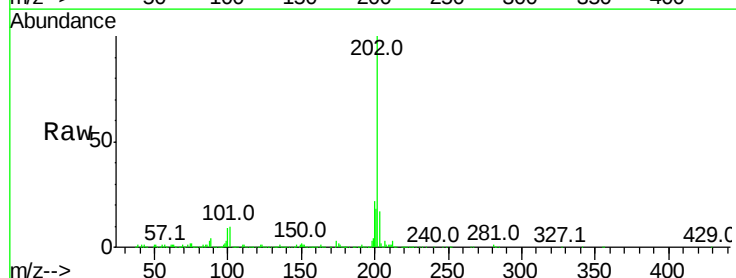

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

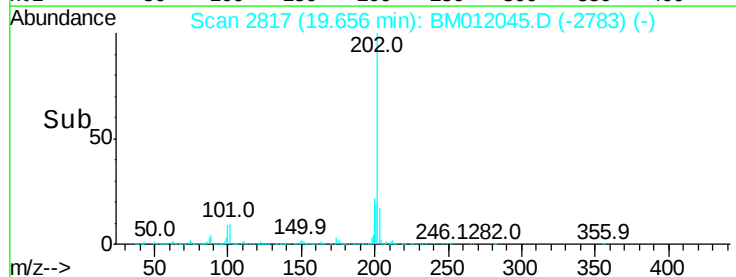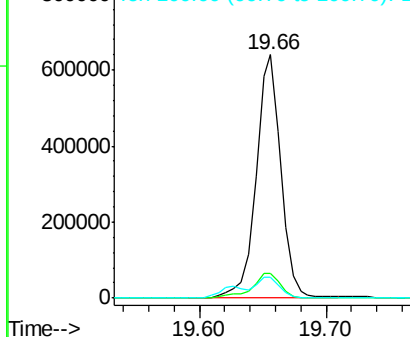







#80
Benzo(a)anthracene
Concen: 6.029 ng/ul
RT: 21.39 min Scan# 3112
Delta R.T. -0.01 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Instrument :
BNA_M
ClientSampleId :
C0AF1

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.3	15.4	23.0
226	26.3	21.4	32.0




Manual Integrations
APPROVED


Sohil
10/11/2017 7:29:01 PM

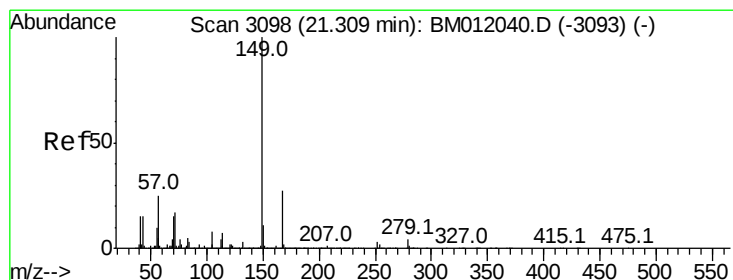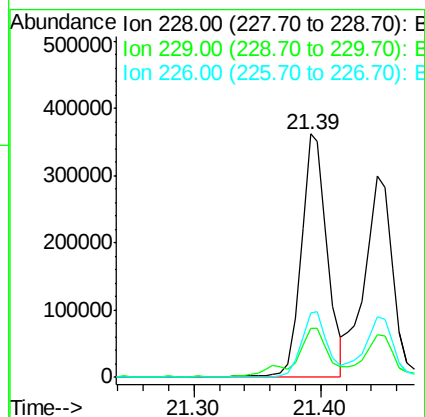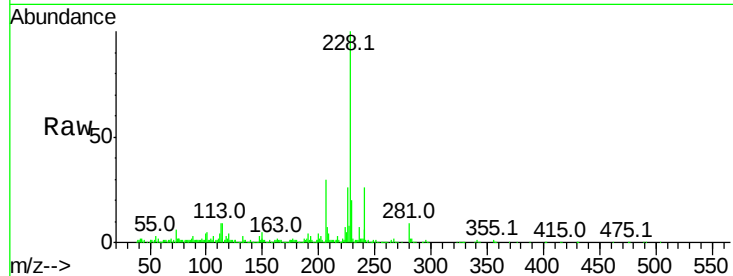

#81
Bis(2-ethylhexyl)phthalate
Concen: 1.721 ng/ul
RT: 21.31 min Scan# 3098
Delta R.T. -0.00 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Tgt Ion	Ratio	Lower	Upper
149	100		
167	24.3	22.8	34.2
279	5.2	4.9	7.3

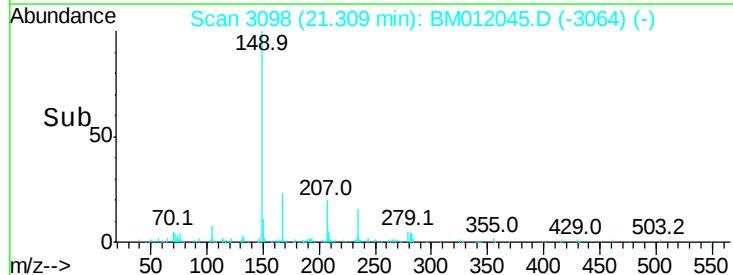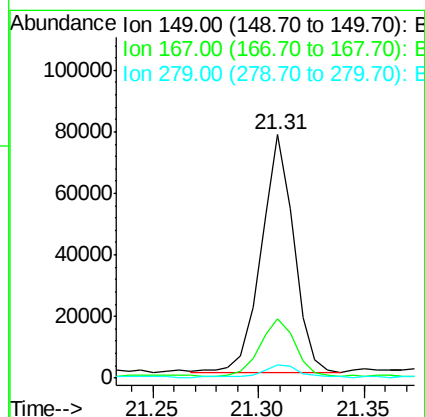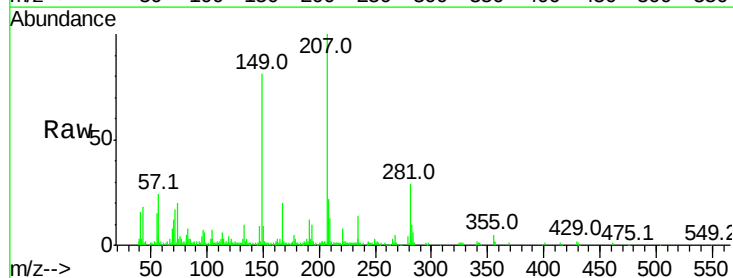

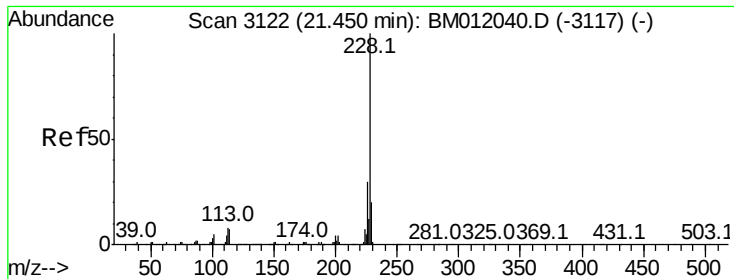





#82
Chrysene
Concen: 5.861 ng/ul
RT: 21.44 min Scan# 3121
Delta R.T. -0.01 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Instrument :
BNA_M
ClientSampled :
C0AF1

Tot Ion:	228	Resp:	470739
Ion Ratio	Lower	Upper	
228	100		
226	30.0	23.4	35.2
229	21.3	15.5	23.3




Manual Integrations
APPROVED


Sohil
10/11/2017 7:29:01 PM

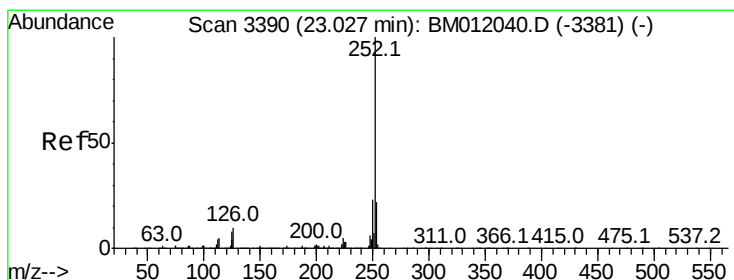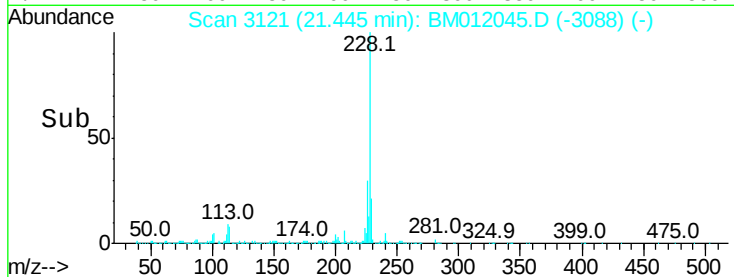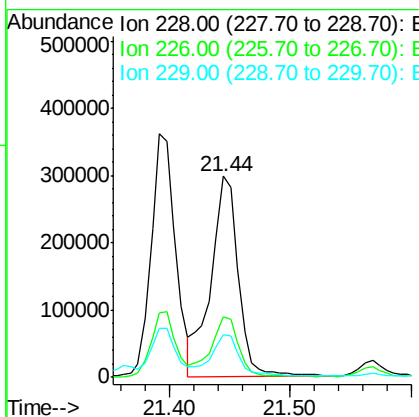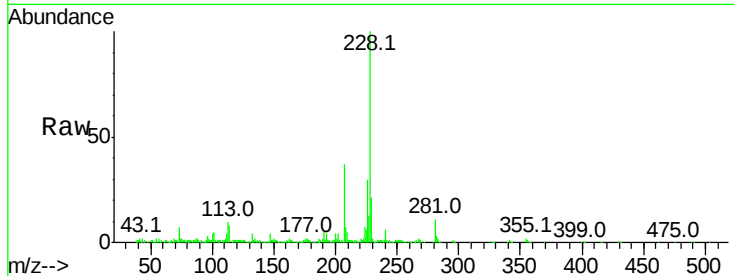

#85
Benzo(b)fluoranthene
Concen: 5.320 ng/ul
RT: 23.03 min Scan# 3390
Delta R.T. -0.00 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Tgt Ion:	252	Resp:	536140
Ion Ratio	Lower	Upper	
252	100		
253	23.1	17.9	26.9
125	10.7	3.6	5.4#

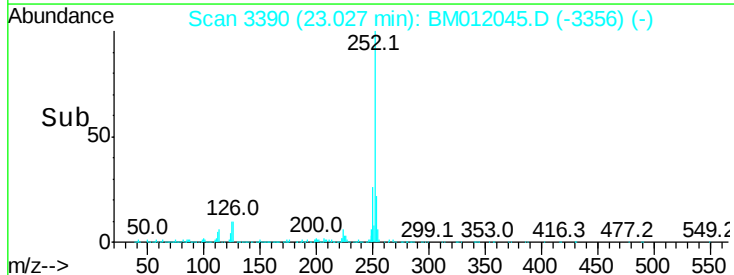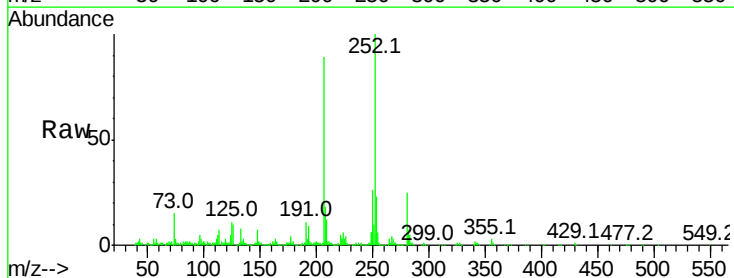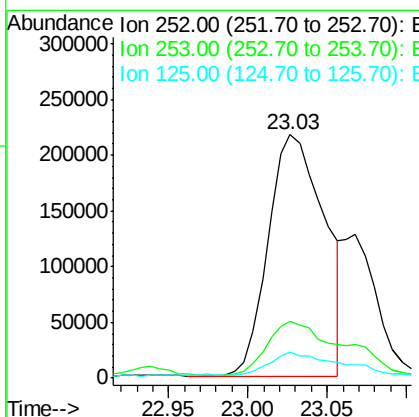







#86
Benzo(k)fluoranthene
Concen: 1.917 ng/ul m
RT: 23.07 min Scan# 3397
Delta R.T. -0.01 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Instrument :
BNA_M
ClientSampled :
C0AF1

Tot Ion	Ratio	Resp Lower	Upper
252	100		
253	23.3	17.1	25.7
125	9.6	3.4	5.2#




Manual Integrations
APPROVED


Sohil
10/11/2017 7:29:01 PM

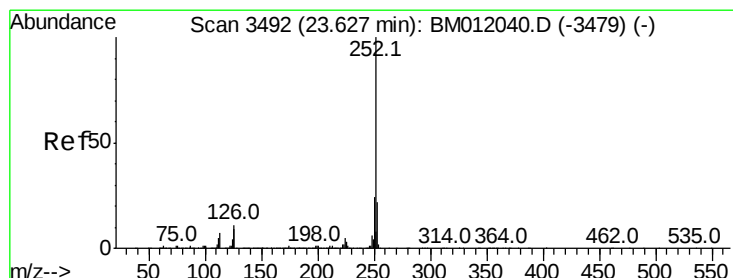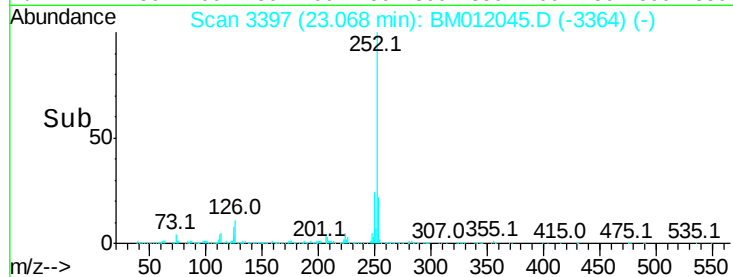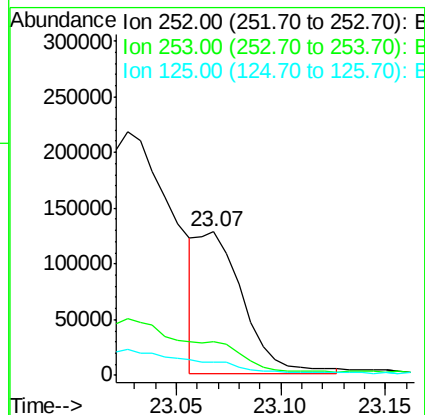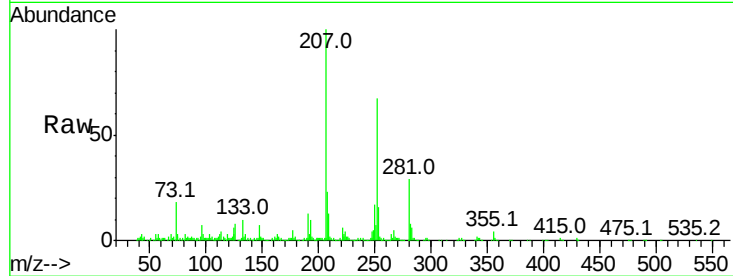

#88
Benzo(a)pyrene
Concen: 3.990 ng/ul
RT: 23.63 min Scan# 3492
Delta R.T. -0.00 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Tgt Ion	Ratio	Resp Lower	Upper
252	100		
253	22.5	18.2	27.2
125	9.8	4.0	6.0#

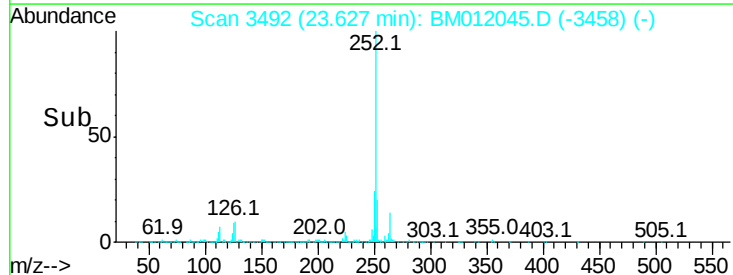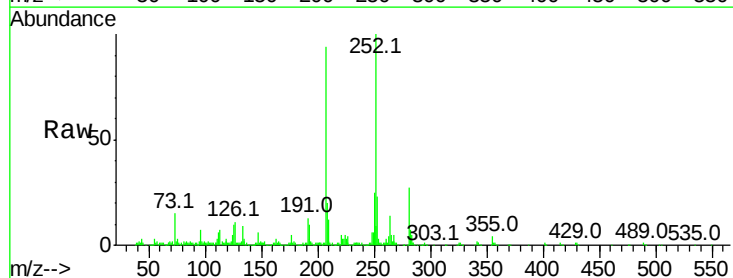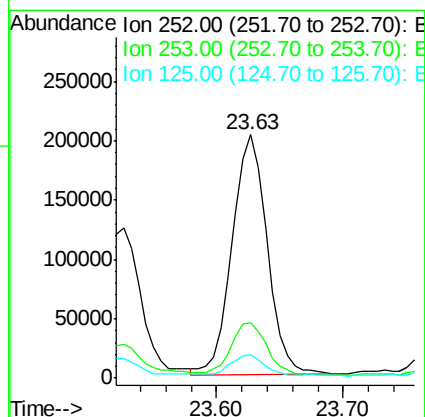







#89
Indeno(1,2,3-cd)pyrene
Concen: 1.971 ng/ul
RT: 26.09 min Scan# 3910
Delta R.T. -0.01 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Instrument :
BNA_M
ClientSampled :
C0AF1

Tot Ion	Ratio	Lower	Upper
276	100		
138	15.9	9.3	13.9#
277	24.6	19.9	29.9

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:01 PM

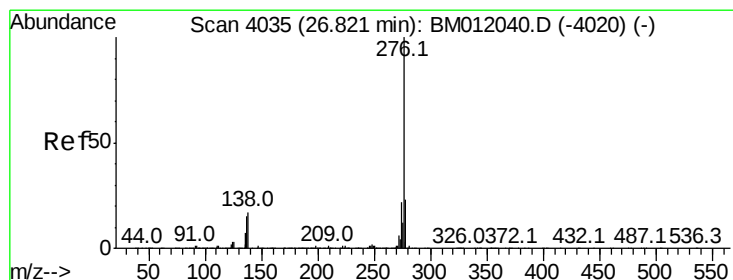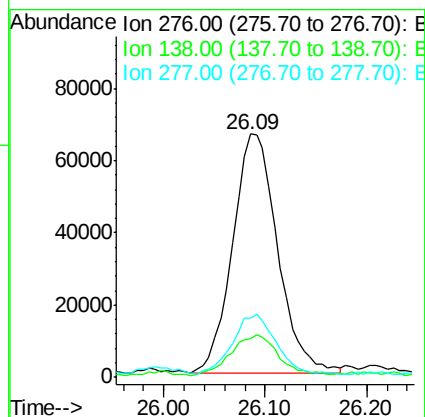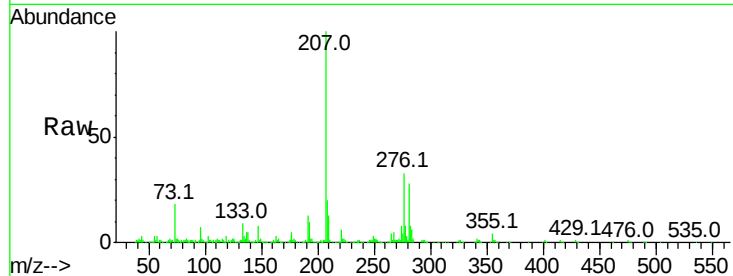

#91
Benzo(g,h,i)perylene
Concen: 1.915 ng/ul
RT: 26.81 min Scan# 4034
Delta R.T. -0.01 min
Lab File: BM012045.D
Acq: 10 Oct 2017 16:55

Tgt Ion	Ratio	Lower	Upper
276	100		
138	18.8	8.5	12.7#
277	25.0	18.6	28.0

