

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101017\
 Data File : BM012066.D
 Acq On : 11 Oct 2017 05:40
 Operator : SJ/JU
 Sample : I5668-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB3G2

Manual Integrations
 APPROVED

Sohil
 10/11/2017 7:29:51 PM

Quant Time: Oct 11 09:13:46 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 11 02:39:56 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	257023	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1127587	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	682219	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	1629111	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	2009813	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	1750608	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	25519	4.70	ng/uL	0.00
5) Phenol-d5	7.00	99	554906	25.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	365528	27.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	486774	27.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	495164	25.90	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	243056	30.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	208321	23.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.26	165	468539	25.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	150424	7.54	ng/ul	0.00
43) Dimethylphthalate-d6	13.89	166	1608590	27.21	ng/ul	0.00
46) Acenaphthylene-d8	14.18	160	2180073	31.38	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	41487m	4.02	ng/ul	0.01
57) Fluorene-d10	15.48	176	1530209	29.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	31478	2.87	ng/ul	0.00
70) Anthracene-d10	17.33	188	2454002	30.57	ng/ul	0.00
76) Pyrene-d10	19.63	212	3076141	33.93	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.58	264	2714011	32.23	ng/ul	0.00

Target Compounds

					Ovalue	
4) Benzaldehyde	6.99	77	21877	1.985	ng/ul#	69
6) Phenol	7.03	94	33490	1.530	ng/ul	94
28) Naphthalene	10.70	128	133962	2.368	ng/ul	99
34) 2-Methylnaphthalene	12.31	142	69773	1.618	ng/ul	98
44) Dimethylphthalate	13.94	163	336502	5.916	ng/ul	99
47) Acenaphthylene	14.21	152	144694	2.148	ng/ul	99
49) Acenaphthene	14.55	153	91235	1.957	ng/ul	97
53) Dibenzofuran	14.89	168	110427	1.632	ng/ul	99
58) Fluorene	15.53	166	123180	2.180	ng/ul#	98
69) Phenanthrene	17.27	178	2723232	30.389	ng/ul	98
71) Anthracene	17.37	178	451303	4.950	ng/ul	99
72) Carbazole	17.64	167	184371	2.334	ng/ul#	95
73) Di-n-butylphthalate	18.19	149	103052	1.089	ng/ul	98
74) Fluoranthene	19.29	202	4191374	38.334	ng/ul#	91
77) Pyrene	19.66	202	4061780	36.448	ng/ul#	90
80) Benzo(a)anthracene	21.39	228	2273210	19.743	ng/ul	97
82) Chrysene	21.44	228	2310587	21.121	ng/ul	98
85) Benzo(b)fluoranthene	23.03	252	2586878	24.311	ng/ul#	97
86) Benzo(k)fluoranthene	23.07	252	841253m	7.919	ng/ul	
88) Benzo(a)pyrene	23.63	252	1597581	15.625	ng/ul#	97
89) Indeno(1,2,3-cd)pyrene	26.09	276	980508	8.961	ng/ul#	94
90) Dibenz(a,h)anthracene	26.09	278	269962	3.003	ng/ul#	85
91) Benzo(g,h,i)perylene	26.82	276	780350	8.622	ng/ul#	95

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101017\
Data File : BM012066.D
Acq On : 11 Oct 2017 05:40
Operator : SJ/JU
Sample : I5668-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB3G2

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:51 PM

Quant Time: Oct 11 09:13:46 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 11 02:39:56 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM101017\
Data File : BM012066.D
Acq On : 11 Oct 2017 05:40
Operator : SJ/JU
Sample : I5668-04
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
CB3G2

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:51 PM

Quant Time: Oct 11 09:13:46 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 11 02:39:56 2017
Response via : Initial Calibration

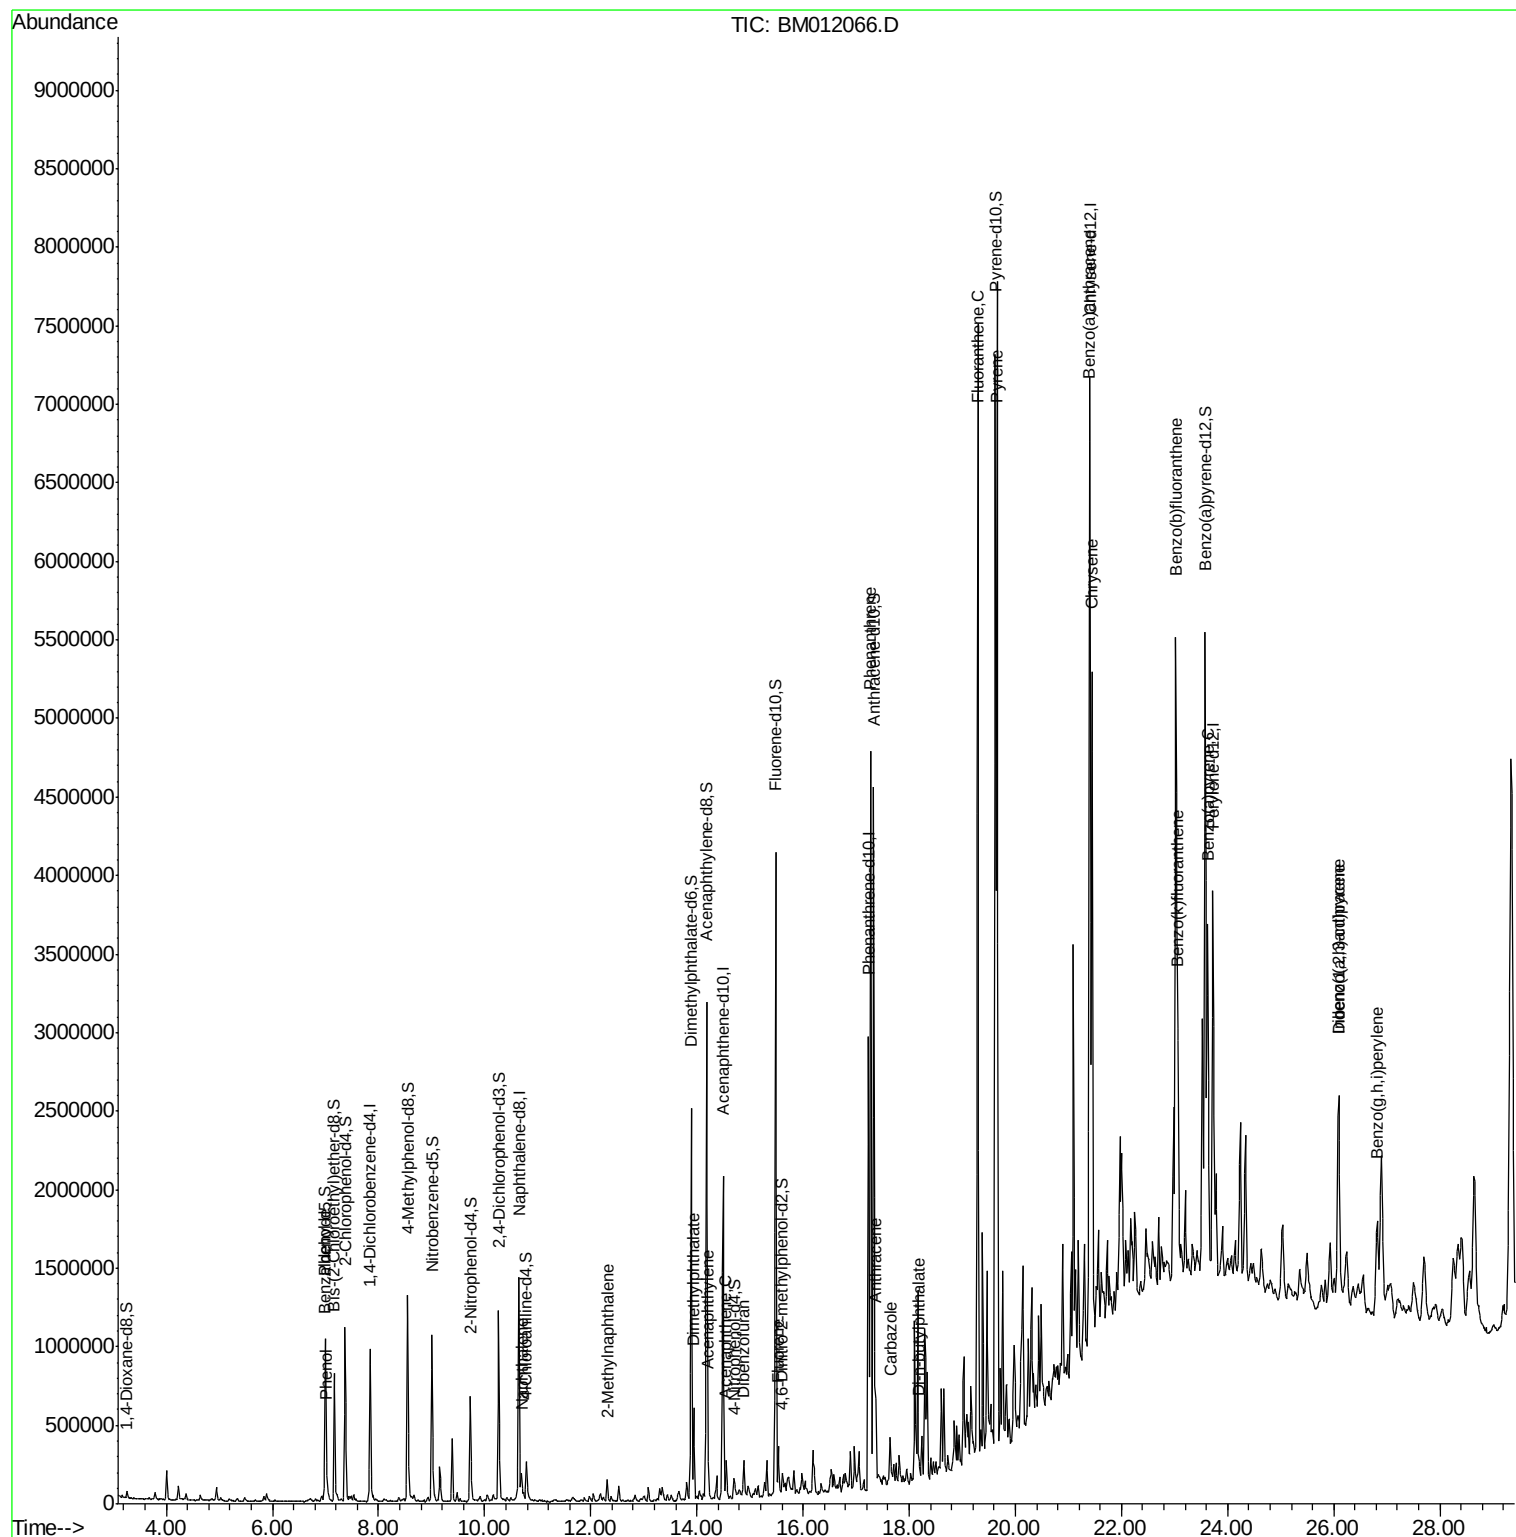

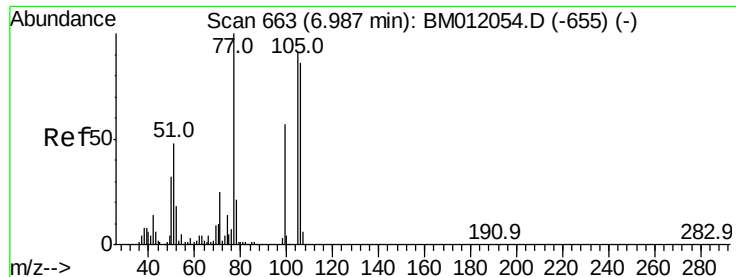

#4

Benzaldehyde

Concen: 1.985 ng/ul

RT: 6.99 min Scan# 663

Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Instrument :

BNA_M





ClientSampled :

CB3G2

Tot Ion	Ratio	Lower	Upper
77	100		
105	139.3	66.1	99.1#
106	85.0	67.8	101.6

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:51 PM

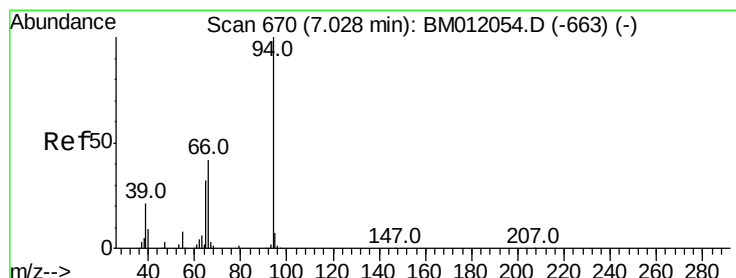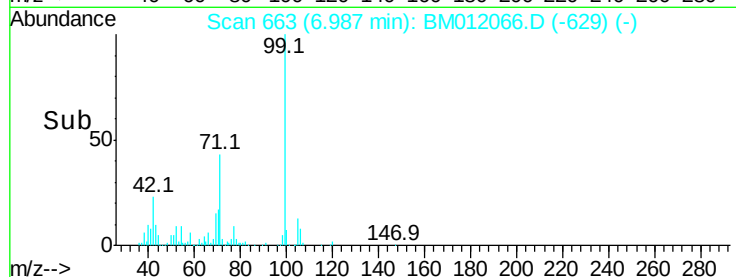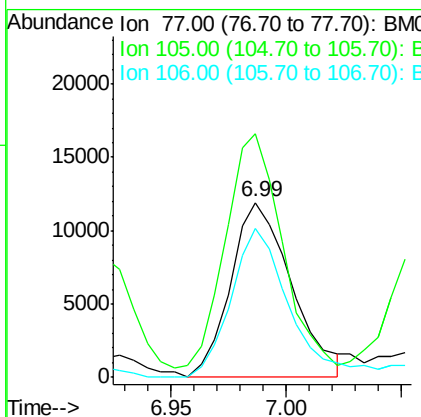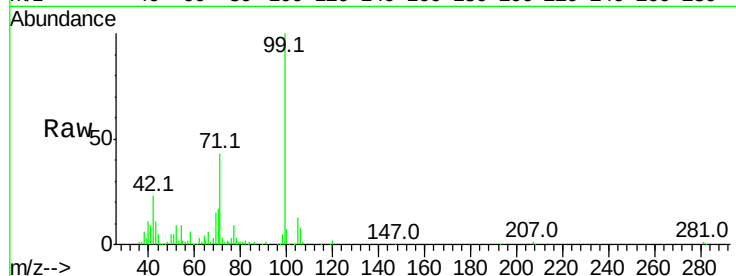

#6

Phenol

Concen: 1.530 ng/ul




RT: 7.03 min Scan# 670


Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Tgt Ion	Ratio	Lower	Upper
94	100		
65	35.3	28.2	42.4
66	52.3	47.2	70.8

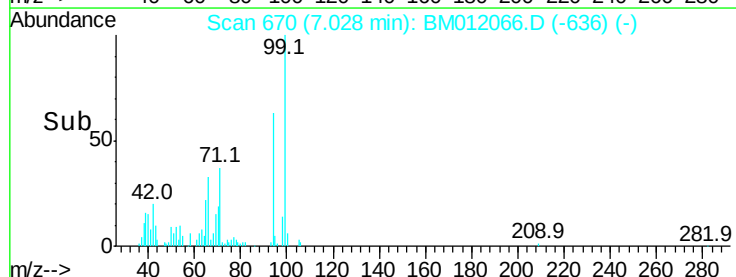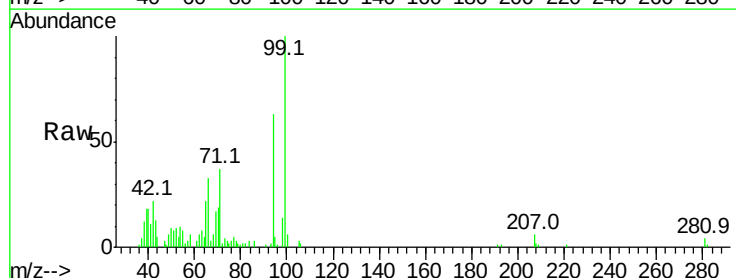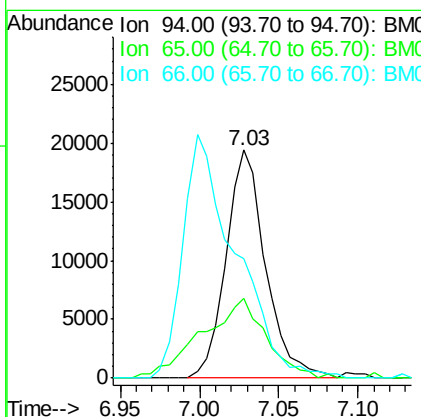



#28

Naphthalene

Concen: 2.368 ng/ul

RT: 10.70 min Scan# 1294

Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Instrument :

BNA_M





ClientSampleId :

CB3G2

Tot Ion:	128	Resp:	133962
Ion Ratio	Lower	Upper	
128	100		
129	11.0	8.8	13.2
127	14.0	10.6	16.0

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:51 PM

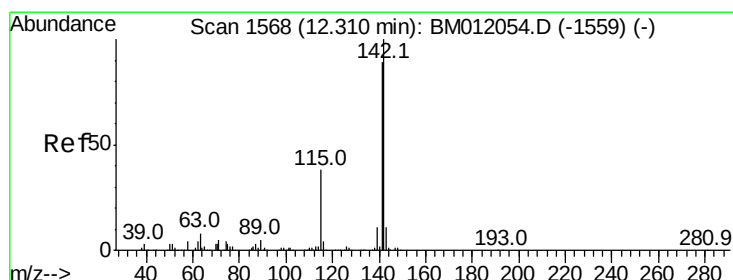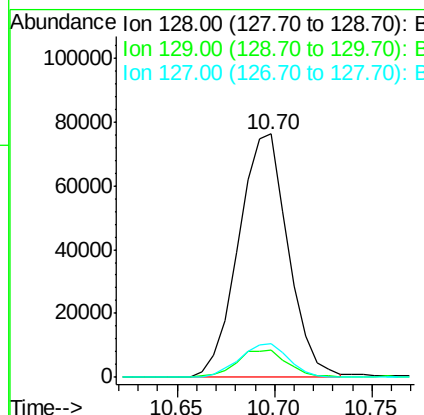

#34

2-Methylnaphthalene

Concen: 1.618 ng/ul




RT: 12.31 min Scan# 1568


Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Tgt Ion:	142	Resp:	69773
Ion Ratio	Lower	Upper	
142	100		
141	94.7	74.1	111.1

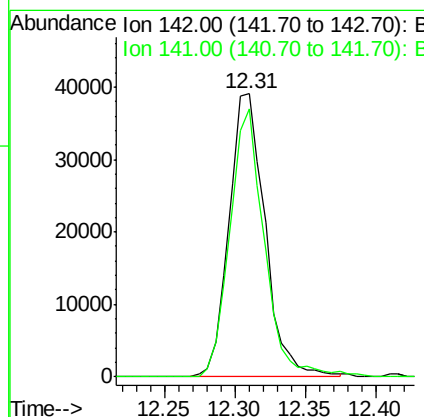

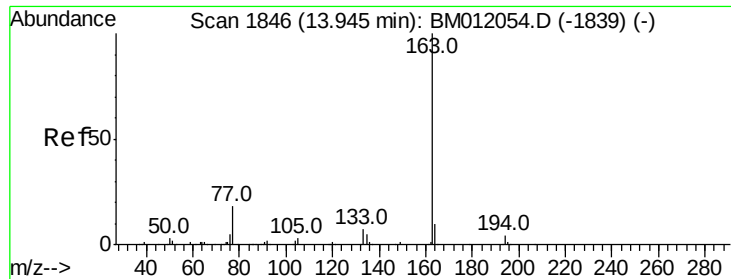





#44
Dimethylphthalate
Concen: 5.916 ng/ul
RT: 13.94 min Scan# 1845
Delta R.T. -0.01 min
Lab File: BM012066.D
Acq: 11 Oct 2017 05:40

Instrument :
BNA_M
ClientSampleId :
CB3G2

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.5	5.3
164	9.9	8.2	12.4




Manual Integrations
APPROVED


Sohil
10/11/2017 7:29:51 PM

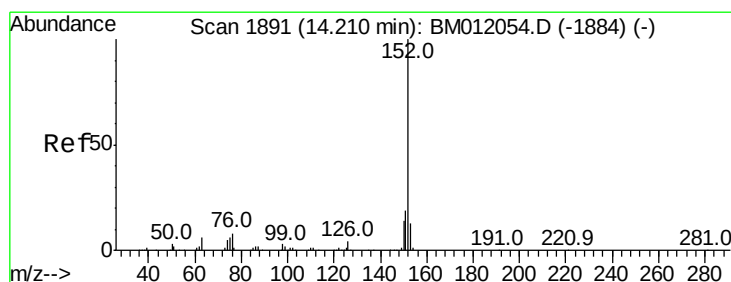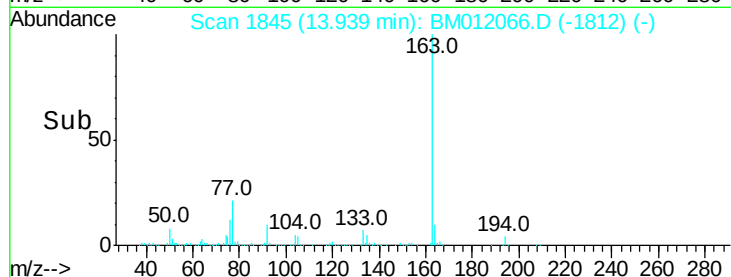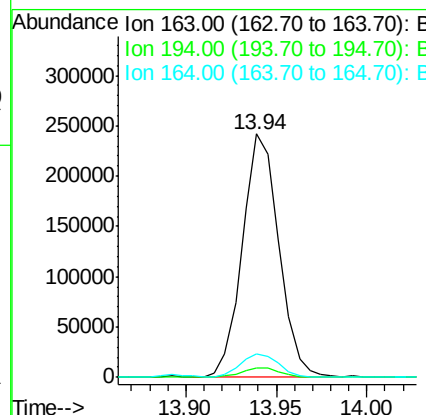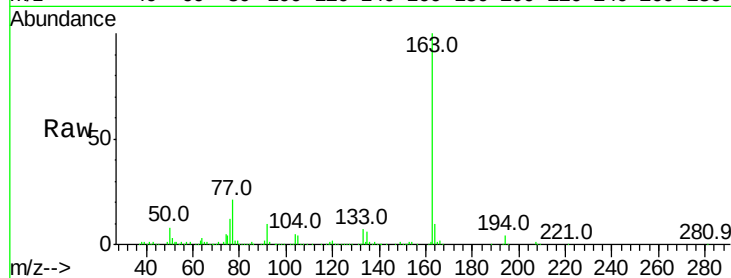

#47
Acenaphthylene
Concen: 2.148 ng/ul
RT: 14.21 min Scan# 1891
Delta R.T. -0.00 min
Lab File: BM012066.D
Acq: 11 Oct 2017 05:40

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.3	16.3	24.5
153	13.8	10.2	15.4

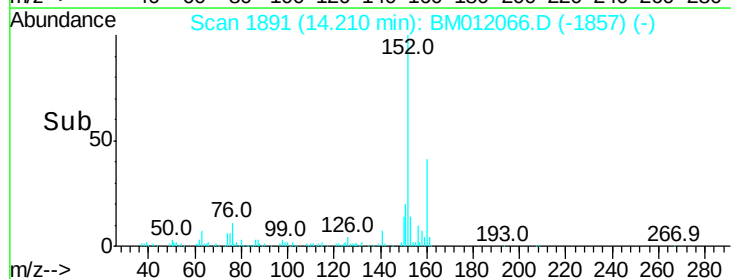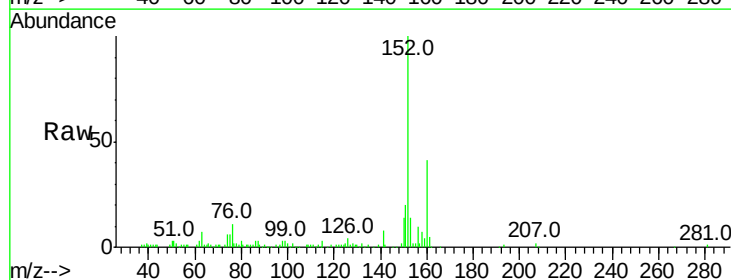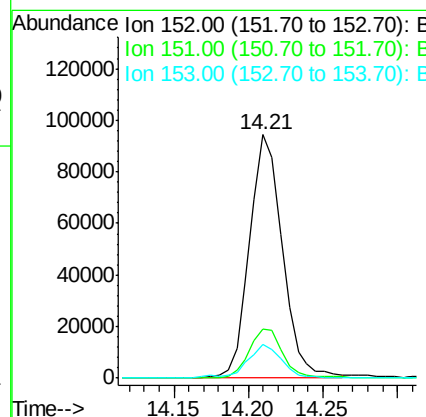



#49

Acenaphthene

Concen: 1.957 ng/ul

RT: 14.55 min Scan# 1949

Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Instrument :

BNA_M





ClientSampled :

CB3G2

Tot Ion:	153	Resp:	91235
Ion Ratio	Lower	Upper	
153	100		
152	46.7	37.6	56.4
154	84.0	70.4	105.6

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:51 PM



#53

Dibenzofuran

Concen: 1.632 ng/ul




RT: 14.89 min Scan# 2006


Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Tgt Ion:	168	Resp:	110427
Ion Ratio	Lower	Upper	
168	100		
139	39.3	30.8	46.2









#58
 Fluorene
 Concen: 2.180 ng/ul
 RT: 15.53 min Scan# 2116
 Delta R.T. -0.01 min
 Lab File: BM012066.D
 Acq: 11 Oct 2017 05:40

Instrument :
 BNA_M
 ClientSampled :
 CB3G2

Tot Ion	Ratio	Lower	Upper
166	100		
165	98.5	77.9	116.9
167	16.1	10.6	16.0#




Manual Integrations
 APPROVED


Sohil
 10/11/2017 7:29:51 PM

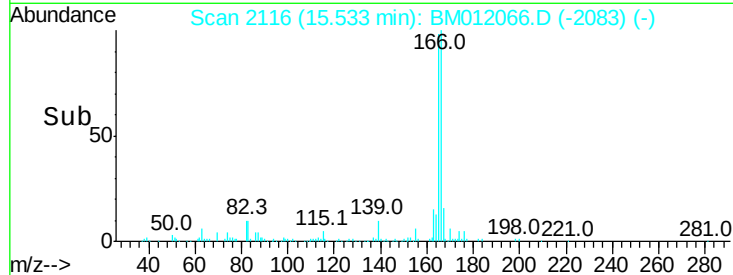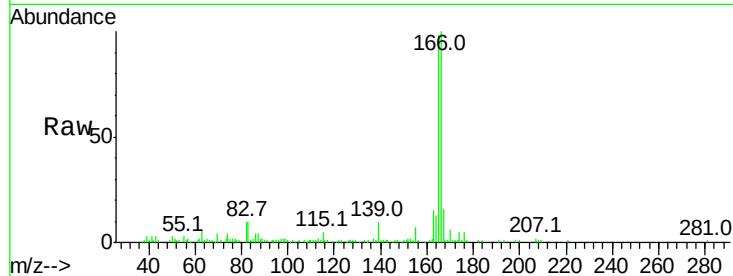

#69
 Phenanthrene
 Concen: 30.389 ng/ul
 RT: 17.27 min Scan# 2412
 Delta R.T. -0.00 min
 Lab File: BM012066.D
 Acq: 11 Oct 2017 05:40

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.5	12.6	19.0
176	19.7	14.9	22.3

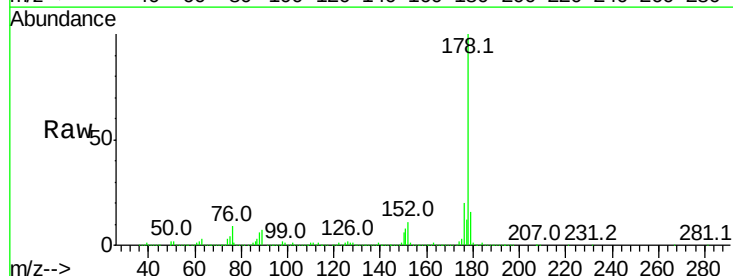







#71
 Anthracene
 Concen: 4.950 ng/ul
 RT: 17.37 min Scan# 2428
 Delta R.T. -0.00 min
 Lab File: BM012066.D
 Acq: 11 Oct 2017 05:40

Instrument :
 BNA_M
 ClientSampled :
 CB3G2

Tot Ion	Ratio	Lower	Upper
178	100		
179	14.7	11.7	17.5
176	18.8	14.6	21.8




Manual Integrations
 APPROVED


Sohil
 10/11/2017 7:29:51 PM

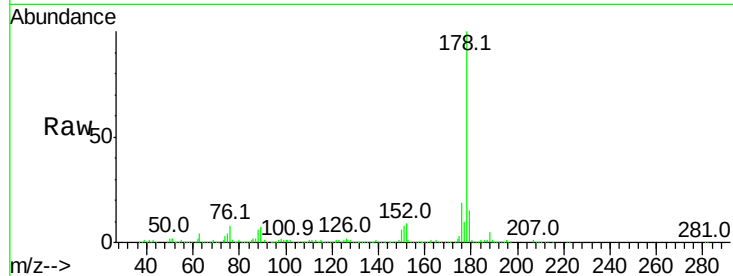

#72
 Carbazole
 Concen: 2.334 ng/ul
 RT: 17.64 min Scan# 2474
 Delta R.T. -0.00 min
 Lab File: BM012066.D
 Acq: 11 Oct 2017 05:40

Tgt Ion	Ratio	Lower	Upper
167	100		
166	23.6	17.1	25.7
139	15.2	10.0	15.0#

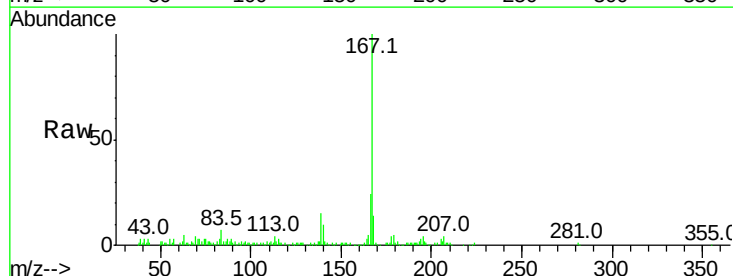

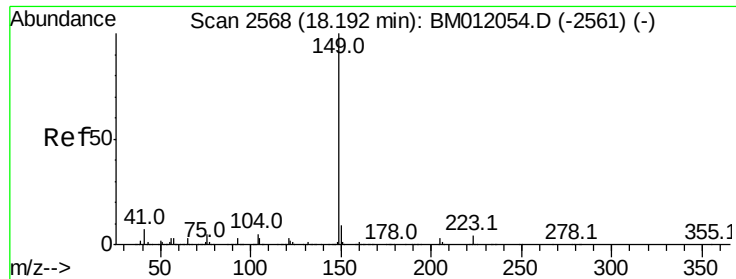

#73

Di-n-butylphthalate

Concen: 1.089 ng/ul

RT: 18.19 min Scan# 2568

Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Instrument :

BNA_M





ClientSampleId :

CB3G2

Tot Ion:	149	Resp:	103052
Ion Ratio	Lower	Upper	
149	100		
150	9.1	7.1	10.7
104	6.0	5.6	8.4

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:51 PM

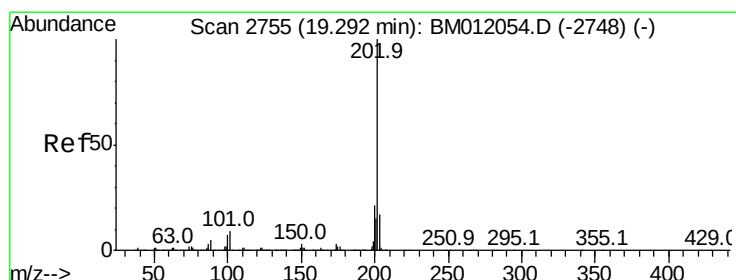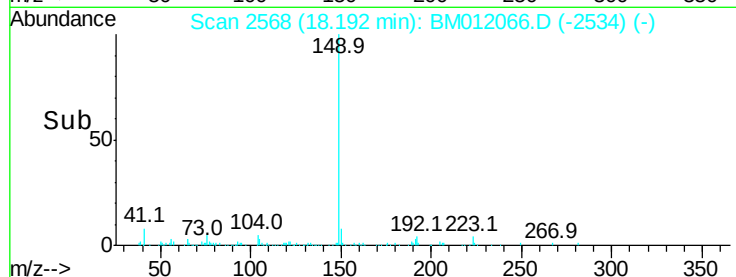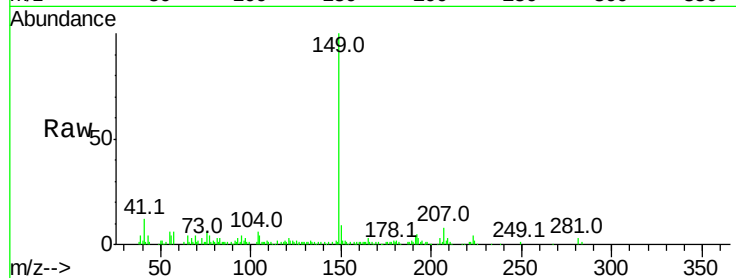

#74

Fluoranthene

Concen: 38.334 ng/ul




RT: 19.29 min Scan# 2755


Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Tgt Ion:	202	Resp:	4191374
Ion Ratio	Lower	Upper	
202	100		
101	9.0	4.6	7.0#
100	7.3	3.4	5.2#

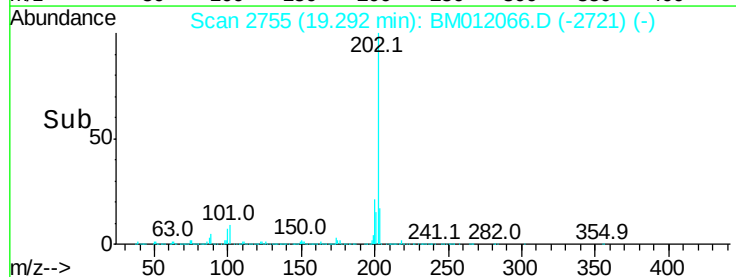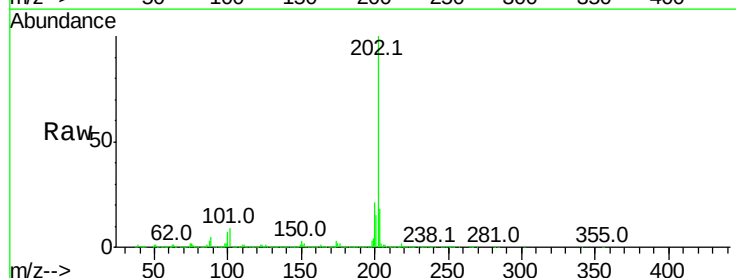

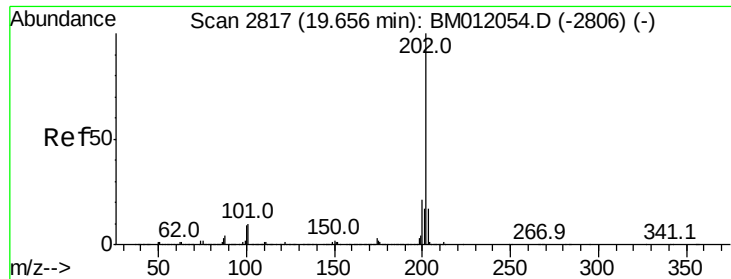

#77

Pvrene

Concen: 36.448 ng/ul

RT: 19.66 min Scan# 2817

Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Instrument :

BNA_M

ClientSampleId :

CB3G2

Tot Ion:202 Resp: 4061780

Ion Ratio Lower Upper

202 100

101 10.8 5.1 7.7#


100 8.8 4.9 7.3#

Manual Integrations

APPROVED

Sohil




10/11/2017 7:29:51 PM

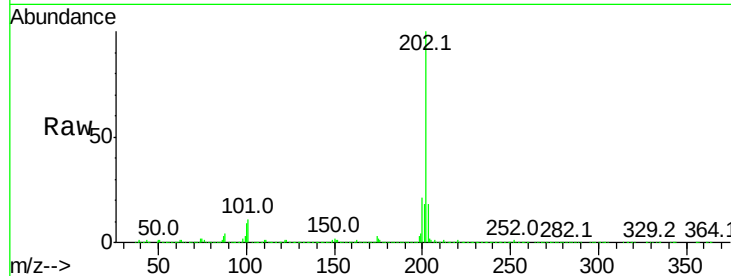

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

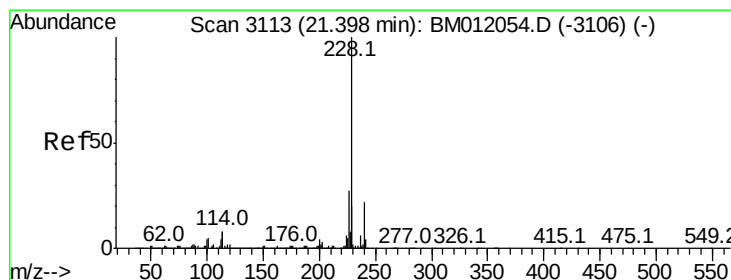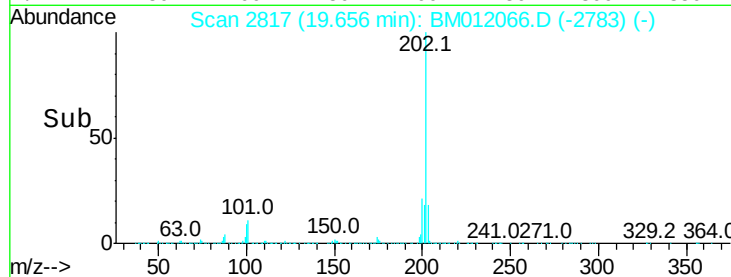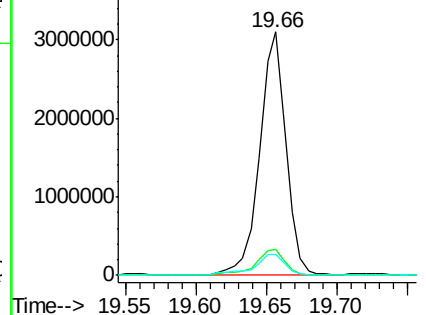

#80

Benzo(a)anthracene

Concen: 19.743 ng/ul

RT: 21.39 min Scan# 3112

Delta R.T. -0.01 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40


Tgt Ion:228 Resp: 2273210

Ion Ratio Lower Upper

228 100

229 21.0 15.4 23.0



226 27.9 21.4 32.0

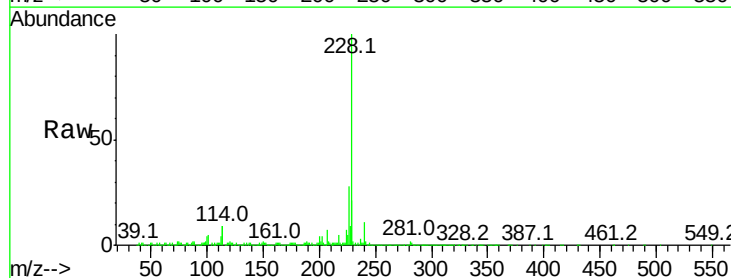


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

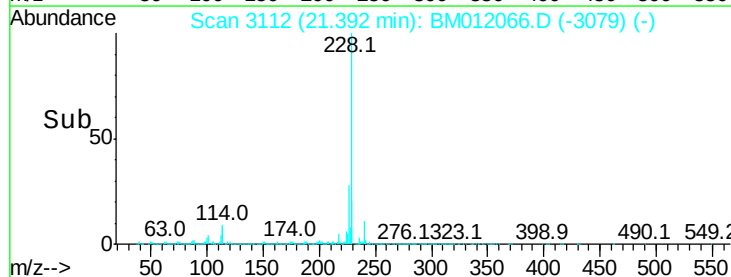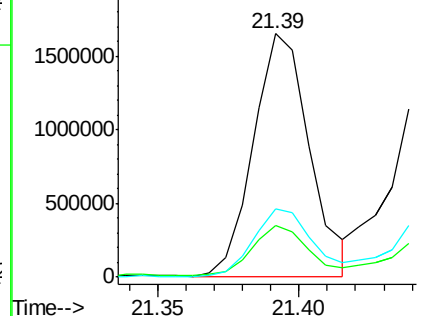

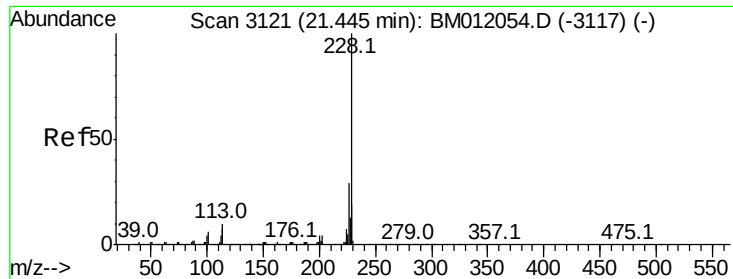

#82

Chrysene

Concen: 21.121 ng/ul

RT: 21.44 min Scan# 3121

Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Instrument :

BNA_M

ClientSampled :

CB3G2

Tot Ion:228 Resp: 2310587

Ion	Ratio	Lower	Upper
228	100		
226	30.2	23.4	35.2
229	20.4	15.5	23.3

228 100

226 30.2 23.4 35.2





229 20.4 15.5 23.3

Manual Integrations

APPROVED

Sohil

10/11/2017 7:29:51 PM

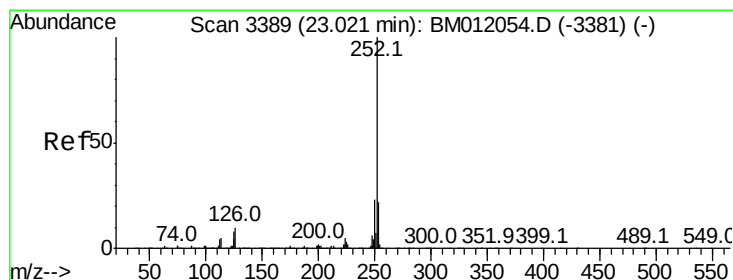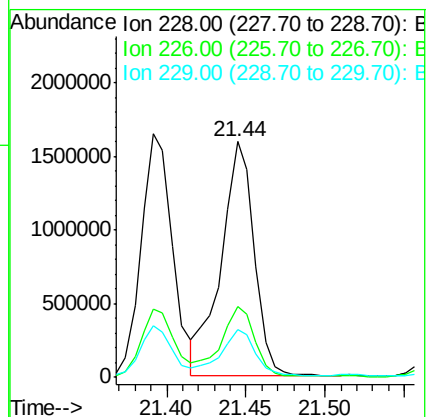

#85

Benzo(b)fluoranthene

Concen: 24.311 ng/ul

RT: 23.03 min Scan# 3390

Delta R.T. 0.01 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40




Tgt Ion:252 Resp: 2586878


Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.9	26.9
125	10.8	3.6	5.4

252 100

253 22.3 17.9 26.9

125 10.8 3.6 5.4

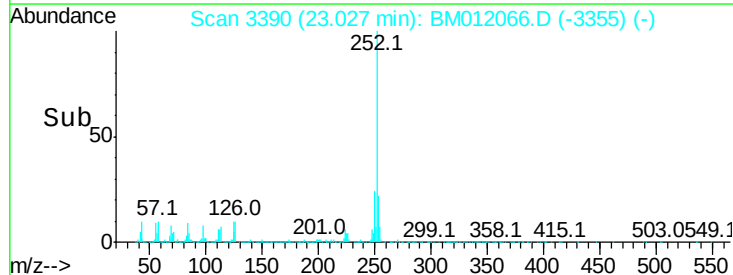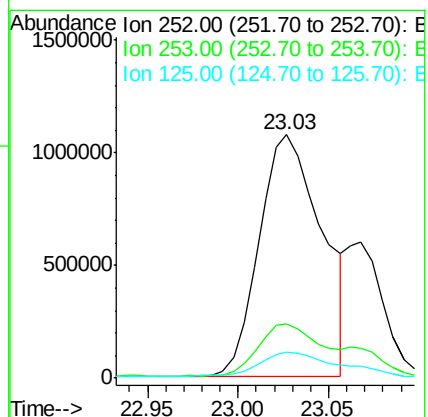

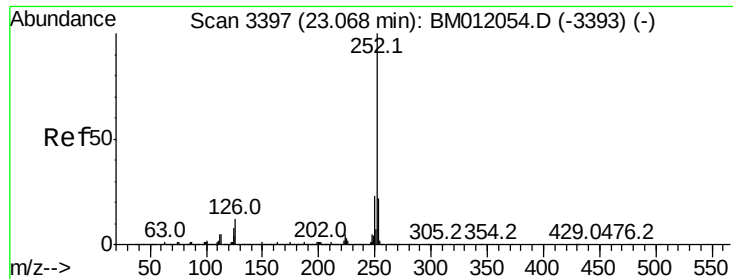





#86
Benzo(k)fluoranthene
Concen: 7.919 ng/ul m
RT: 23.07 min Scan# 3397
Delta R.T. -0.00 min
Lab File: BM012066.D
Acq: 11 Oct 2017 05:40

Instrument :
BNA_M
ClientSampleId :
CB3G2

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.4	17.1	25.7
125	9.2	3.4	5.2#




Manual Integrations
APPROVED


Sohil
10/11/2017 7:29:51 PM

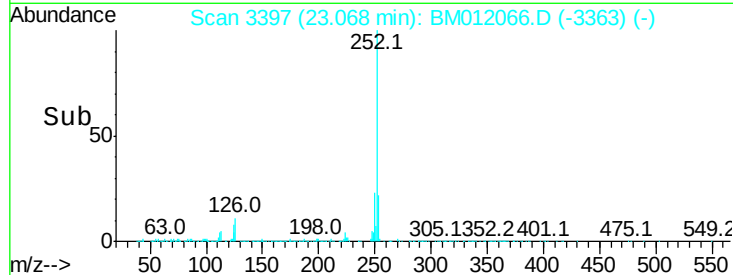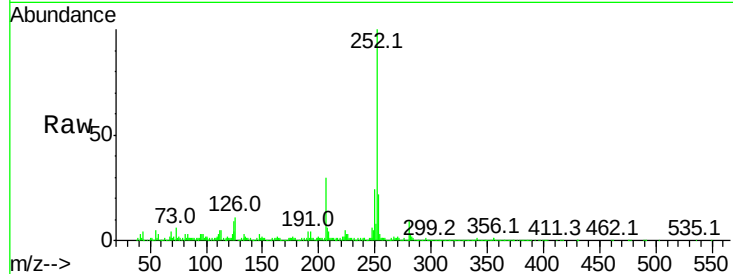

#88
Benzo(a)pyrene
Concen: 15.625 ng/ul
RT: 23.63 min Scan# 3492
Delta R.T. -0.00 min
Lab File: BM012066.D
Acq: 11 Oct 2017 05:40

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.4	18.2	27.2
125	9.4	4.0	6.0#

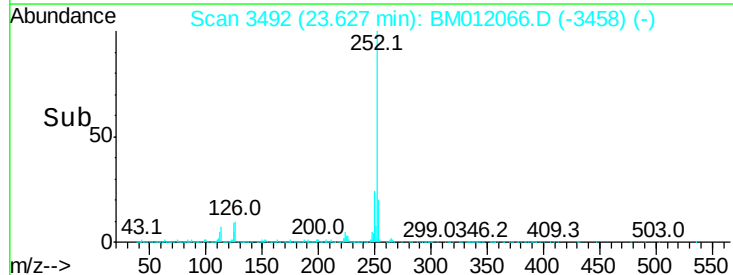

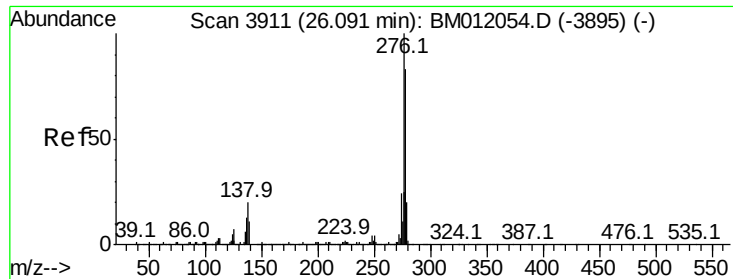





#89
Indeno(1,2,3-cd)pyrene
Concen: 8.961 ng/ul
RT: 26.09 min Scan# 3911
Delta R.T. -0.00 min
Lab File: BM012066.D
Acq: 11 Oct 2017 05:40

Instrument :
BNA_M
ClientSampled :
CB3G2

Tot Ion	Ratio	Lower	Upper
276	100		
138	18.0	9.3	13.9#
277	24.3	19.9	29.9




Manual Integrations
APPROVED


Sohil
10/11/2017 7:29:51 PM

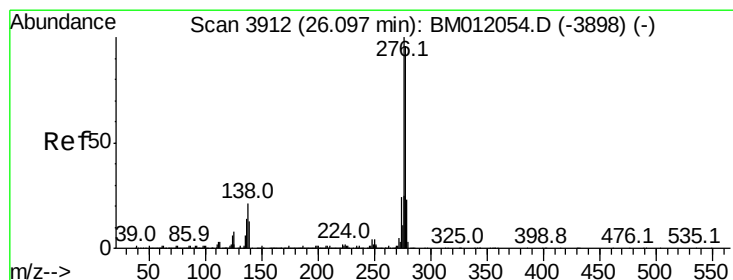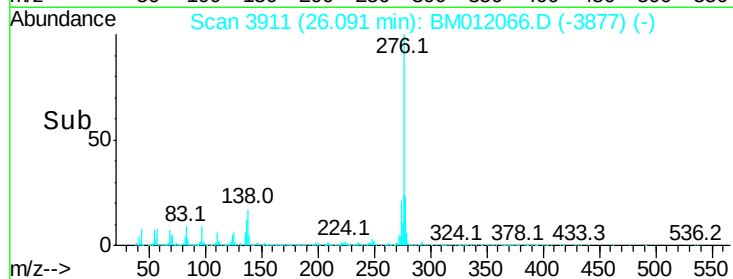

#90
Dibenzo(a,h)anthracene
Concen: 3.003 ng/ul
RT: 26.09 min Scan# 3910
Delta R.T. -0.01 min
Lab File: BM012066.D
Acq: 11 Oct 2017 05:40

Tgt Ion	Ratio	Lower	Upper
278	100		
139	19.8	5.8	8.8#
279	27.3	18.6	27.8

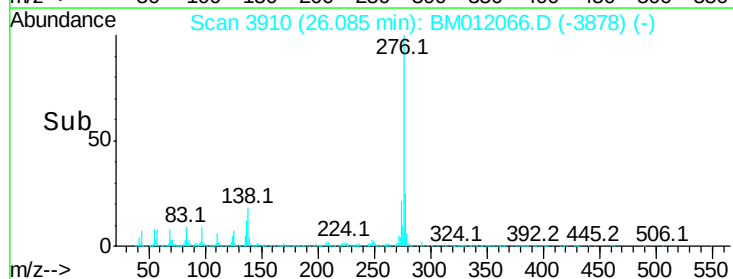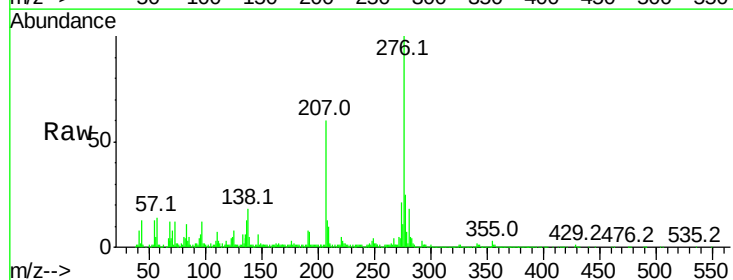

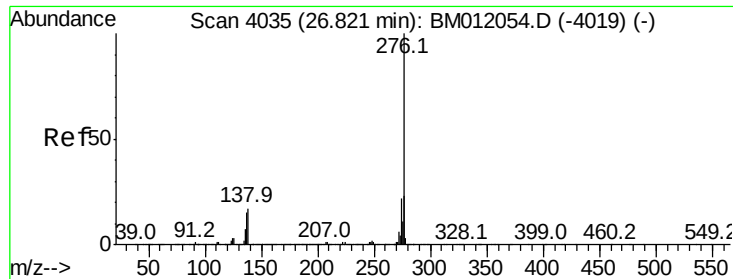

#91

Benzo(a,h,i)perylene

Concen: 8.622 ng/ul

RT: 26.82 min Scan# 4035

Delta R.T. -0.00 min

Lab File: BM012066.D

Acq: 11 Oct 2017 05:40

Instrument :

BNA_M

ClientSampleId :

CB3G2

Tot Ion:	276	Resp:	780350
Ion Ratio	Lower	Upper	
276	100		
138	17.1	8.5	12.7#
277	23.3	18.6	28.0

Manual Integrations
APPROVED

Sohil
10/11/2017 7:29:51 PM

