

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036936.D
 Acq On : 11 Oct 2022 09:06
 Operator : CG/JU
 Sample : PB148185BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK185

Quant Time: Oct 12 01:25:16 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7703	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	26309	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.576	164	14186	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.314	188	27481	0.400	ng/ul	0.00
17) Chrysene-d12	21.481	240	17276	0.400	ng/ul	0.00
23) Perylene-d12	23.878	264	13961	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	51950	4.782	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	11949	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.332	212	19932	0.386	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.566	166	3514	0.061	ng/ul#	14
20) Pyrene	19.699	202	2860	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.723	252	4302	0.085	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036936.D
Acq On : 11 Oct 2022 09:06
Operator : CG/JU
Sample : PB148185BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK185

Quant Time: Oct 12 01:25:16 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration




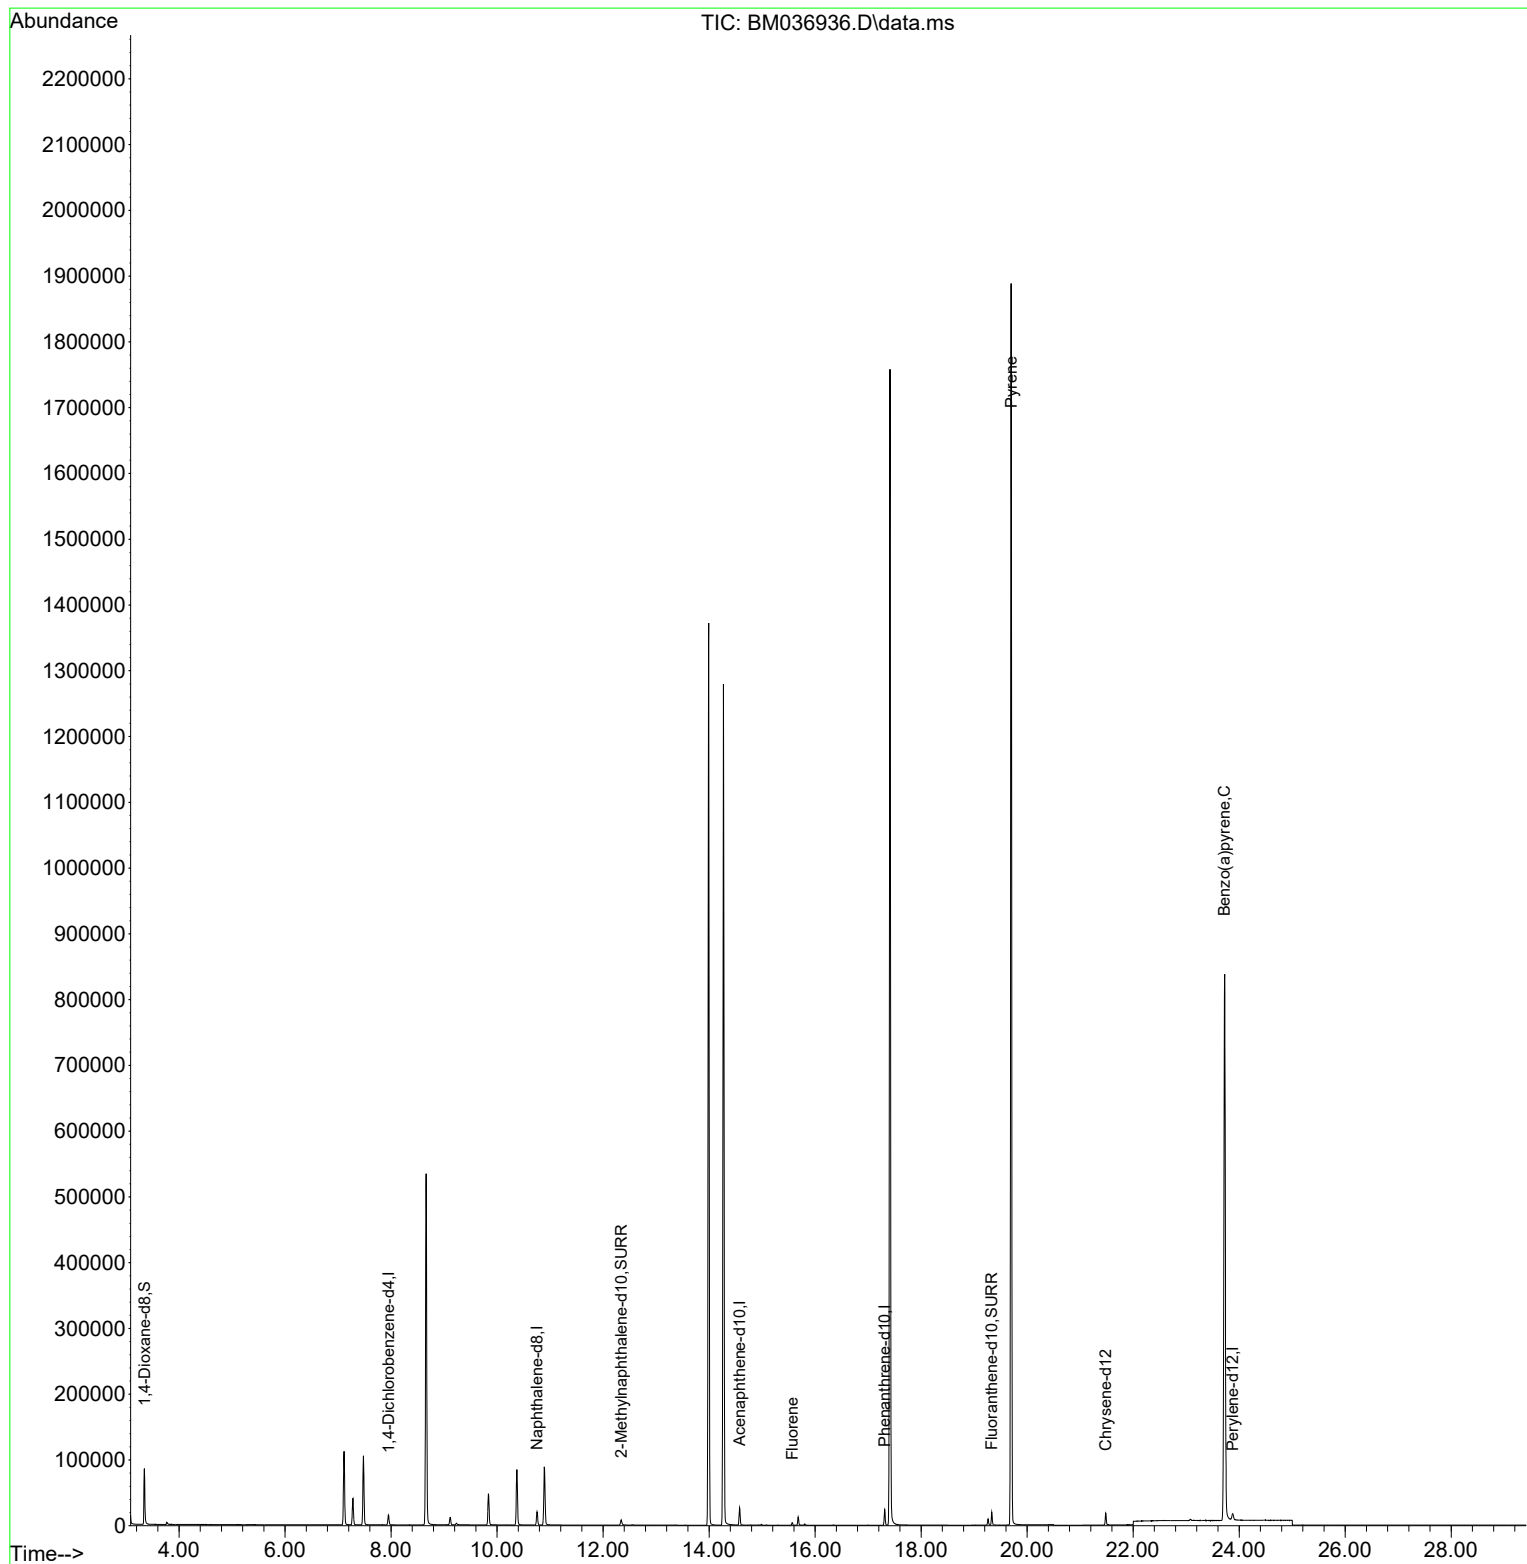


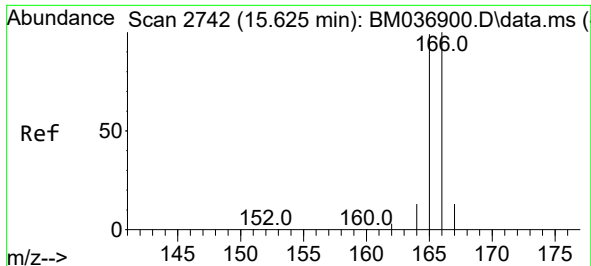

#12
Fluorene
Concen: 0.061 ng/ul
RT: 15.566 min Scan# 21
Delta R.T. -0.055 min
Lab File: BM036936.D
Acq: 11 Oct 2022 09:06




Instrument :
BNA_M
ClientSampleId :
SBLK185


Tgt Ion:166 Resp: 3514
Ion Ratio Lower Upper
166 100
165 7.3 78.9 118.3#
167 31.2 11.3 16.9#

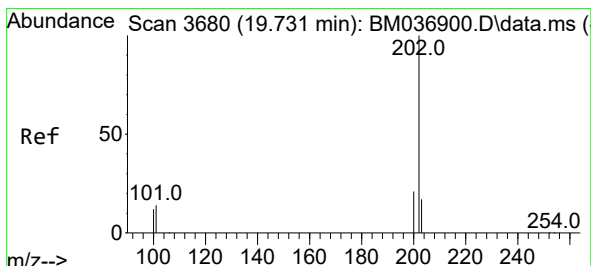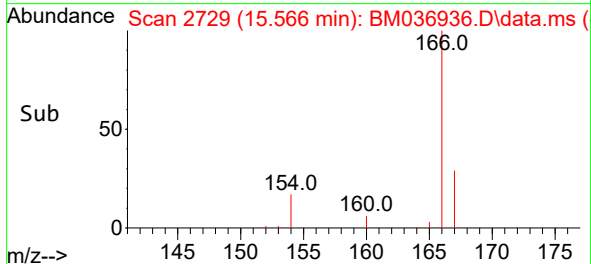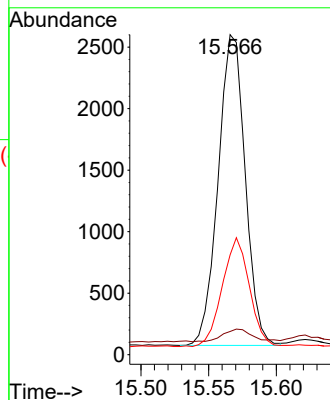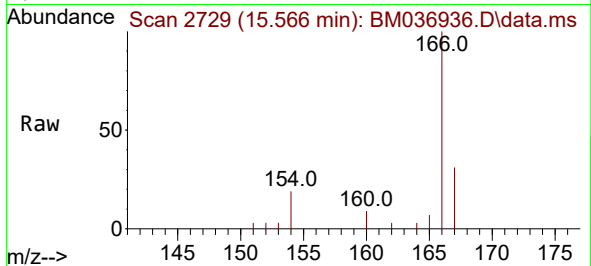

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.699 min Scan# 3673
Delta R.T. -0.027 min
Lab File: BM036936.D
Acq: 11 Oct 2022 09:06


Tgt Ion:202 Resp: 2860
Ion Ratio Lower Upper
202 100
101 162.1 12.0 18.0#
100 1180.4 9.8 14.6#

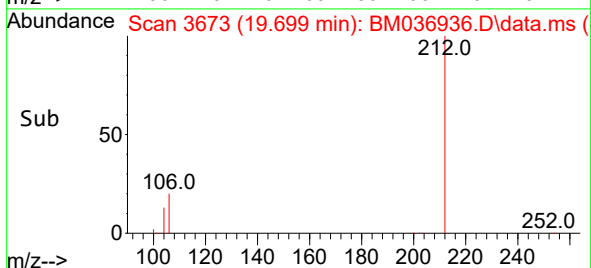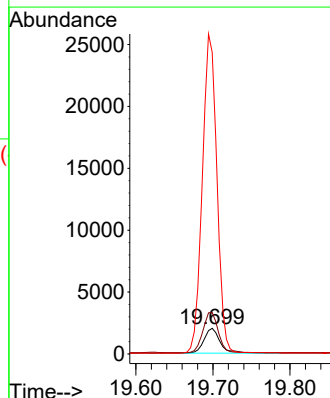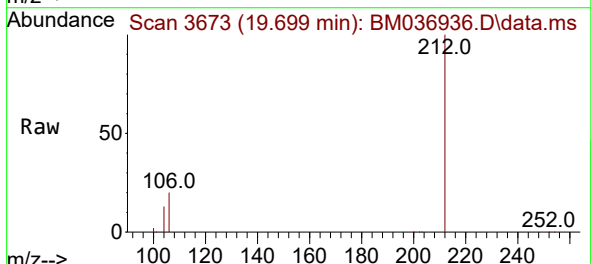

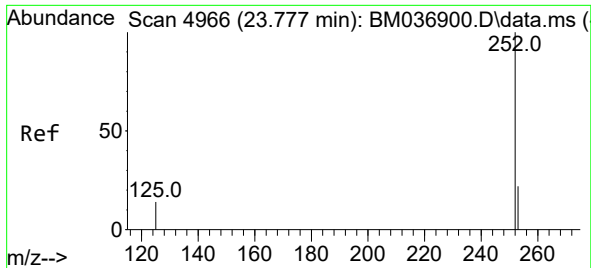

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.723 min Scan# 4948
Delta R.T. -0.048 min
Lab File: BM036936.D
Acq: 11 Oct 2022 09:06

Instrument :
BNA_M
ClientSampleId :
SBLK185

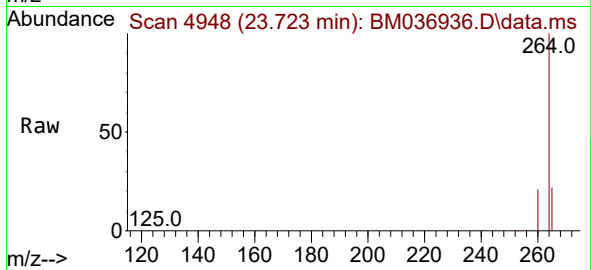

Tgt Ion:252 Resp: 4302
Ion Ratio Lower Upper
252 100
253 53.7 29.7 44.5#
125 61.9 23.6 35.4#

