

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036949.D
 Acq On : 11 Oct 2022 17:41
 Operator : CG/JU
 Sample : PB148212BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK212

Quant Time: Oct 12 01:27:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	10615	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	37811	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.580	164	21340	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.317	188	43264	0.400	ng/ul	0.00
17) Chrysene-d12	21.485	240	29070	0.400	ng/ul	0.00
23) Perylene-d12	23.885	264	22236	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	63124	4.217	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	15791	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	29377	0.338	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.570	166	4713	0.054	ng/ul#	13
20) Pyrene	19.703	202	4102	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.730	252	5999	0.074	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036949.D
Acq On : 11 Oct 2022 17:41
Operator : CG/JU
Sample : PB148212BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK212

Quant Time: Oct 12 01:27:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration




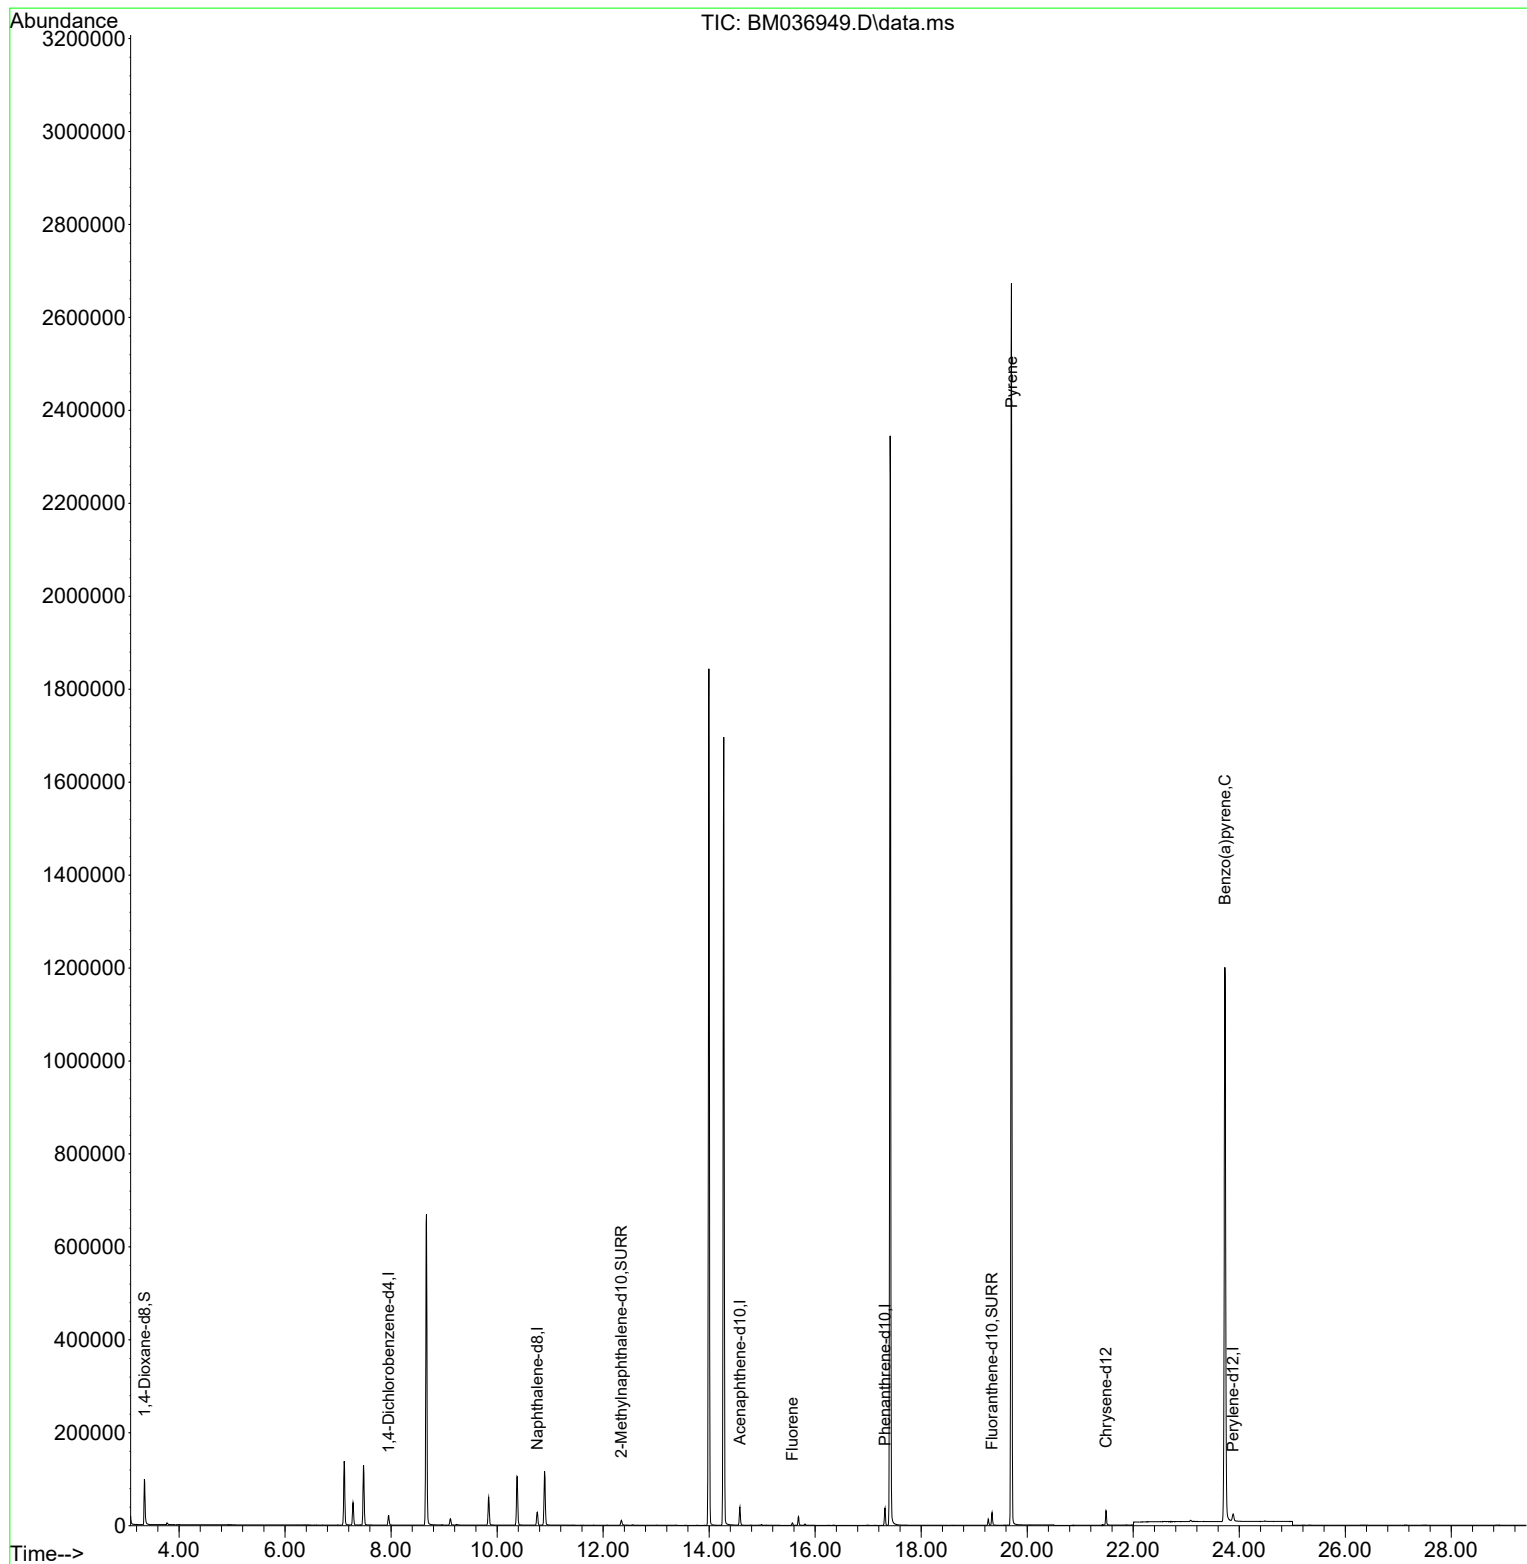


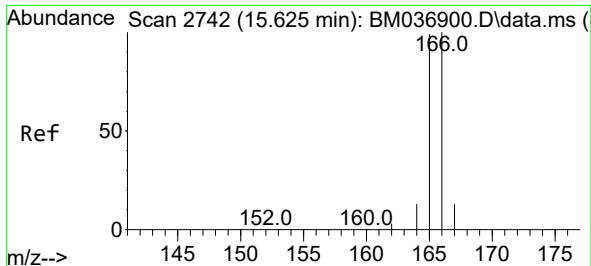

#12
Fluorene
Concen: 0.054 ng/ul
RT: 15.570 min Scan# 21
Delta R.T. -0.051 min
Lab File: BM036949.D
Acq: 11 Oct 2022 17:41




Instrument :
BNA_M
ClientSampleId :
SBLK212


Tgt Ion:166 Resp: 4713
Ion Ratio Lower Upper
166 100
165 6.9 78.9 118.3#
167 32.4 11.3 16.9#

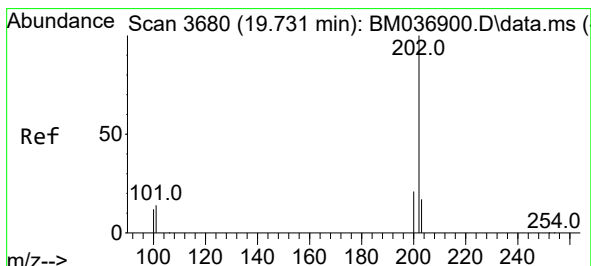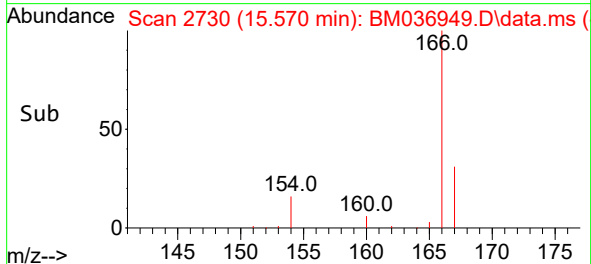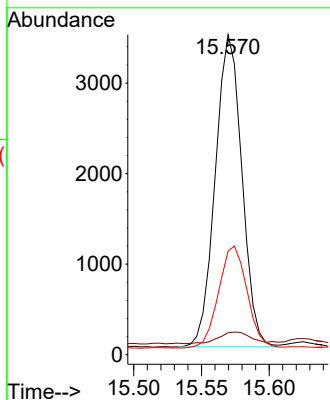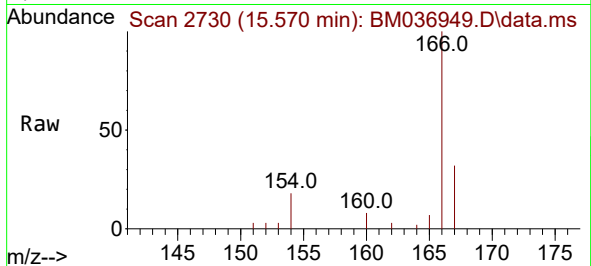

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.703 min Scan# 3674
Delta R.T. -0.023 min
Lab File: BM036949.D
Acq: 11 Oct 2022 17:41


Tgt Ion:202 Resp: 4102
Ion Ratio Lower Upper
202 100
101 155.5 12.0 18.0#
100 1122.0 9.8 14.6#

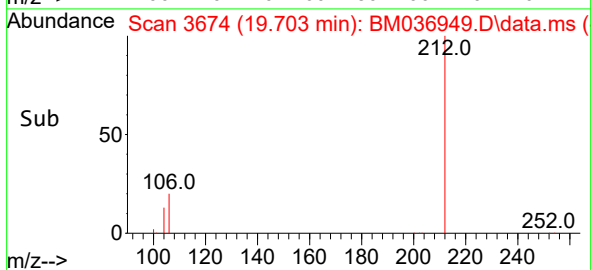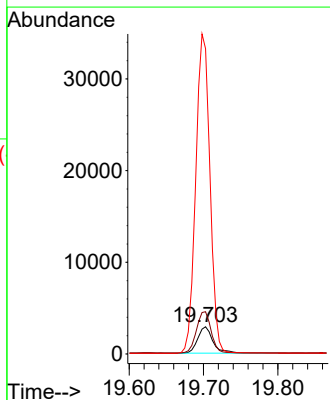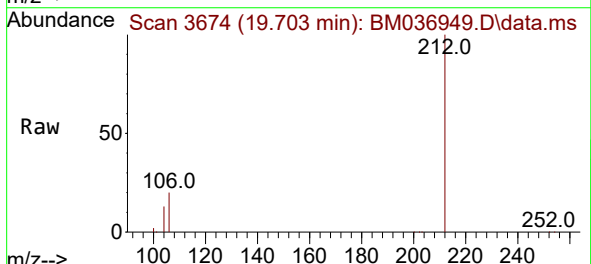

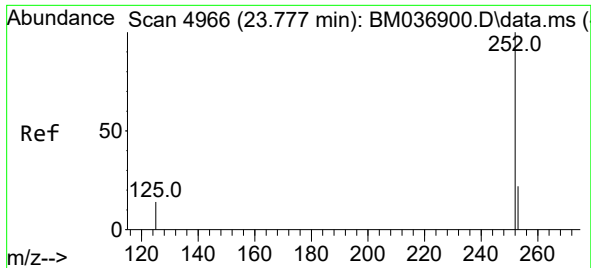

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.730 min Scan# 4950
Delta R.T. -0.041 min
Lab File: BM036949.D
Acq: 11 Oct 2022 17:41

Instrument :
BNA_M
ClientSampleId :
SBLK212

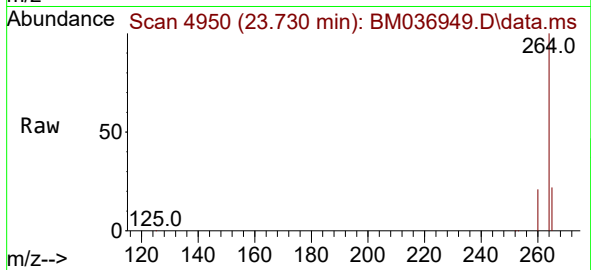

Tgt Ion:252 Resp: 5999
Ion Ratio Lower Upper
252 100
253 49.9 29.7 44.5#
125 55.7 23.6 35.4#

