

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036991.D
 Acq On : 12 Oct 2022 19:33
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 95 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 12 23:12:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	8594	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	31200	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.575	164	16118	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.317	188	27403	0.400	ng/ul	0.00
17) Chrysene-d12	21.485	240	15329	0.400	ng/ul	0.00
23) Perylene-d12	23.882	264	14110	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	3891	0.321	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.338	152	18459	0.392	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	23375	0.510	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.386	88	3948	0.333	ng/ul	90
5) Naphthalene	10.803	128	34865	0.391	ng/ul	97
7) 2-Methylnaphthalene	12.409	142	21646	0.397	ng/ul	92
8) 1-Methylnaphthalene	12.629	142	21903	0.395	ng/ul	99
10) Acenaphthylene	14.297	152	28564	0.426	ng/ul	98
11) Acenaphthene	14.640	153	22600	0.389	ng/ul	98
12) Fluorene	15.621	166	23781	0.361	ng/ul	98
14) Pentachlorophenol	16.971	266	1992	0.300	ng/ul	99
15) Phenanthrene	17.355	178	33511	0.383	ng/ul	99
16) Anthracene	17.448	178	30226	0.413	ng/ul	98
19) Fluoranthene	19.368	202	30398	0.499	ng/ul	98
20) Pyrene	19.726	202	30540	0.480	ng/ul	99
21) Benzo(a)anthracene	21.468	228	23107	0.417	ng/ul	100
22) Chrysene	21.520	228	22928	0.386	ng/ul	99
24) Benzo(b)fluoranthene	23.151	252	22264	0.353	ng/ul	96
25) Benzo(k)fluoranthene	23.198	252	22073	0.359	ng/ul	97
26) Benzo(a)pyrene	23.774	252	20025	0.392	ng/ul	94
27) Indeno(1,2,3-cd)pyrene	26.373	276	27036	0.373	ng/ul	99
28) Dibenzo(a,h)anthracene	26.390	278	21490	0.367	ng/ul	95
29) Benzo(g,h,i)perylene	27.138	276	22825	0.358	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036991.D
Acq On : 12 Oct 2022 19:33
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 95 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 12 23:12:54 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration




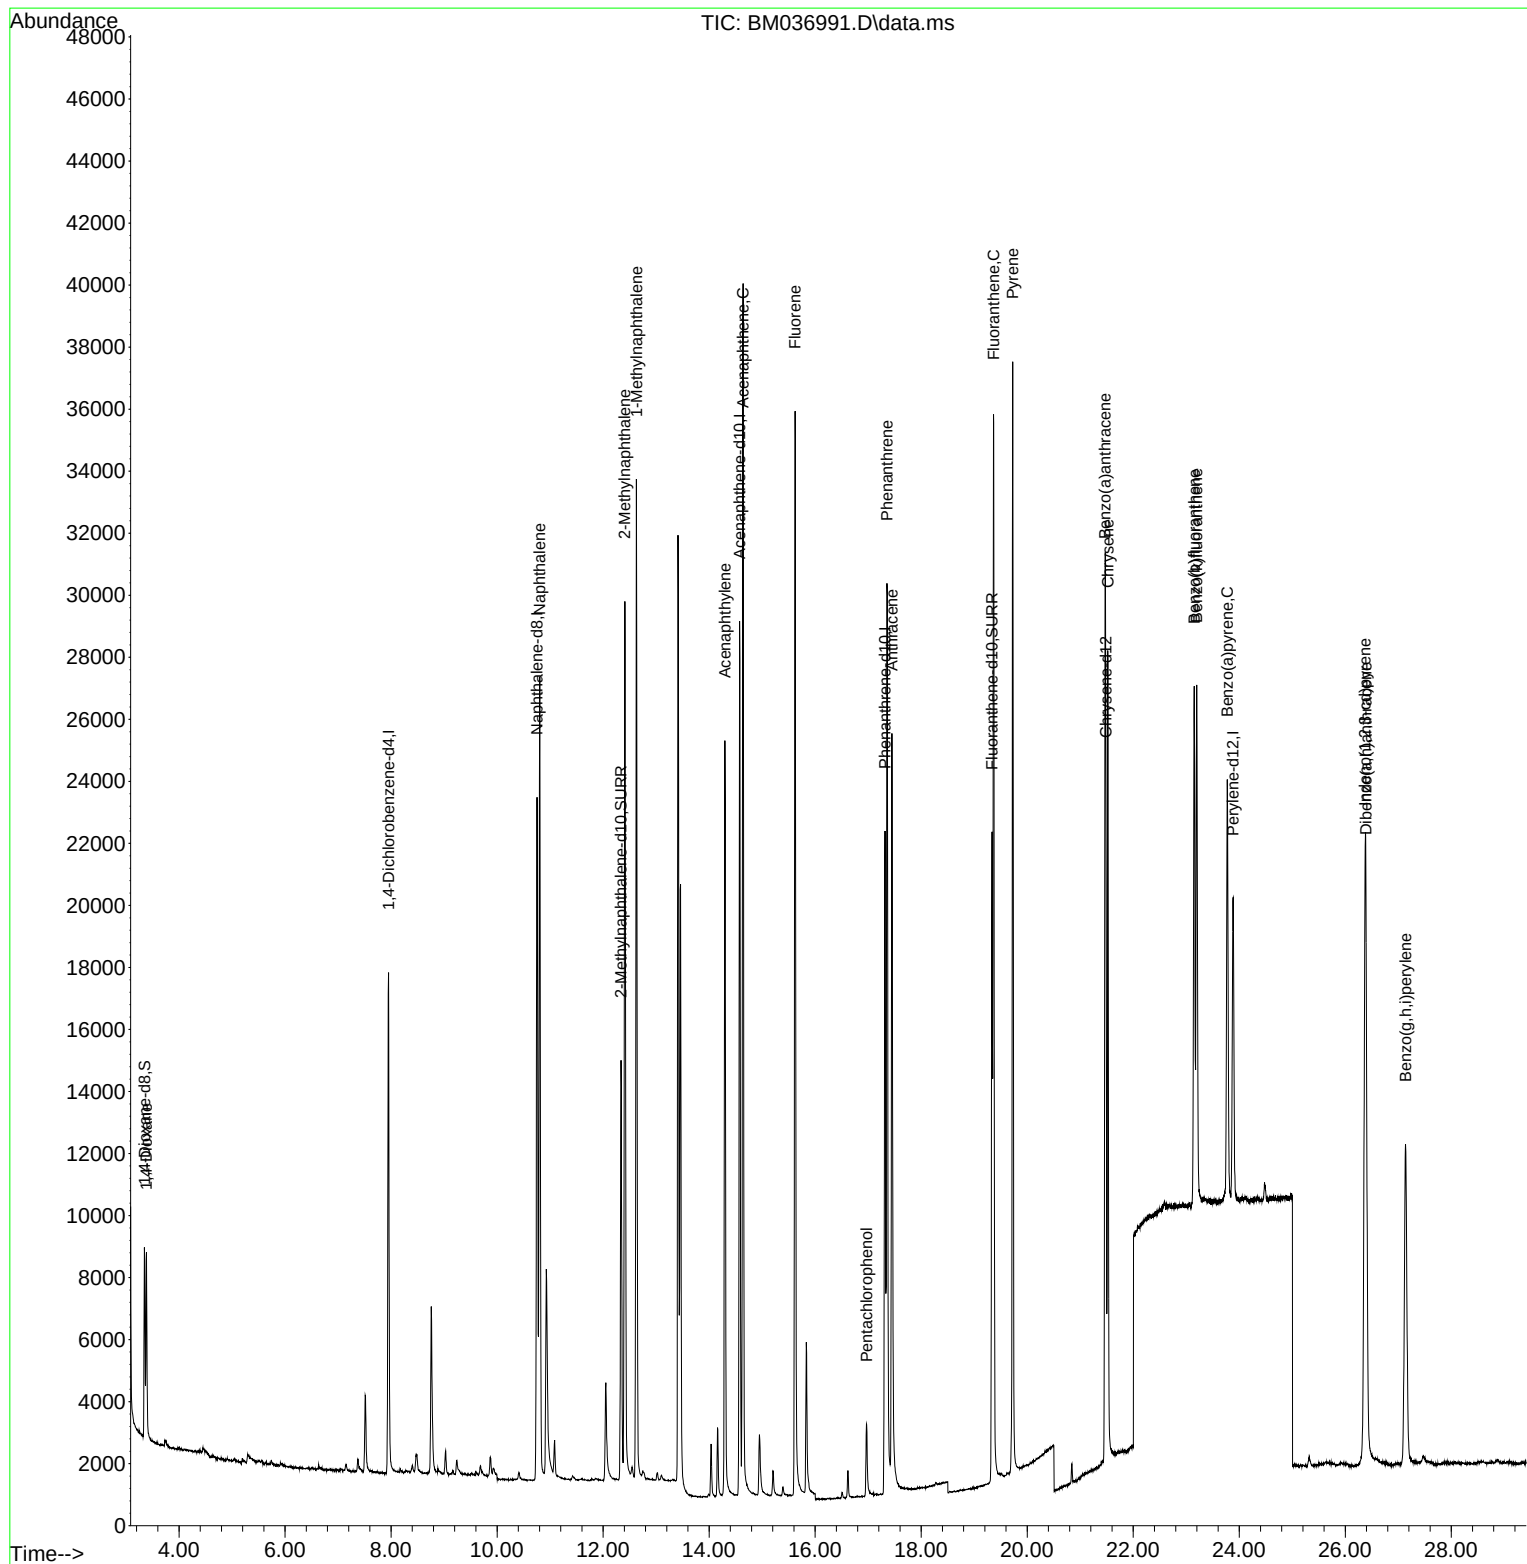




#2
 1,4-Dioxane
 Concen: 0.333 ng/ul
 RT: 3.386 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BM036991.D
 Acq: 12 Oct 2022 19:33




Instrument :
 BNA_M
 ClientSampleId :


Tgt Ion: 88 Resp: 3948
 Ion Ratio Lower Upper
 88 100
 43 42.8 37.8 56.6
 58 63.1 42.6 63.8

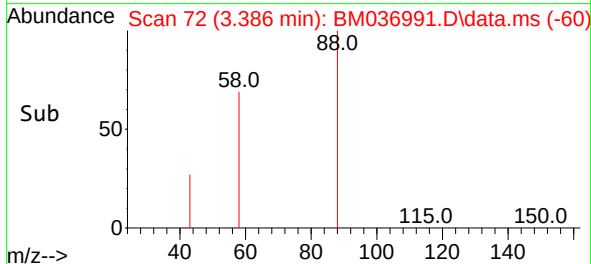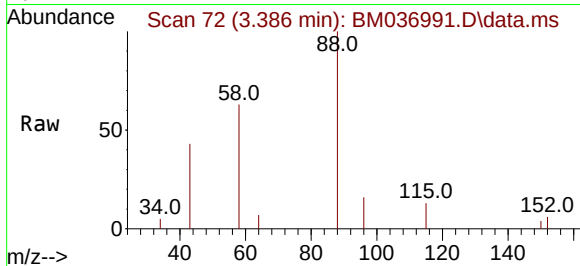

#5
 Naphthalene
 Concen: 0.391 ng/ul
 RT: 10.803 min Scan# 1789
 Delta R.T. 0.000 min
 Lab File: BM036991.D
 Acq: 12 Oct 2022 19:33

Tgt Ion: 128 Resp: 34865
 Ion Ratio Lower Upper
 128 100
 129 11.7 10.2 15.2
 127 13.1 11.7 17.5


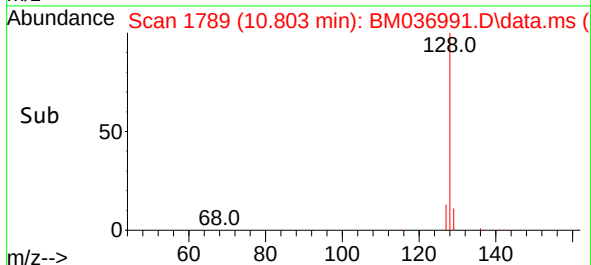

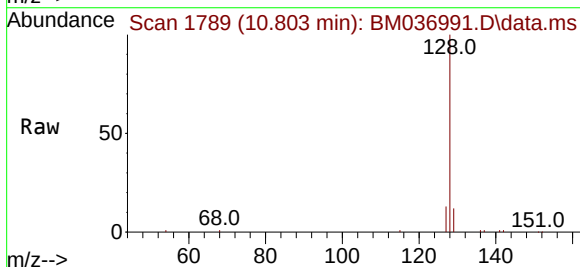




#7
2-Methylnaphthalene
Concen: 0.397 ng/ul
RT: 12.409 min Scan# 2081
Delta R.T. -0.005 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:142 Resp: 21646
Ion Ratio Lower Upper
142 100
141 88.5 77.4 116.0

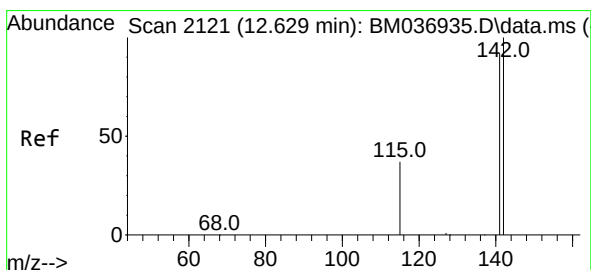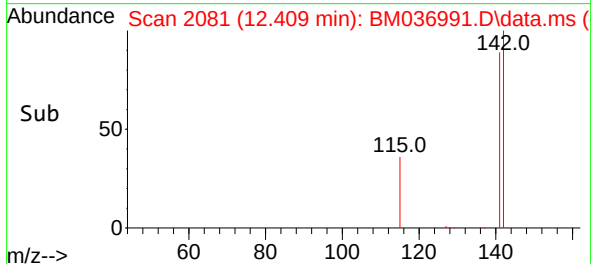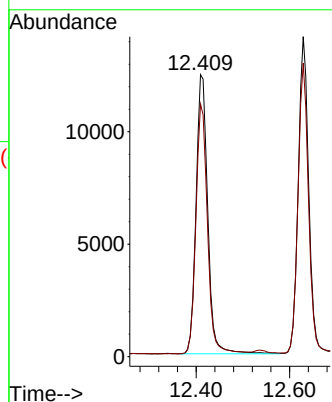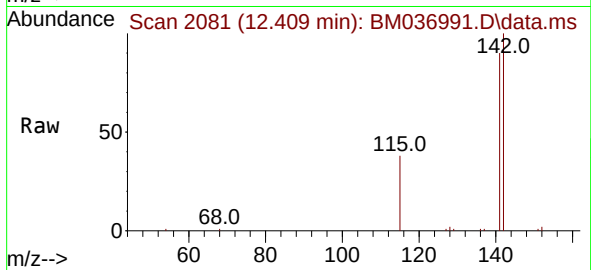

#8
1-Methylnaphthalene
Concen: 0.395 ng/ul
RT: 12.629 min Scan# 2121
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

Tgt Ion:142 Resp: 21903
Ion Ratio Lower Upper
142 100
141 91.7 74.1 111.1


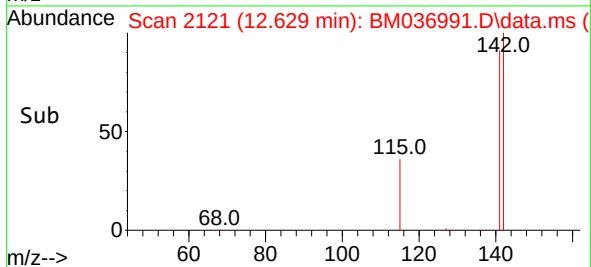
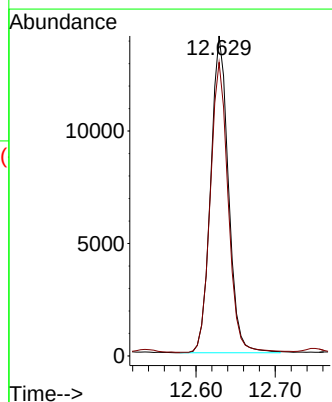
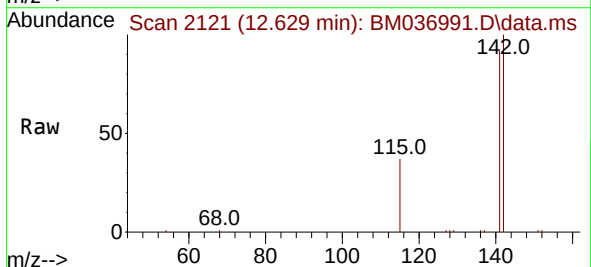




#10
Acenaphthylene
Concen: 0.426 ng/ul
RT: 14.297 min Scan# 2455
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:152 Resp: 28564
Ion Ratio Lower Upper
152 100
151 20.0 16.6 24.8
153 13.5 11.4 17.0

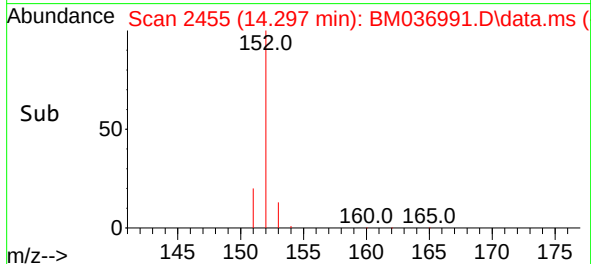

#11
Acenaphthene
Concen: 0.389 ng/ul
RT: 14.640 min Scan# 2529
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33


Tgt Ion:153 Resp: 22600
Ion Ratio Lower Upper
153 100
152 50.1 40.2 60.4
154 89.3 69.7 104.5

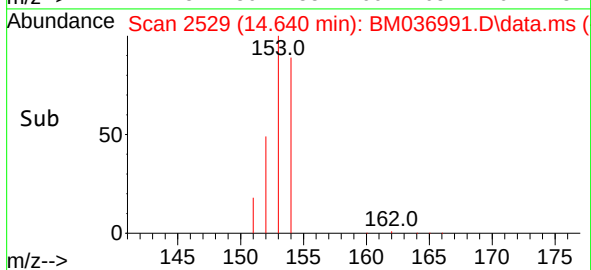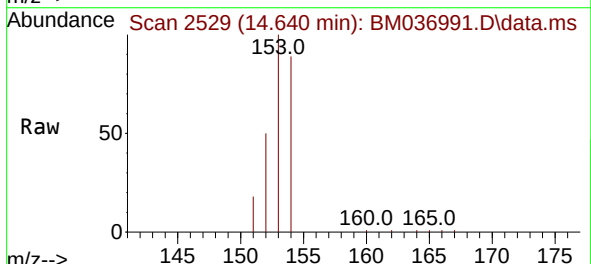






#12
Fluorene
Concen: 0.361 ng/ul
RT: 15.621 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

Instrument :
BNA_M
ClientSampleId :







Tgt Ion:166 Resp: 23781
Ion Ratio Lower Upper
166 100
165 100.8 78.9 118.3
167 13.8 11.3 16.9

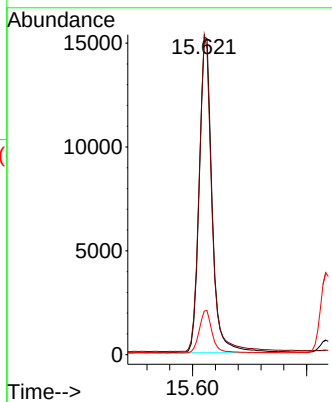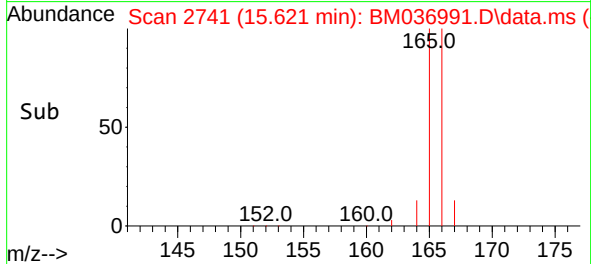

#14
Pentachlorophenol
Concen: 0.300 ng/ul
RT: 16.971 min Scan# 3053
Delta R.T. 0.004 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

Tgt Ion:266 Resp: 1992
Ion Ratio Lower Upper
266 100
264 62.1 50.3 75.5
268 65.5 53.5 80.3



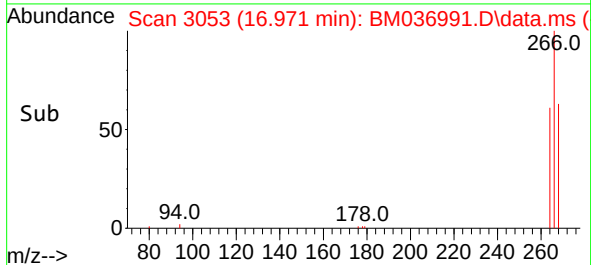
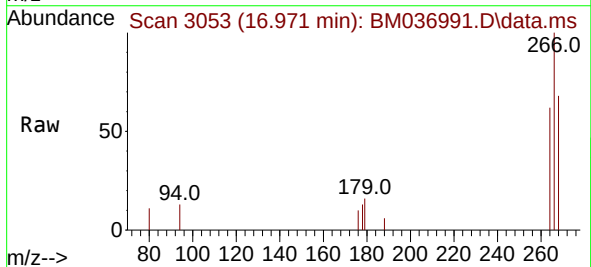




#15
Phenanthrene
Concen: 0.383 ng/u1
RT: 17.355 min Scan# 3144
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:178 Resp: 33511
Ion Ratio Lower Upper
178 100
179 16.0 13.0 19.6
176 19.7 15.6 23.4

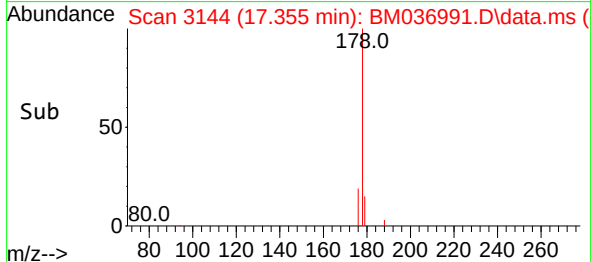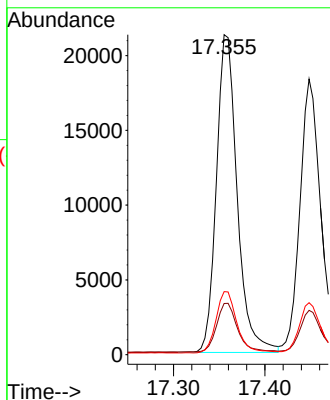

#16
Anthracene
Concen: 0.413 ng/u1
RT: 17.448 min Scan# 3166
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33


Tgt Ion:178 Resp: 30226
Ion Ratio Lower Upper
178 100
179 16.1 13.6 20.4
176 18.8 15.6 23.4

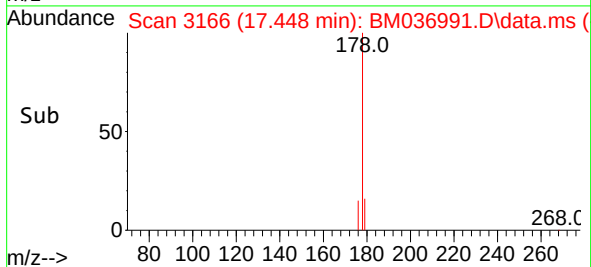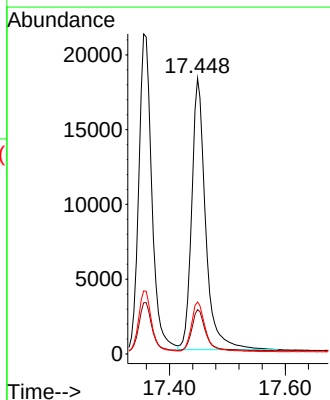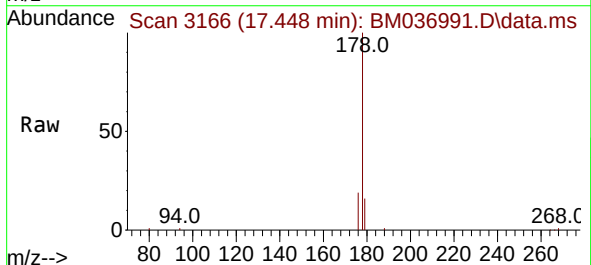






#19
Fluoranthene
Concen: 0.499 ng/ul
RT: 19.368 min Scan# 3602
Delta R.T. 0.005 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33


Instrument :
BNA_M
ClientSampleId :





Tgt Ion:202 Resp: 30398
Ion Ratio Lower Upper
202 100
101 12.0 10.1 15.1
100 8.8 7.9 11.9

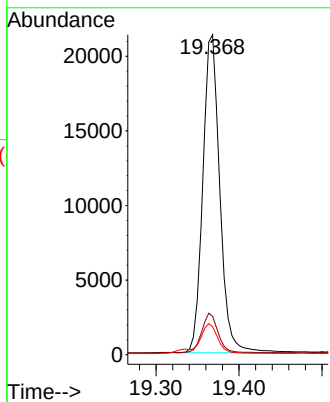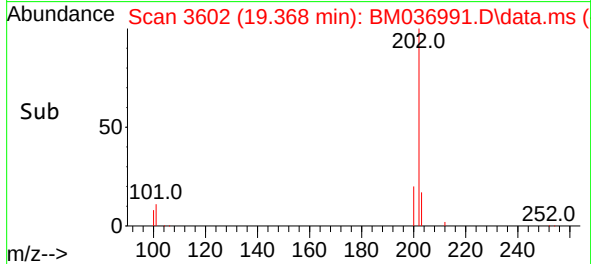


#20
Pyrene
Concen: 0.480 ng/ul
RT: 19.726 min Scan# 3679
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

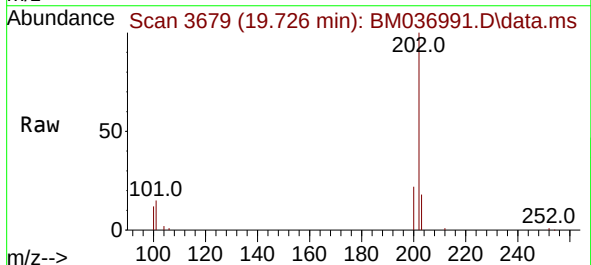

Tgt Ion:202 Resp: 30540
Ion Ratio Lower Upper
202 100
101 14.7 12.0 18.0
100 11.5 9.8 14.6



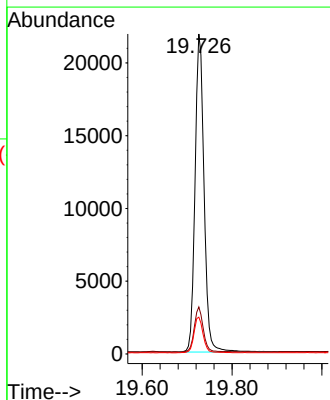
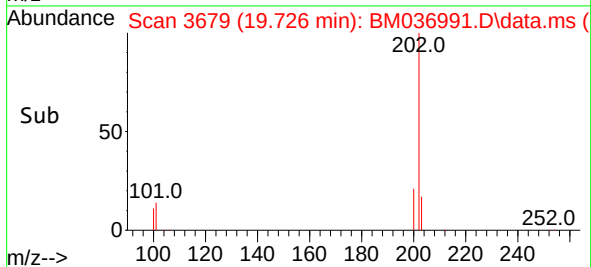




#21
Benzo(a)anthracene
Concen: 0.417 ng/ul
RT: 21.468 min Scan# 4176
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:228 Resp: 23107
Ion Ratio Lower Upper
228 100
229 20.4 16.2 24.2
226 28.1 22.5 33.7

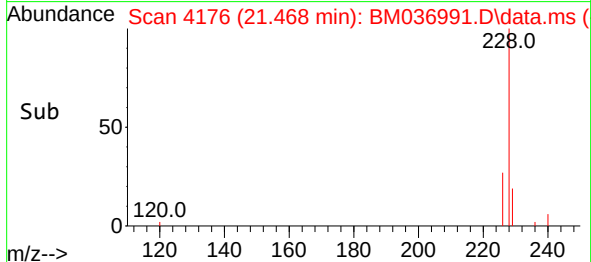

#22
Chrysene
Concen: 0.386 ng/ul
RT: 21.520 min Scan# 4194
Delta R.T. 0.000 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

Tgt Ion:228 Resp: 22928
Ion Ratio Lower Upper
228 100
226 31.2 24.6 37.0
229 20.2 16.4 24.6


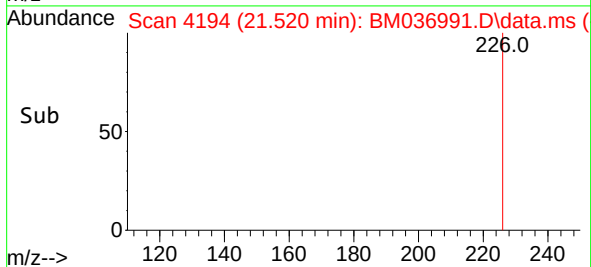

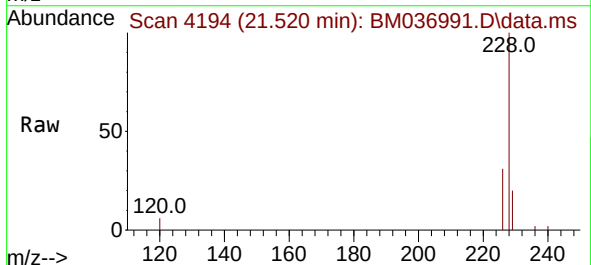




#24
Benzo(b)fluoranthene
Concen: 0.353 ng/ul
RT: 23.151 min Scan# 4752
Delta R.T. 0.006 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:252 Resp: 22264
Ion Ratio Lower Upper
252 100
253 30.0 0.0 61.4
125 25.3 0.0 42.6

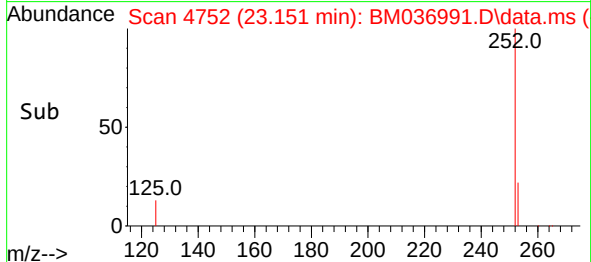

#25
Benzo(k)fluoranthene
Concen: 0.359 ng/ul
RT: 23.198 min Scan# 4768
Delta R.T. 0.003 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33


Tgt Ion:252 Resp: 22073
Ion Ratio Lower Upper
252 100
253 30.1 25.2 37.8
125 25.0 18.3 27.5

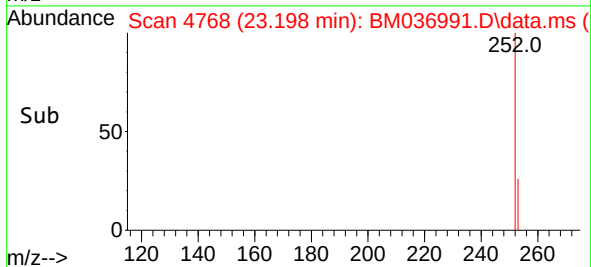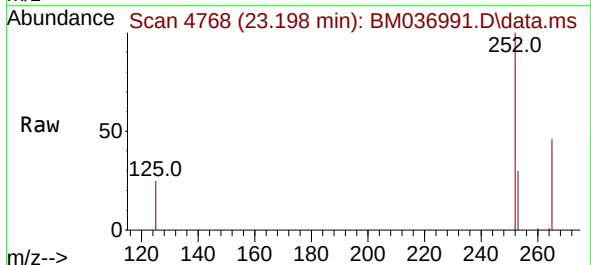






#26
Benzo(a)pyrene
Concen: 0.392 ng/ul
RT: 23.774 min Scan# 4964
Delta R.T. 0.003 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

Instrument :
BNA_M
ClientSampleId :







Tgt Ion:252 Resp: 20025
Ion Ratio Lower Upper
252 100
253 32.1 29.7 44.5
125 30.9 23.6 35.4

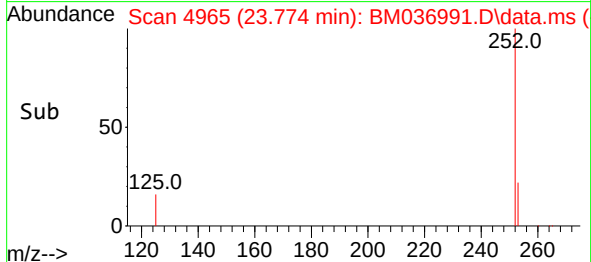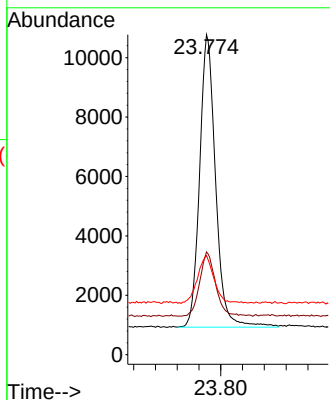

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.373 ng/ul
RT: 26.373 min Scan# 5794
Delta R.T. 0.010 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

Tgt Ion:276 Resp: 27036
Ion Ratio Lower Upper
276 100
138 30.7 23.9 35.9
227 0.1 0.1 0.1


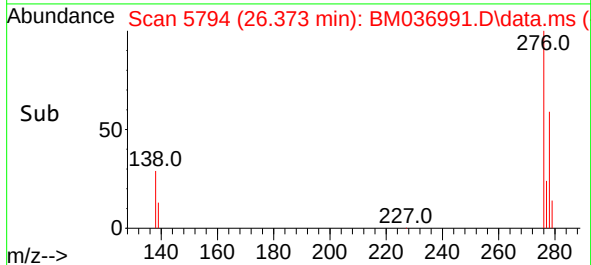
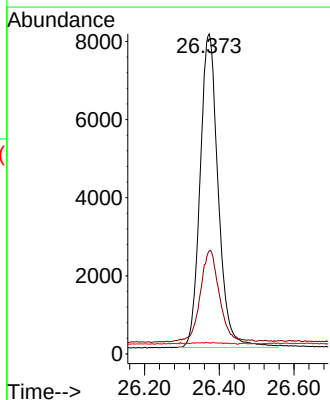
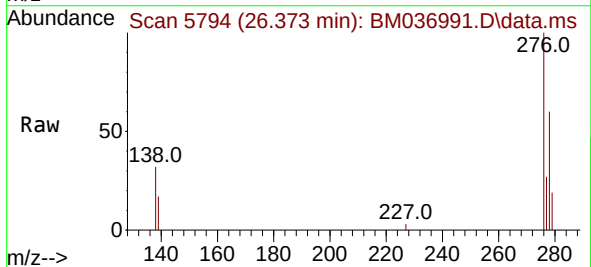




#28
Dibenzo(a,h)anthracene
Concen: 0.367 ng/ul
RT: 26.390 min Scan# 51
Delta R.T. 0.010 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:278 Resp: 21490
Ion Ratio Lower Upper
278 100
139 25.5 19.8 29.6
279 30.1 27.7 41.5

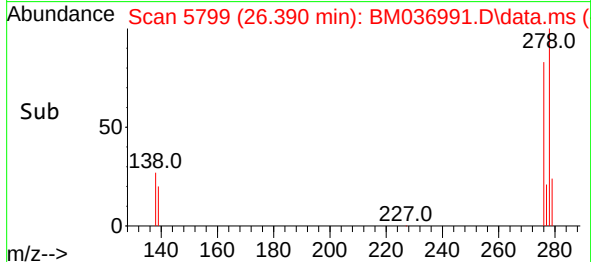

#29
Benzo(g,h,i)perylene
Concen: 0.358 ng/ul
RT: 27.138 min Scan# 6022
Delta R.T. 0.010 min
Lab File: BM036991.D
Acq: 12 Oct 2022 19:33

Tgt Ion:276 Resp: 22825
Ion Ratio Lower Upper
276 100
138 29.6 23.4 35.0
277 26.8 21.0 31.4

