

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036914.D
 Acq On : 10 Oct 2022 19:01
 Operator : CG/JU
 Sample : N4952-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8T4

Quant Time: Oct 11 02:18:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 10 00:54:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	9088	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	32647	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.584	164	18736	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.317	188	38346	0.400	ng/ul	0.00
17) Chrysene-d12	21.488	240	24202	0.400	ng/ul	0.00
23) Perylene-d12	23.885	264	19558	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	42843	3.343	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.349	152	12353	0.251	ng/ul	0.00
18) Fluoranthene-d10	19.340	212	28852	0.399	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.386	88	1644	0.131	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036914.D
Acq On : 10 Oct 2022 19:01
Operator : CG/JU
Sample : N4952-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8T4

Quant Time: Oct 11 02:18:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 00:54:15 2022
Response via : Initial Calibration

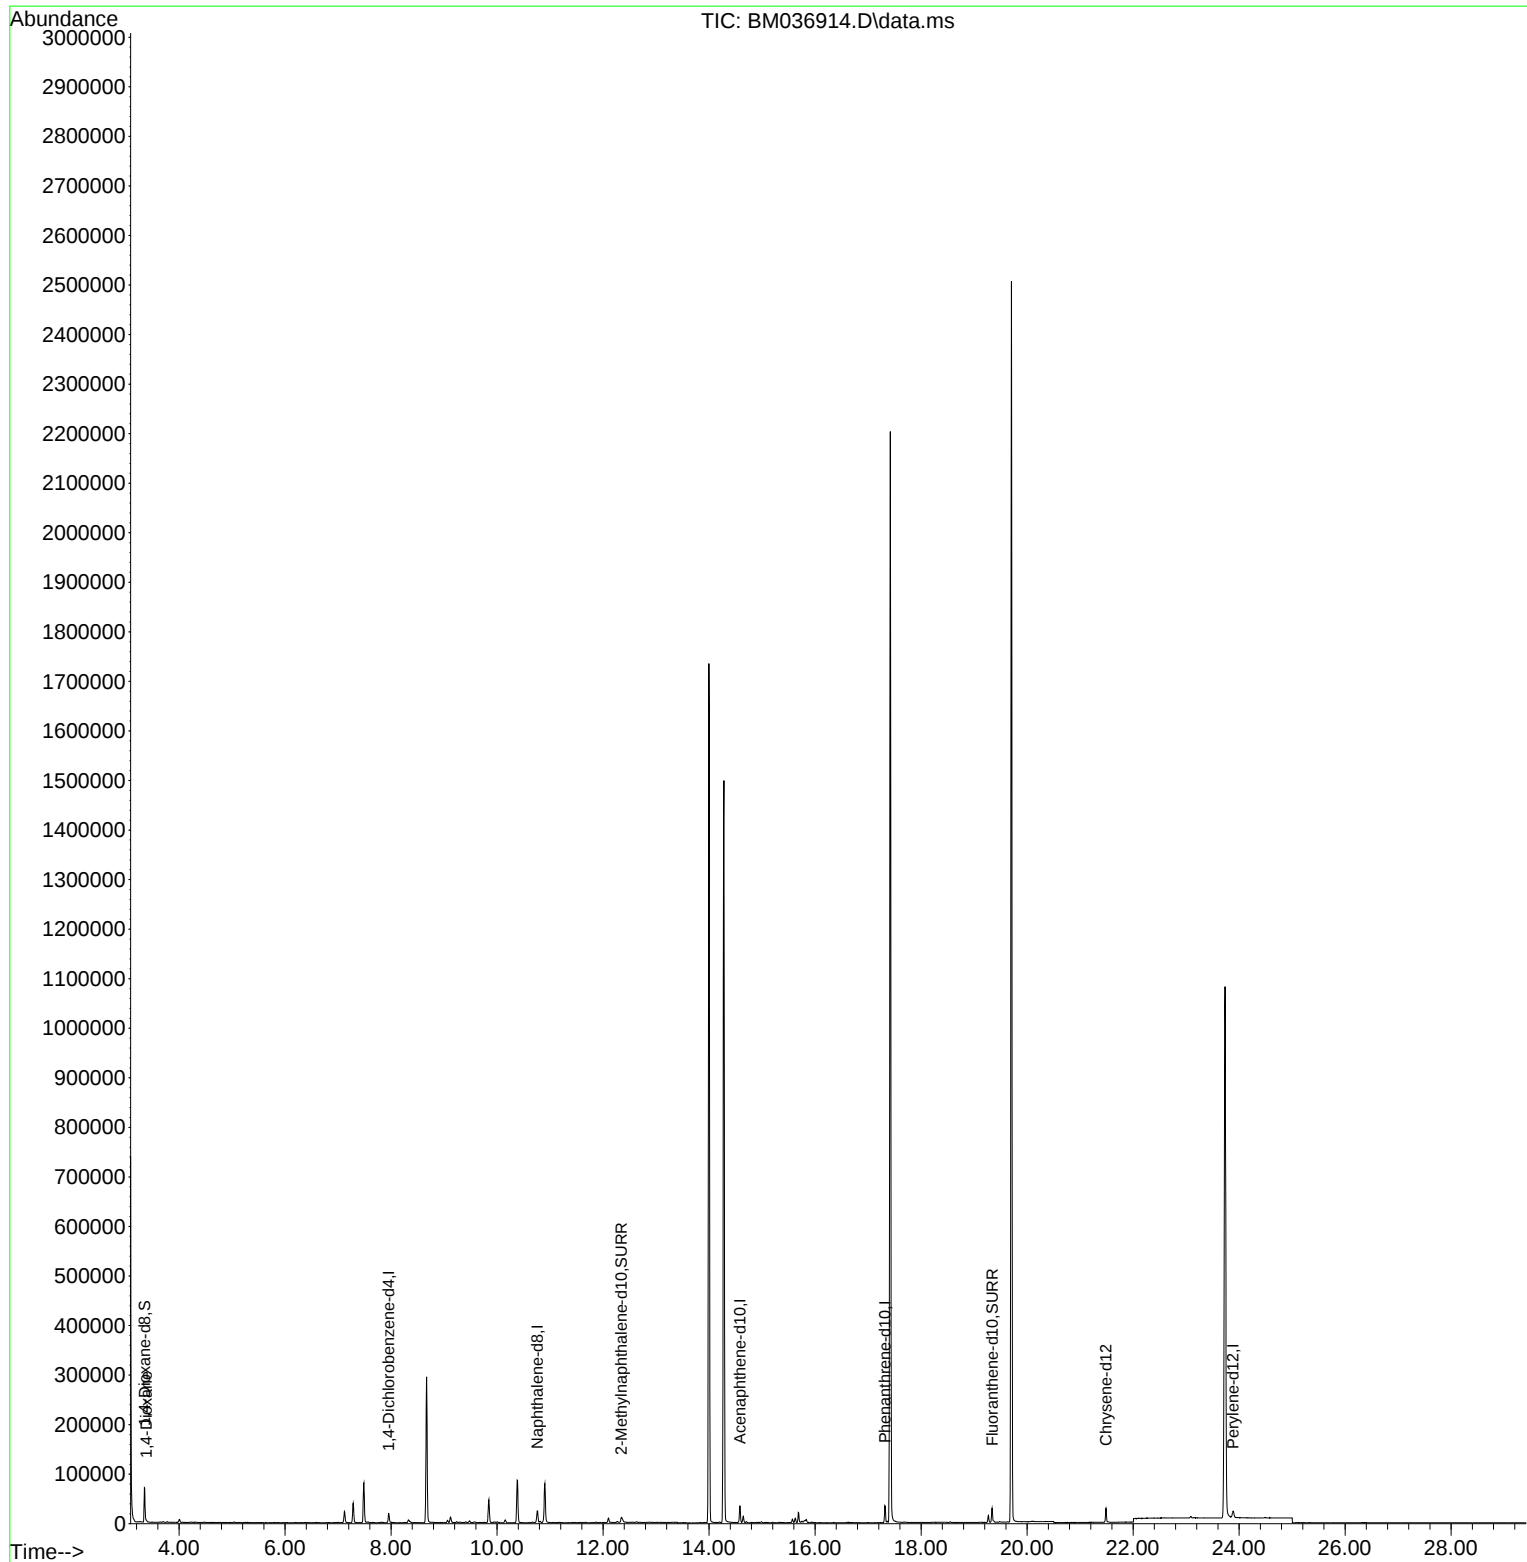

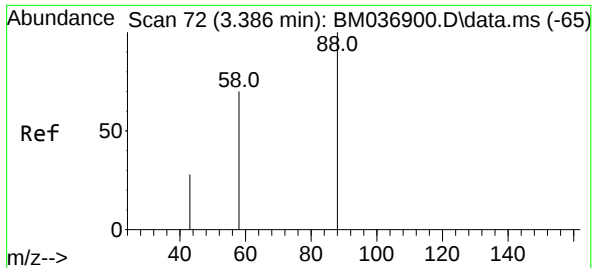

#2
 1,4-Dioxane
 Concen: 0.131 ng/ul
 RT: 3.386 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM036914.D
 Acq: 10 Oct 2022 19:01

Instrument :
 BNA_M
 ClientSampleId :
 CB8T4

Tgt Ion: 88	Resp: 1644
Ion Ratio	Lower Upper
88	100
43	69.5 37.8 56.6#
58	64.5 42.6 63.8#

