

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036927.D
 Acq On : 11 Oct 2022 03:16
 Operator : CG/JU
 Sample : N4991-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BG1

Quant Time: Oct 11 03:52:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 10 00:54:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7479	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	25840	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.576	164	14152	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.314	188	28871	0.400	ng/ul	0.00
17) Chrysene-d12	21.481	240	22806	0.400	ng/ul	0.00
23) Perylene-d12	23.878	264	18755	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	57895	5.489	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	14362	0.368	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	24087	0.353	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.803	128	2645	0.036	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036927.D
Acq On : 11 Oct 2022 03:16
Operator : CG/JU
Sample : N4991-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BG1


Quant Time: Oct 11 03:52:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 00:54:15 2022
Response via : Initial Calibration

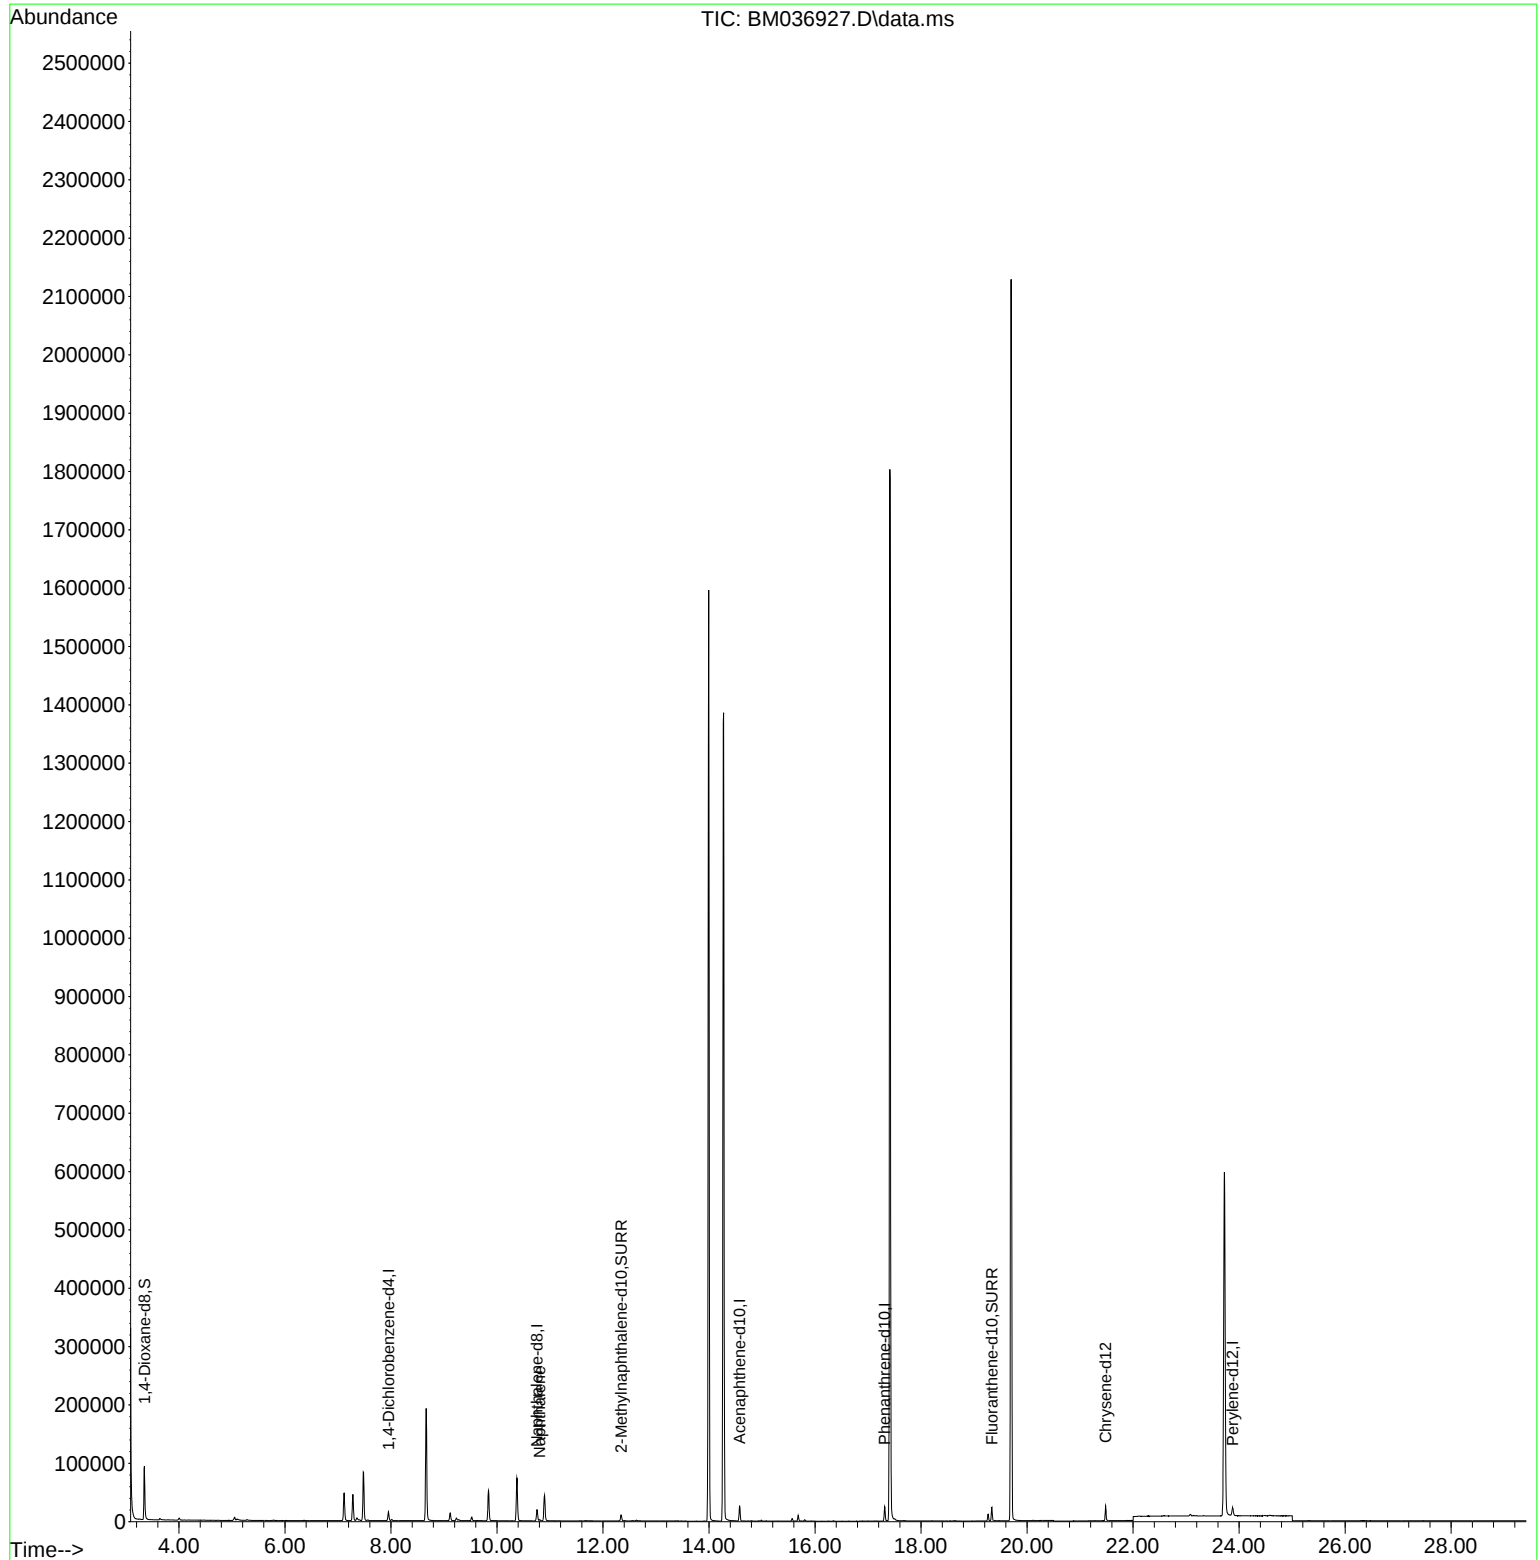

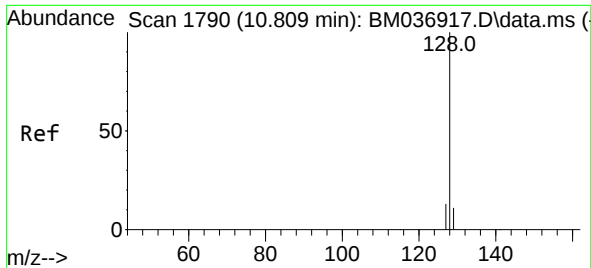

#5
Naphthalene
Concen: 0.036 ng/ul
RT: 10.803 min Scan# 11
Delta R.T. -0.011 min
Lab File: BM036927.D
Acq: 11 Oct 2022 03:16

Instrument :
BNA_M
ClientSampleId :
C0BG1

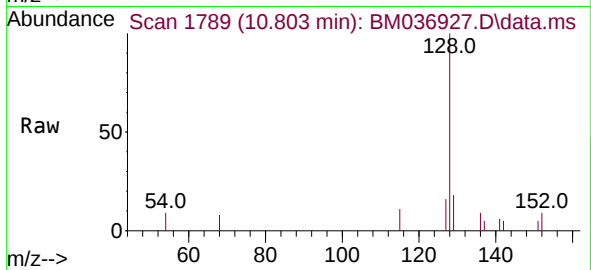

Tgt Ion:128 Resp: 2645
Ion Ratio Lower Upper
128 100
129 17.9 10.2 15.2#
127 15.7 11.7 17.5

