

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036932.D
 Acq On : 11 Oct 2022 06:11
 Operator : CG/JU
 Sample : N4991-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BF9

Quant Time: Oct 11 06:46:31 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 10 00:54:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7608	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	26126	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.576	164	14458	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.314	188	29076	0.400	ng/ul	0.00
17) Chrysene-d12	21.481	240	21580	0.400	ng/ul	0.00
23) Perylene-d12	23.878	264	17748	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	73526	6.853	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.338	152	16737	0.424	ng/ul	-0.01
18) Fluoranthene-d10	19.336	212	30555	0.473	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.803	128	2531	0.034	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036932.D
Acq On : 11 Oct 2022 06:11
Operator : CG/JU
Sample : N4991-07
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BF9


Quant Time: Oct 11 06:46:31 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 00:54:15 2022
Response via : Initial Calibration

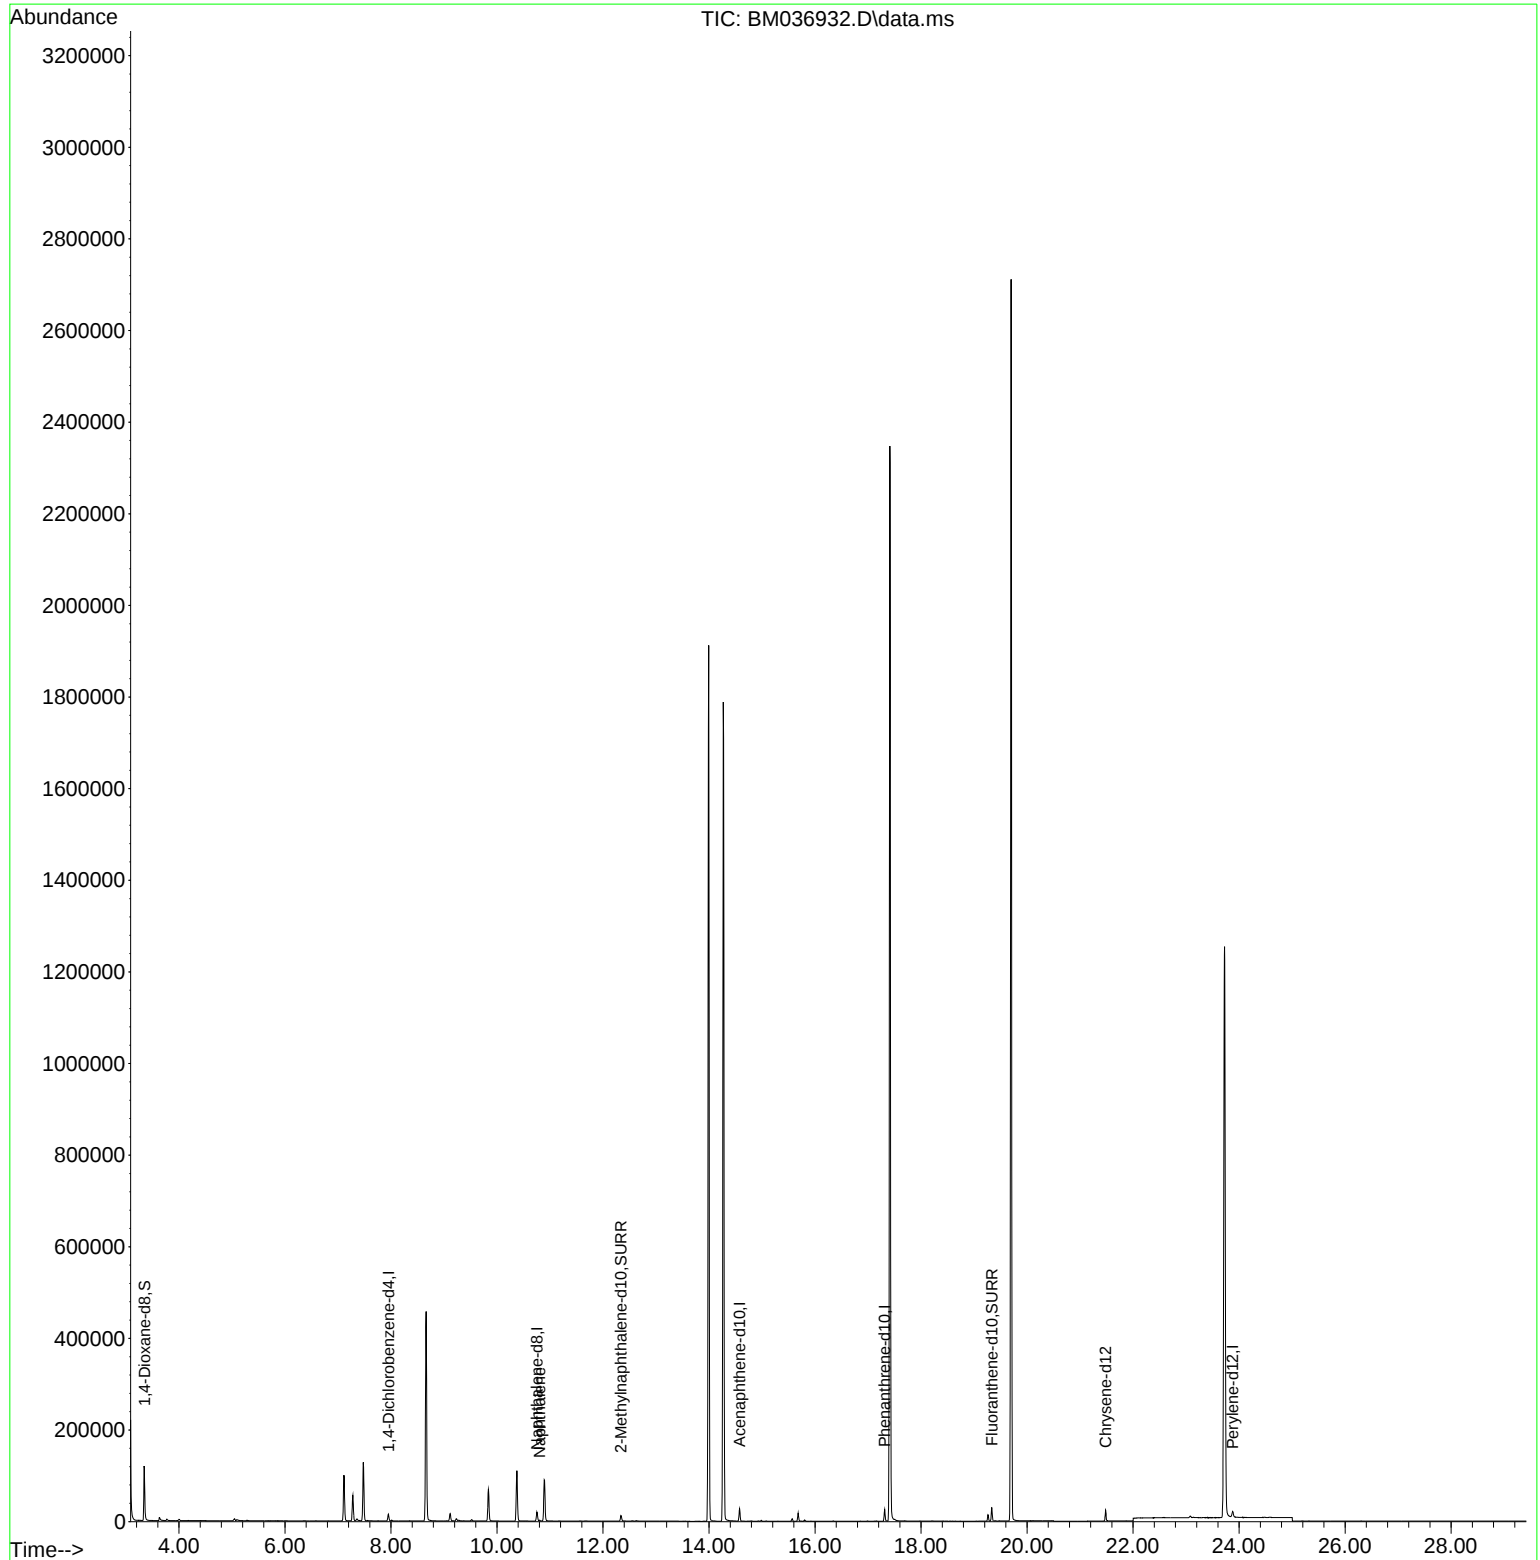

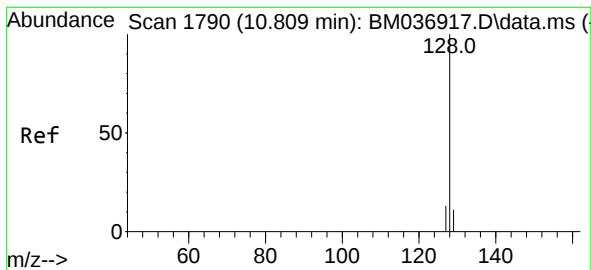

#5
Naphthalene
Concen: 0.034 ng/ul
RT: 10.803 min Scan# 11
Delta R.T. -0.011 min
Lab File: BM036932.D
Acq: 11 Oct 2022 06:11

Instrument :
BNA_M
ClientSampleId :
C0BF9

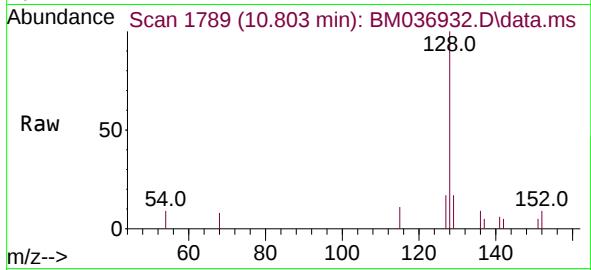

Tgt Ion:128 Resp: 2531
Ion Ratio Lower Upper
128 100
129 16.6 10.2 15.2#
127 16.8 11.7 17.5

