

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036969.D
 Acq On : 12 Oct 2022 06:08
 Operator : CG/JU
 Sample : N4980-04
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8X1

Quant Time: Oct 12 07:32:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.947	152	9199	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	31834	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.571	164	19489	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.310	188	31784	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.481	240	19378	0.400	ng/ul	# 0.00
23) Perylene-d12	23.875	264	18898	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.344	96	41933	3.232	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	11763	0.245	ng/ul	0.00
18) Fluoranthene-d10	19.332	212	19330	0.334	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.382	88	336646	26.547	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036969.D
Acq On : 12 Oct 2022 06:08
Operator : CG/JU
Sample : N4980-04
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8X1


Quant Time: Oct 12 07:32:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration

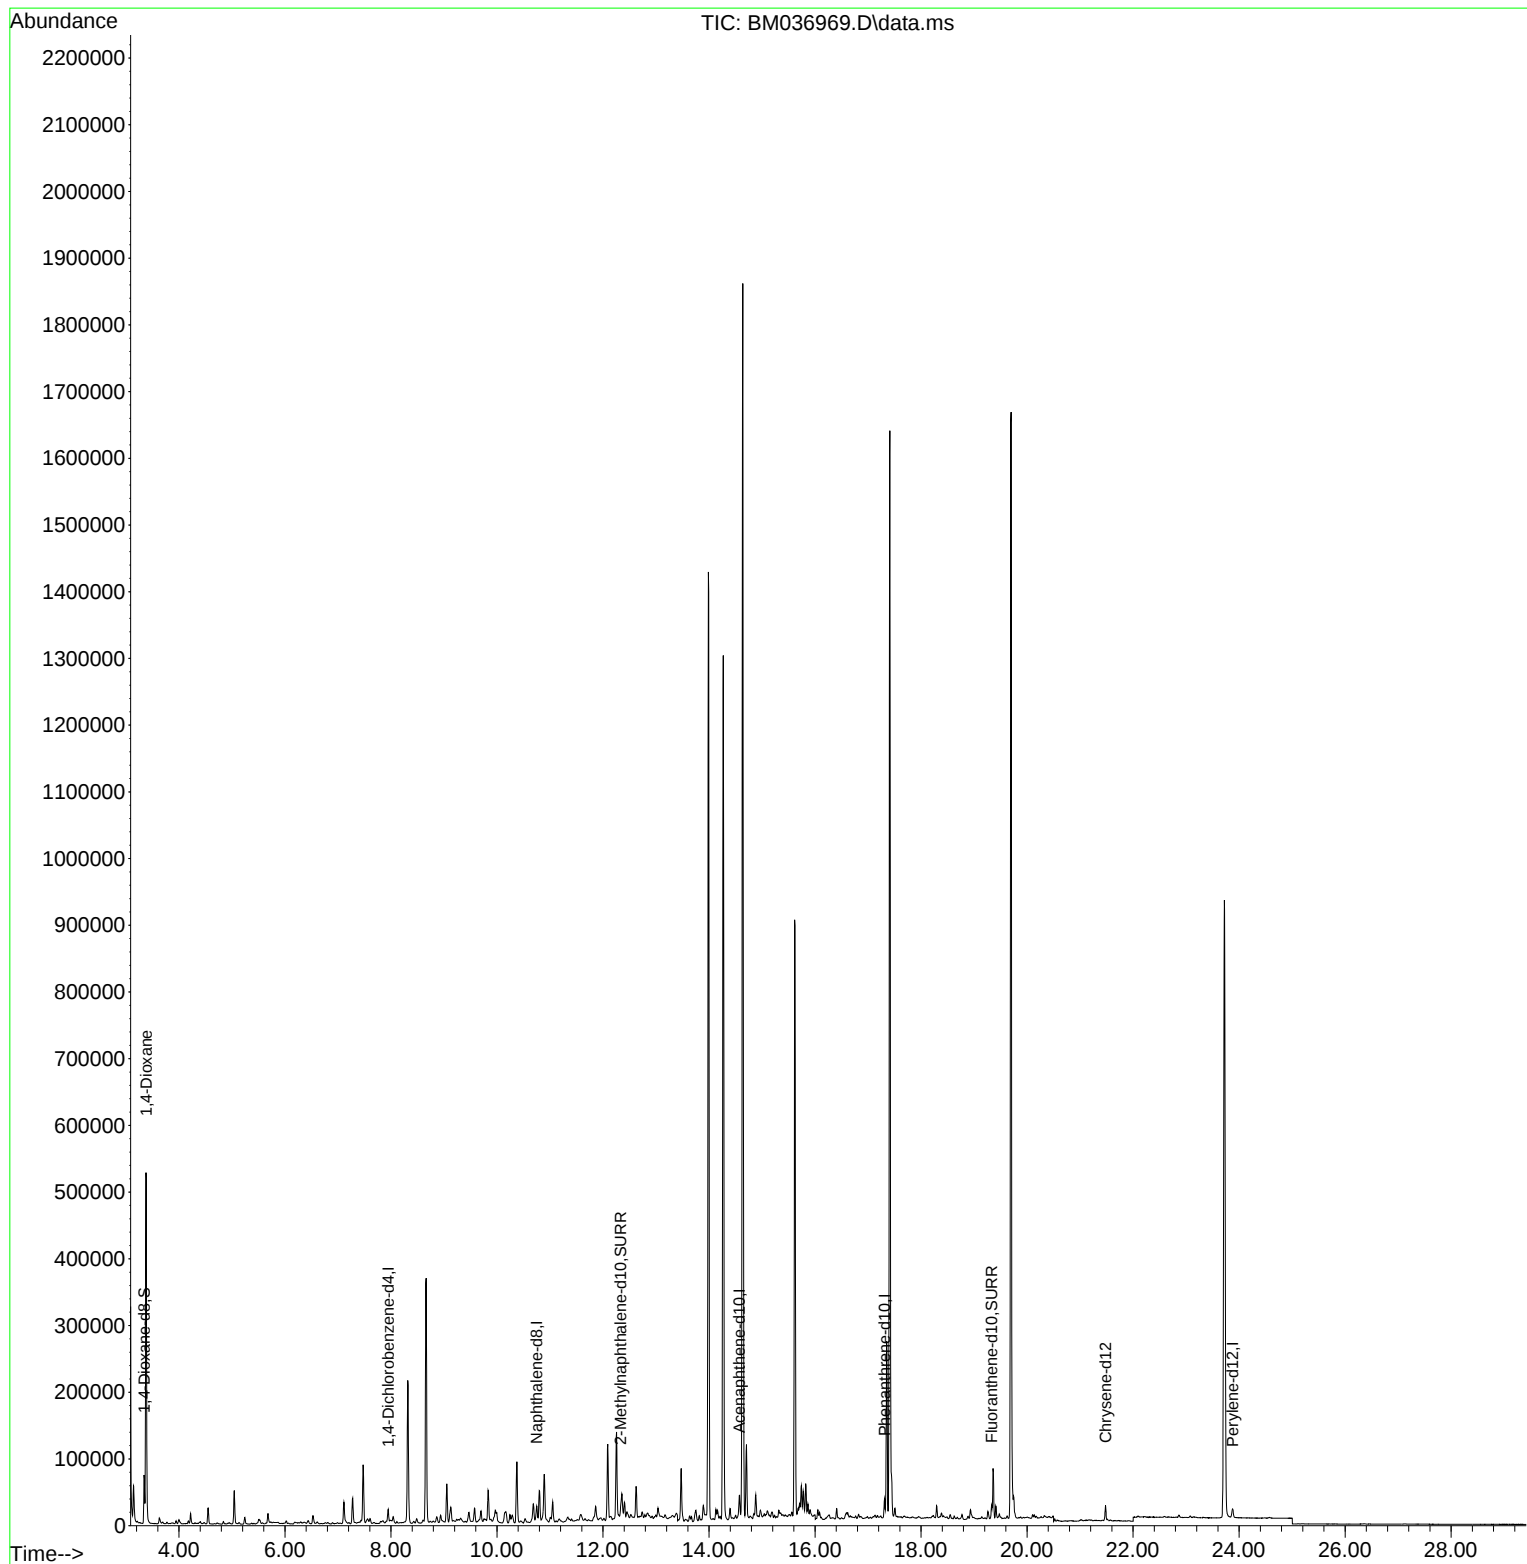

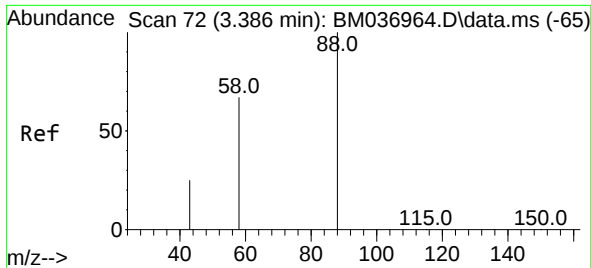

#2
 1,4-Dioxane
 Concen: 26.547 ng/ul
 RT: 3.382 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM036969.D
 Acq: 12 Oct 2022 06:08

Instrument :
 BNA_M
 ClientSampleId :
 CB8X1

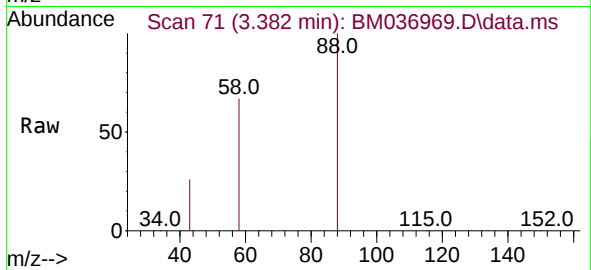

Tgt Ion: 88 Resp: 336646
 Ion Ratio Lower Upper
 88 100
 43 25.7 37.8 56.6#
 58 66.9 42.6 63.8#

