

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
 Data File : BM036984.D
 Acq On : 12 Oct 2022 15:17
 Operator : CG/JU
 Sample : N5024-10DL 5X
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BP9DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
 Supervised By :mohammad ahmed 10/14/2022

Quant Time: Oct 12 23:11:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 09:03:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.947	152	7966	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	28060	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.576	164	14655	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.314	188	25494	0.400	ng/ul	0.00
17) Chrysene-d12	21.481	240	16043	0.400	ng/ul	0.00
23) Perylene-d12	23.881	264	14230	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	7821	0.696	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.338	152	1905	0.045	ng/ul	0.00
18) Fluoranthene-d10	19.332	212	2768	0.058	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.803	128	13610	0.170	ng/ul	98
7) 2-Methylnaphthalene	12.409	142	13167	0.268	ng/ul	92
8) 1-Methylnaphthalene	12.629	142	10901	0.219	ng/ul	99
10) Acenaphthylene	14.298	152	2338	0.038	ng/ul#	74
11) Acenaphthene	14.636	153	2722	0.051	ng/ul	97
12) Fluorene	15.621	166	2953	0.049	ng/ul#	94
15) Phenanthrene	17.352	178	61431	0.755	ng/ul	99
16) Anthracene	17.445	178	7770	0.114	ng/ul	97
19) Fluoranthene	19.364	202	57686	0.904	ng/ul	97
20) Pyrene	19.727	202	49527	0.744	ng/ul	96
21) Benzo(a)anthracene	21.467	228	21657	0.374	ng/ul	97
22) Chrysene	21.519	228	23453	0.377	ng/ul	98
24) Benzo(b)fluoranthene	23.147	252	29072	0.457	ng/ul	96
25) Benzo(k)fluoranthene	23.191	252	9437m	0.152	ng/ul	
26) Benzo(a)pyrene	23.770	252	19010	0.369	ng/ul	95
27) Indeno(1,2,3-cd)pyrene	26.362	276	13901	0.190	ng/ul#	92
28) Dibenzo(a,h)anthracene	26.369	278	3529	0.060	ng/ul#	59
29) Benzo(g,h,i)perylene	27.130	276	12601	0.196	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101022\
Data File : BM036984.D
Acq On : 12 Oct 2022 15:17
Operator : CG/JU
Sample : N5024-10DL 5X
Misc :
ALS Vial : 88 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0BP9DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022


Quant Time: Oct 12 23:11:00 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 09:03:52 2022
Response via : Initial Calibration

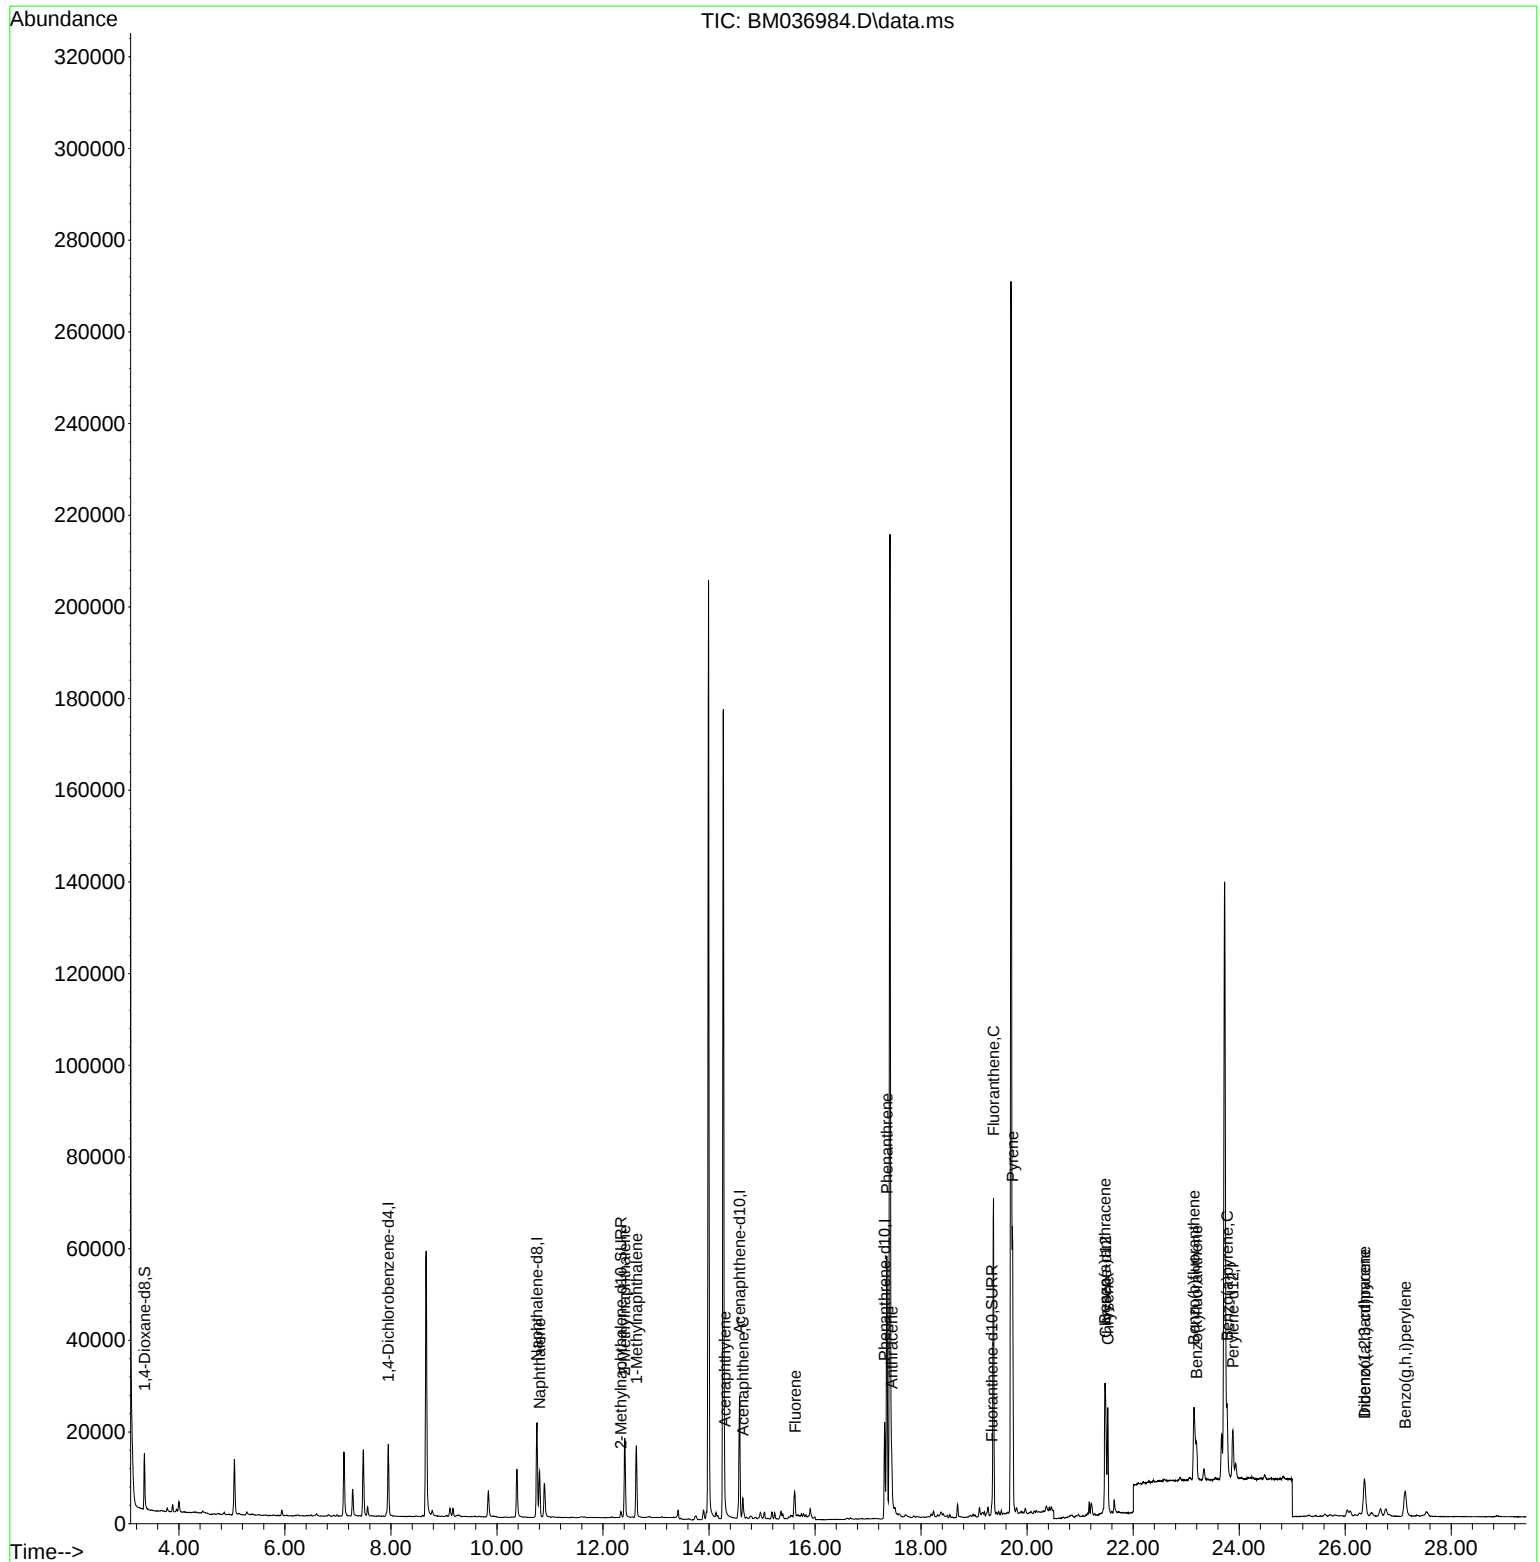



#5
Naphthalene
Concen: 0.170 ng/ul
RT: 10.803 min Scan# 1789
Delta R.T. 0.000 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL



Tgt Ion:128 Resp: 13610
Ion Ratio Lower Upper
128 100
129 12.2 10.2 15.2
127 13.4 11.7 17.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

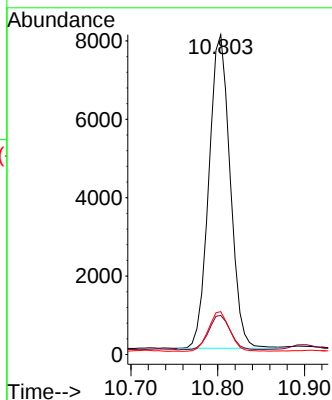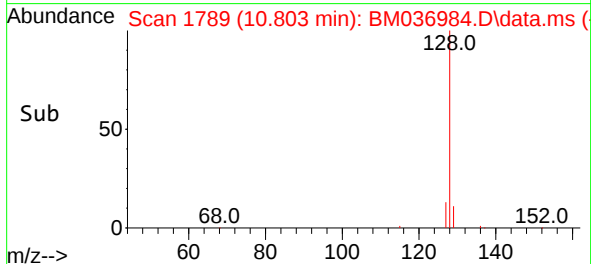

#7
2-Methylnaphthalene
Concen: 0.268 ng/ul
RT: 12.409 min Scan# 2081
Delta R.T. -0.005 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17


Tgt Ion:142 Resp: 13167
Ion Ratio Lower Upper
142 100
141 88.5 77.4 116.0

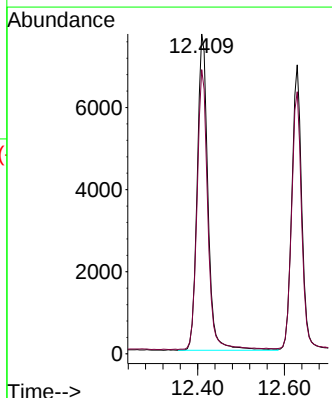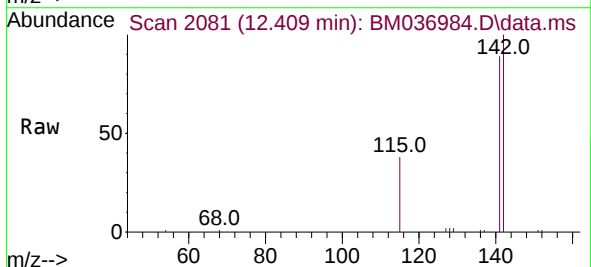



#8
1-Methylnaphthalene
Concen: 0.219 ng/ul
RT: 12.629 min Scan# 2120
Delta R.T. 0.000 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL



Tgt Ion:142 Resp: 10901
Ion Ratio Lower Upper
142 100
141 91.6 74.1 111.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

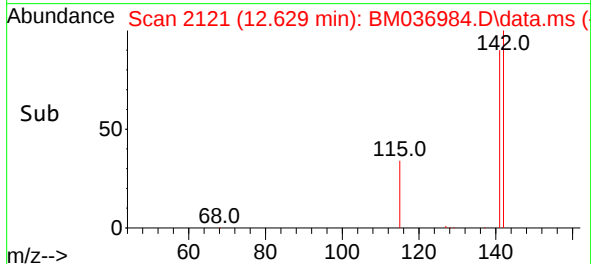

#10
Acenaphthylene
Concen: 0.038 ng/ul
RT: 14.298 min Scan# 2455
Delta R.T. 0.001 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17


Tgt Ion:152 Resp: 2338
Ion Ratio Lower Upper
152 100
151 27.8 16.6 24.8#
153 31.4 11.4 17.0#

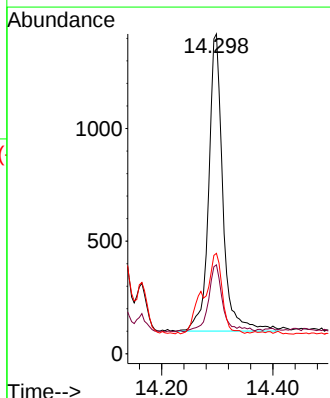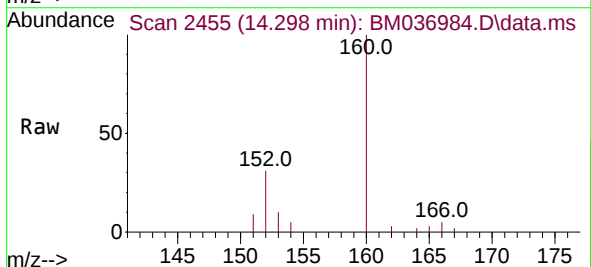

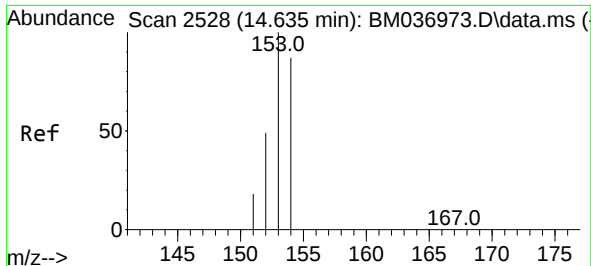

#11
Acenaphthene
Concen: 0.051 ng/u1
RT: 14.636 min Scan# 2528
Delta R.T. -0.004 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL



Tgt Ion:153 Resp: 2722
Ion Ratio Lower Upper
153 100
152 53.3 40.2 60.4
154 84.5 69.7 104.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

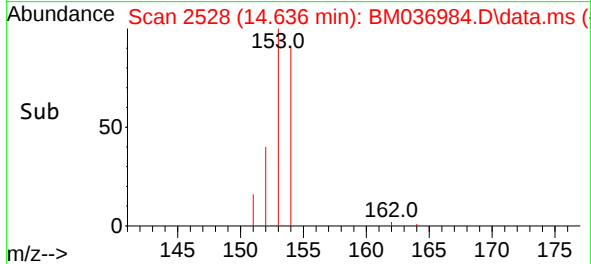

#12
Fluorene
Concen: 0.049 ng/u1
RT: 15.621 min Scan# 2741
Delta R.T. 0.001 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17


Tgt Ion:166 Resp: 2953
Ion Ratio Lower Upper
166 100
165 102.9 78.9 118.3
167 21.7 11.3 16.9#

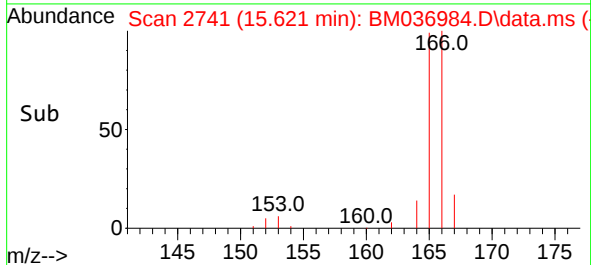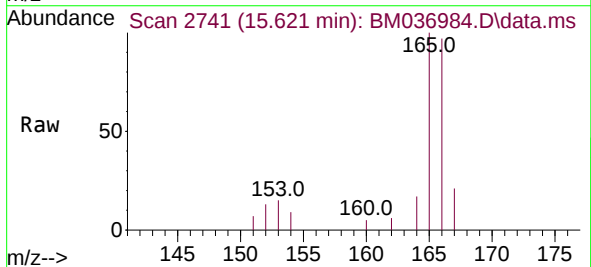

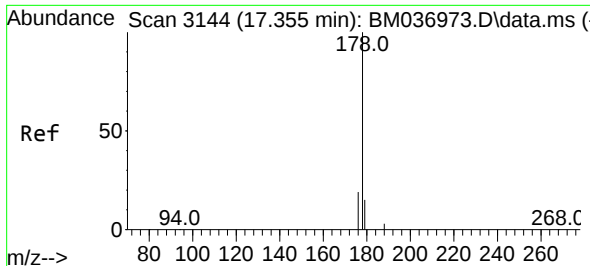

#15
Phenanthrene
Concen: 0.755 ng/ul
RT: 17.352 min Scan# 3143
Delta R.T. -0.003 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL

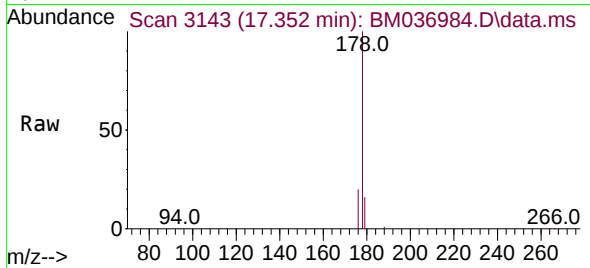

Tgt Ion:178 Resp: 6143
Ion Ratio Lower Upper
178 100
179 15.7 13.0 19.6
176 19.7 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

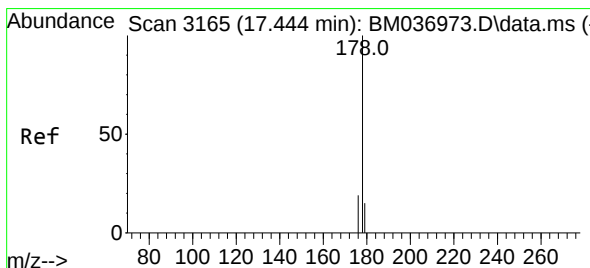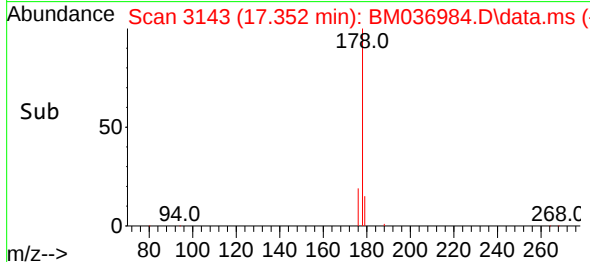

#16
Anthracene
Concen: 0.114 ng/ul
RT: 17.445 min Scan# 3165
Delta R.T. -0.003 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17


Tgt Ion:178 Resp: 7770
Ion Ratio Lower Upper
178 100
179 19.1 13.6 20.4
176 19.8 15.6 23.4

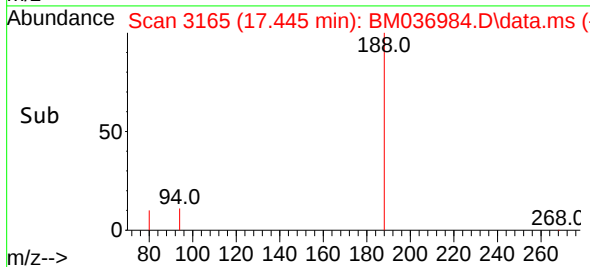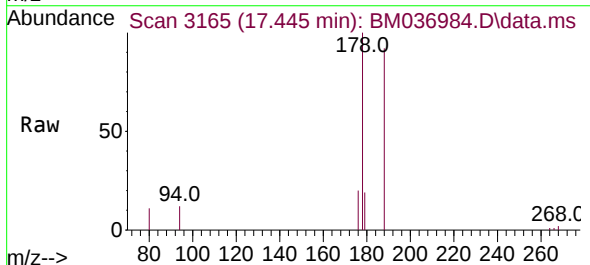

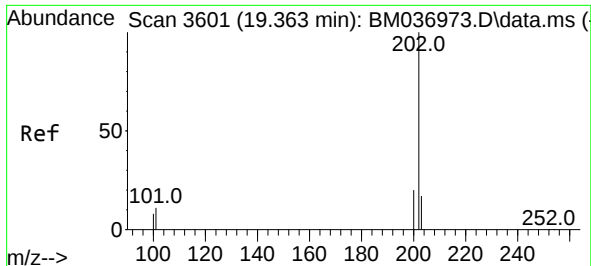

#19
Fluoranthene
Concen: 0.904 ng/u1
RT: 19.364 min Scan# 3601
Delta R.T. 0.001 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL



Tgt Ion:202 Resp: 57686
Ion Ratio Lower Upper
202 100
101 11.8 10.1 15.1
100 8.6 7.9 11.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

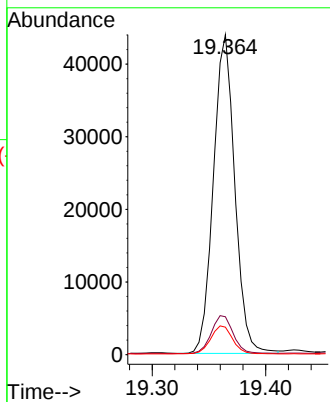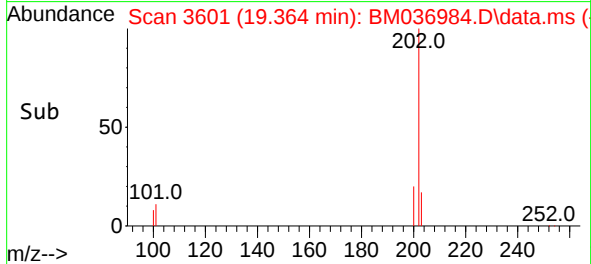

#20
Pyrene
Concen: 0.744 ng/u1
RT: 19.727 min Scan# 3679
Delta R.T. 0.001 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17


Tgt Ion:202 Resp: 49527
Ion Ratio Lower Upper
202 100
101 13.2 12.0 18.0
100 10.5 9.8 14.6

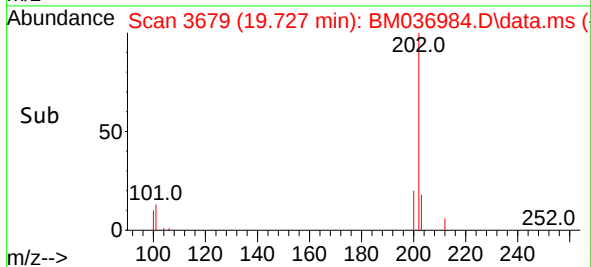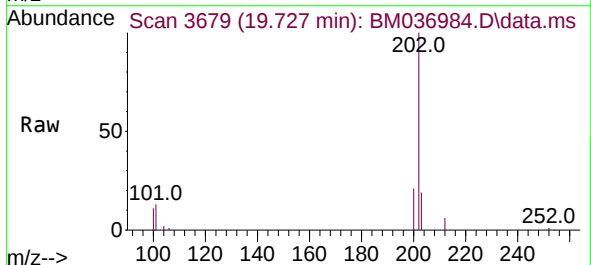

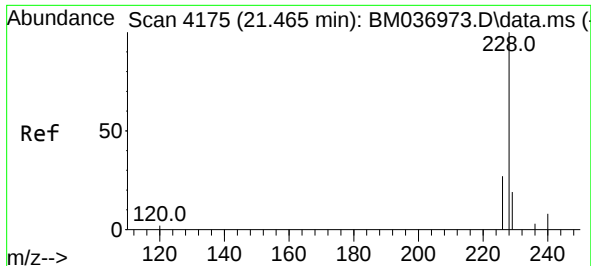

#21
Benzo(a)anthracene
Concen: 0.374 ng/ul
RT: 21.467 min Scan# 4175
Delta R.T. -0.001 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL



Tgt Ion:228 Resp: 21652
Ion Ratio Lower Upper
228 100
229 22.7 16.2 24.2
226 28.5 22.5 33.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

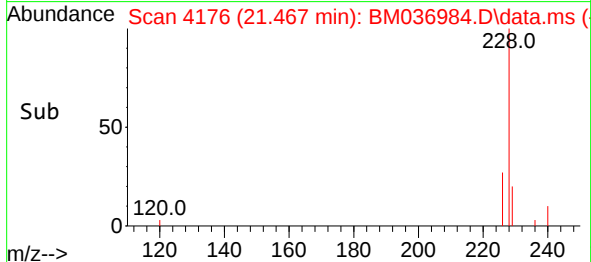

#22
Chrysene
Concen: 0.377 ng/ul
RT: 21.519 min Scan# 4194
Delta R.T. -0.001 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17


Tgt Ion:228 Resp: 23453
Ion Ratio Lower Upper
228 100
226 30.9 24.6 37.0
229 23.2 16.4 24.6

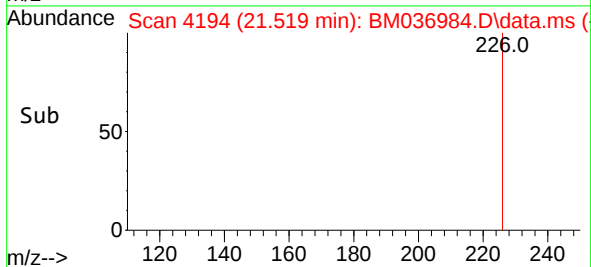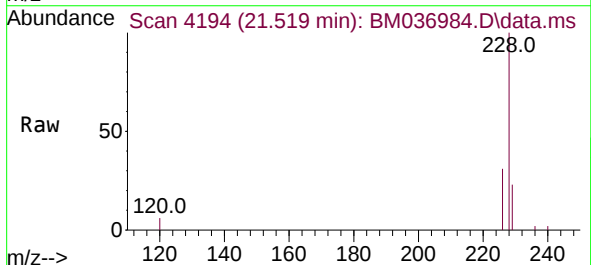

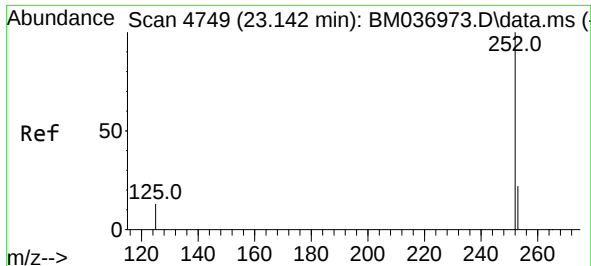

#24
Benzo(b)fluoranthene
Concen: 0.457 ng/ul
RT: 23.147 min Scan# 4751
Delta R.T. 0.002 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL



Tgt Ion:252 Resp: 29072
Ion Ratio Lower Upper
252 100
253 30.0 0.0 61.4
125 25.5 0.0 42.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

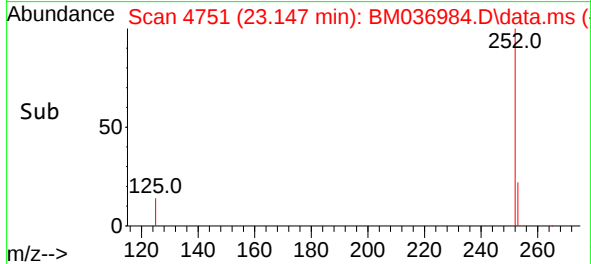

#25
Benzo(k)fluoranthene
Concen: 0.152 ng/ul m
RT: 23.191 min Scan# 4766
Delta R.T. -0.004 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17


Tgt Ion:252 Resp: 9437
Ion Ratio Lower Upper
252 100
253 36.1 25.2 37.8
125 33.5 18.3 27.5#

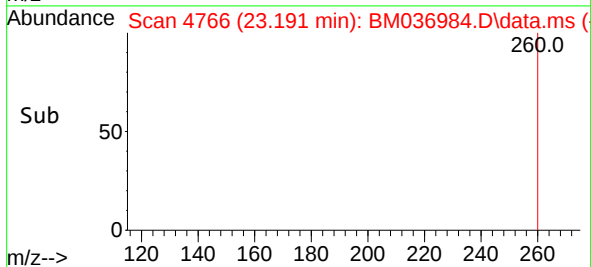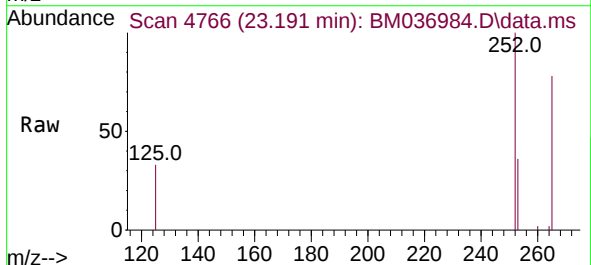

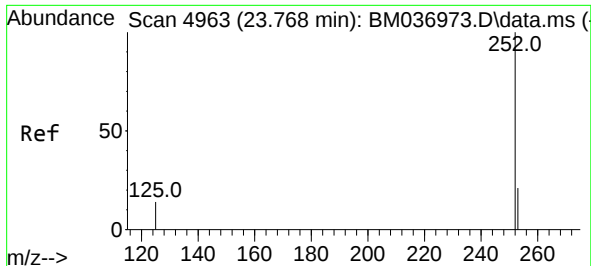

#26
Benzo(a)pyrene
Concen: 0.369 ng/ul
RT: 23.770 min Scan# 4963
Delta R.T. -0.001 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL



Tgt Ion:252 Resp: 19010
Ion Ratio Lower Upper
252 100
253 31.5 29.7 44.5
125 29.5 23.6 35.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

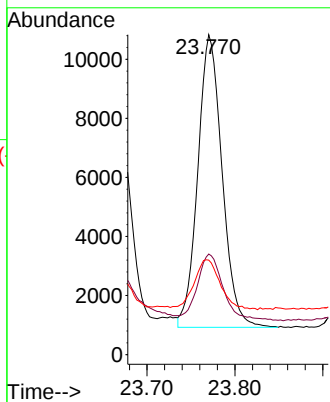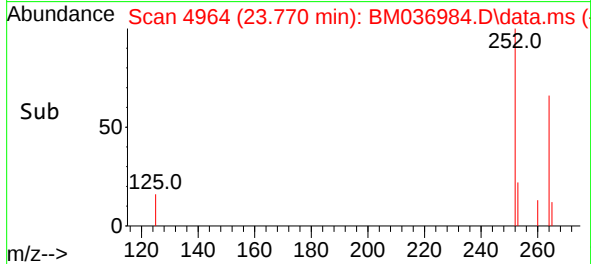

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.190 ng/ul
RT: 26.362 min Scan# 5791
Delta R.T. -0.001 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17


Tgt Ion:276 Resp: 13901
Ion Ratio Lower Upper
276 100
138 25.6 23.9 35.9
227 0.1 0.1 0.1#

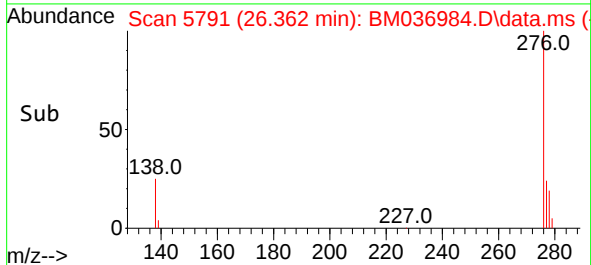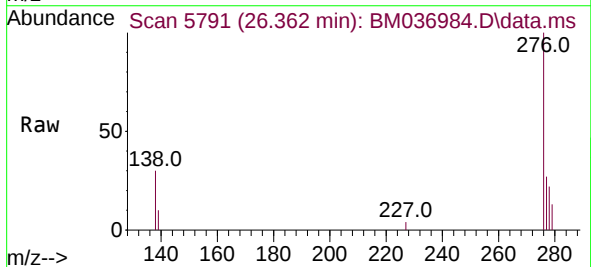

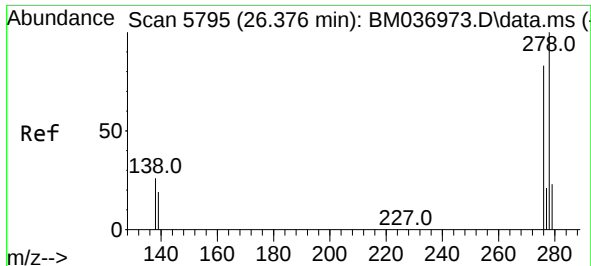

#28
Dibenzo(a,h)anthracene
Concen: 0.060 ng/ul
RT: 26.369 min Scan# 5795
Delta R.T. -0.011 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17




Instrument :
BNA_M
ClientSampleId :
C0BP9DL




Tgt Ion:278 Resp: 3529
Ion Ratio Lower Upper
278 100
139 43.6 19.8 29.6
279 59.8 27.7 41.5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 10/13/2022
Supervised By :mohammad ahmed 10/14/2022

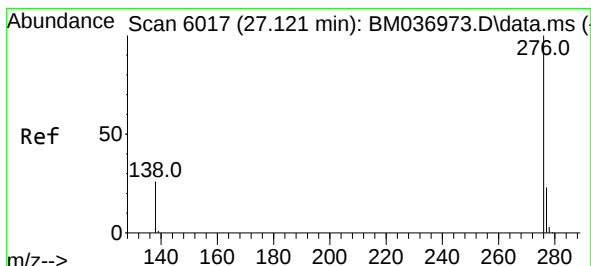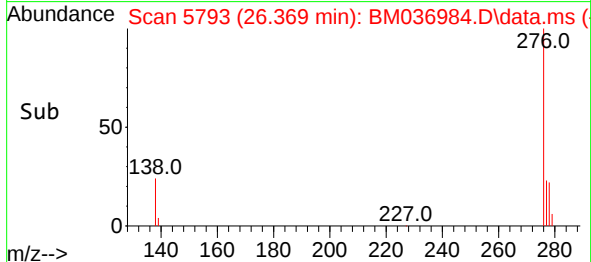

#29
Benzo(g,h,i)perylene
Concen: 0.196 ng/ul
RT: 27.130 min Scan# 6020
Delta R.T. 0.003 min
Lab File: BM036984.D
Acq: 12 Oct 2022 15:17

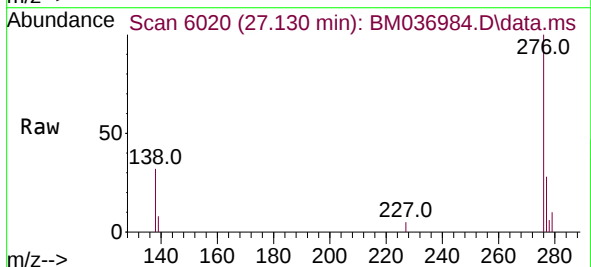

Tgt Ion:276 Resp: 12601
Ion Ratio Lower Upper
276 100
138 31.7 23.4 35.0
277 27.5 21.0 31.4

